

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100520\
 Data File : FB025015.D
 Signal(s) : FID2B.CH
 Acq On : 5 Oct 2020 10:52
 Operator : DD/AJ
 Sample : BSF1005S1
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 06 01:29:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	402219	19.159 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	853905	28.394 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	913238	29.880 ng/ml
3) t n-Heptane	7.758	301878	9.923 ng/ml
4) t Benzene	7.893	361116	9.694 ng/ml
6) t Toluene	10.630	1010943	28.959 ng/ml
7) t Ethylbenzene	13.070	307247	9.478 ng/ml
8) t m-Xylene	13.203	613325	19.308 ng/ml
9) t O-Xylene	13.930	588857	19.378 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	495596	19.540 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100520\
Data File : FB025015.D
Signal(s) : FID2B.CH
Acq On : 5 Oct 2020 10:52
Operator : DD/AJ
Sample : BSF1005S1
Misc : 5.01/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 06 01:29:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

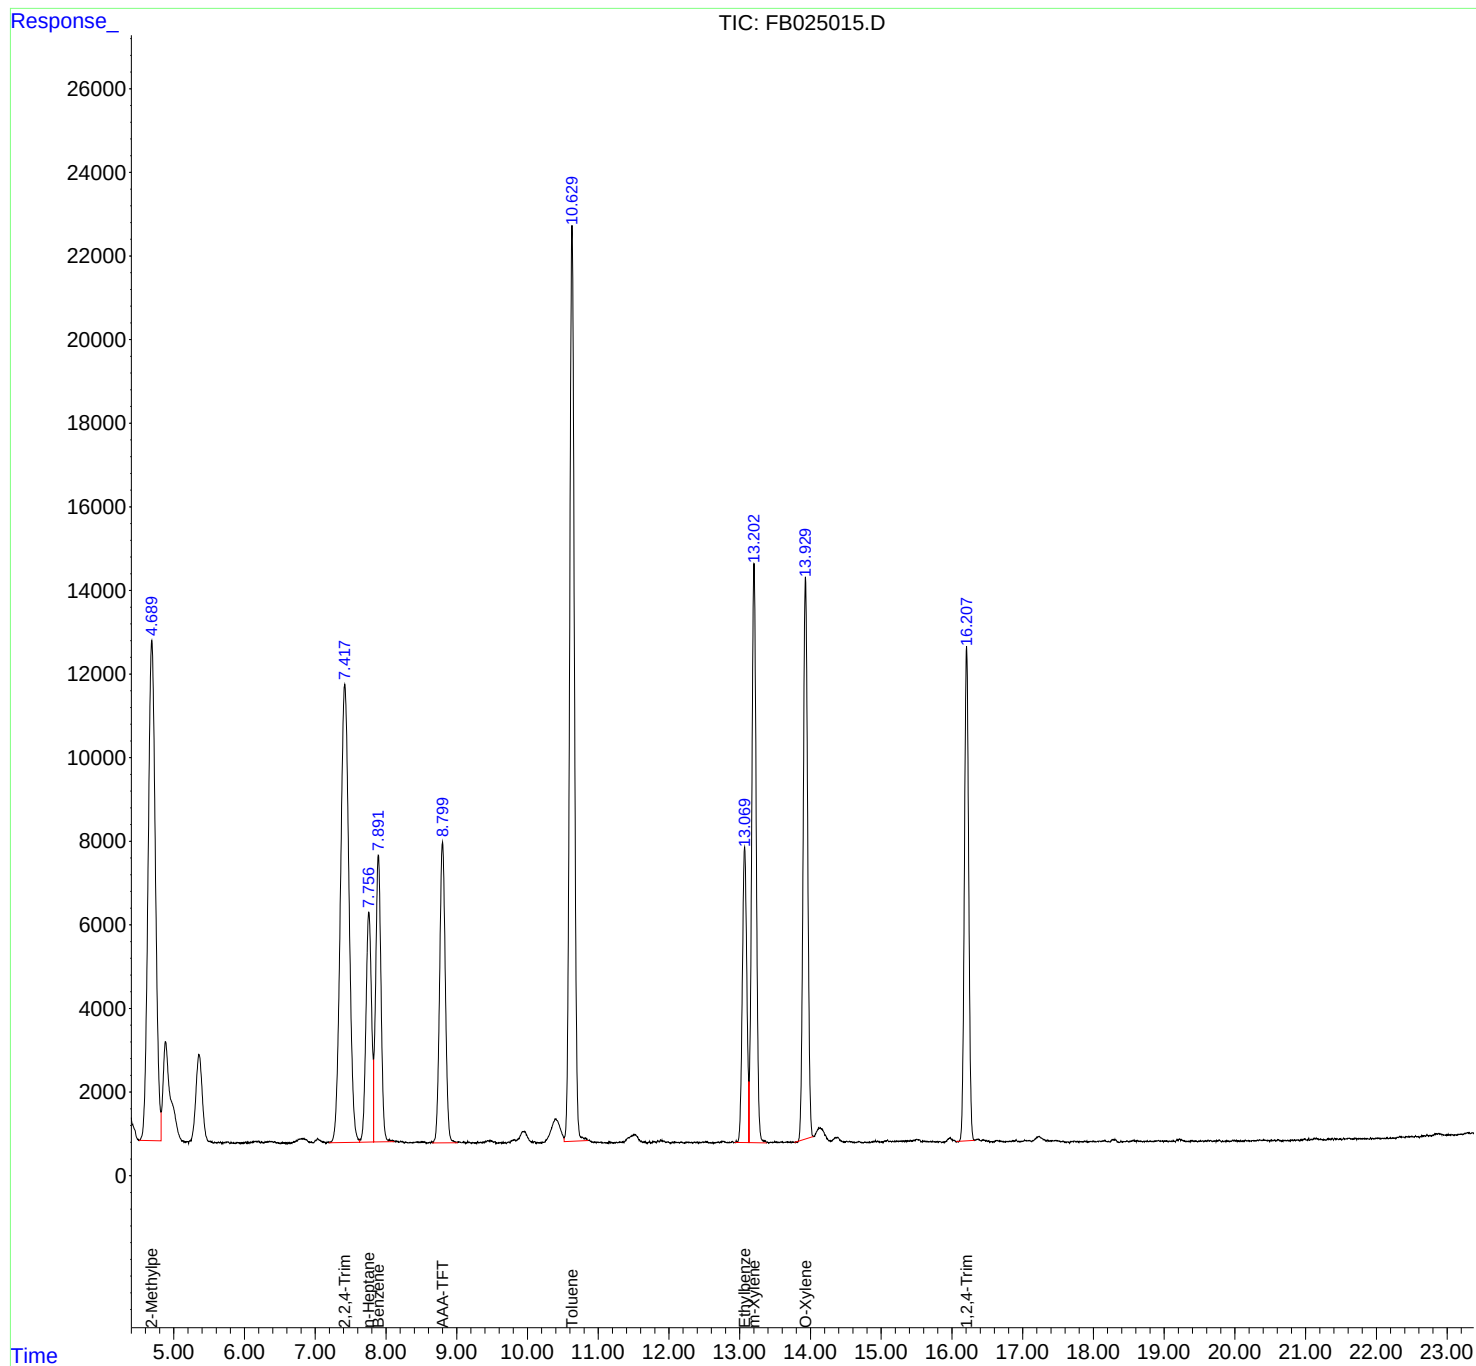

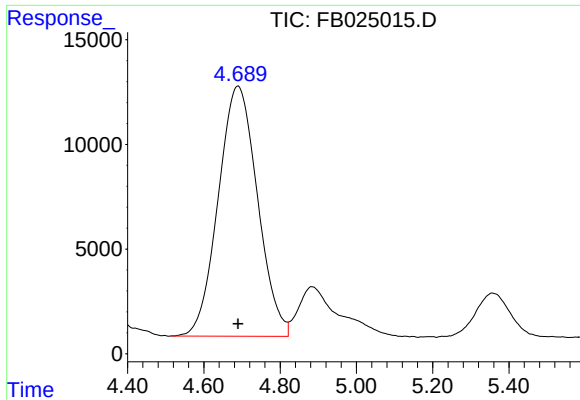


#1 2-Methylpentane

R.T.: 4.691 min
Delta R.T.: 0.000 min
Response: 853905
Conc: 28.39 ng/ml

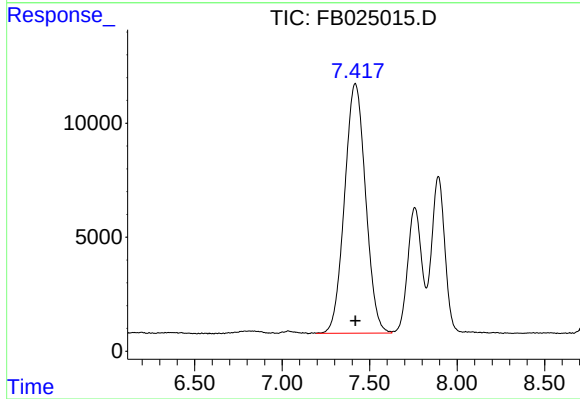


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 913238
Conc: 29.88 ng/ml

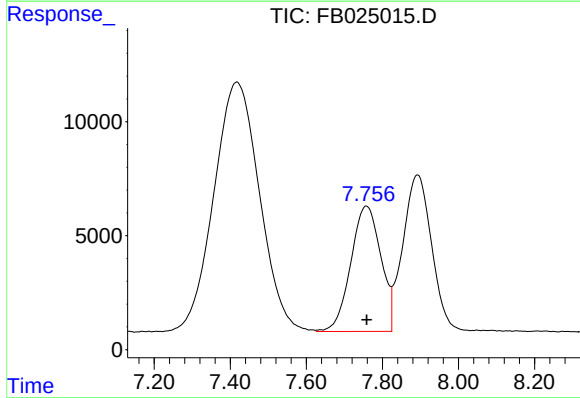


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: -0.001 min
Response: 301878
Conc: 9.92 ng/ml

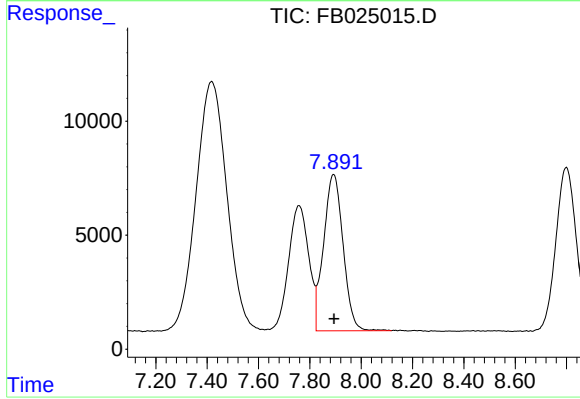


#4 Benzene

R.T.: 7.893 min
Delta R.T.: -0.002 min
Response: 361116
Conc: 9.69 ng/ml

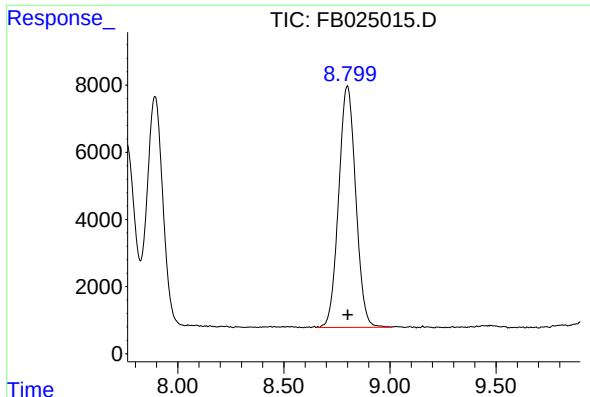


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 402219
Conc: 19.16 ng/ml

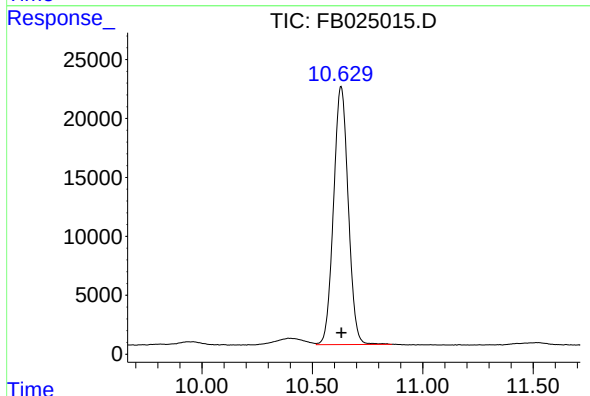


#6 Toluene

R.T.: 10.630 min
Delta R.T.: -0.001 min
Response: 1010943
Conc: 28.96 ng/ml

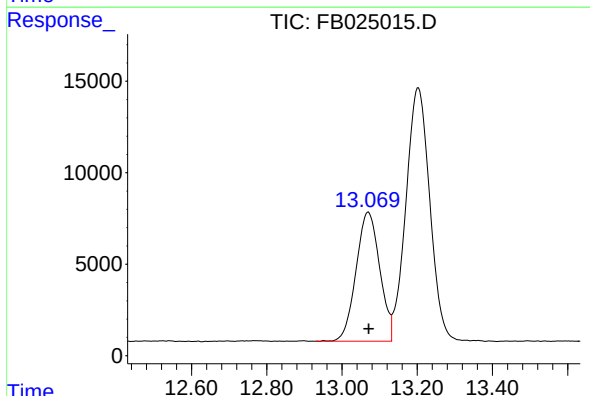


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: -0.001 min
Response: 307247
Conc: 9.48 ng/ml

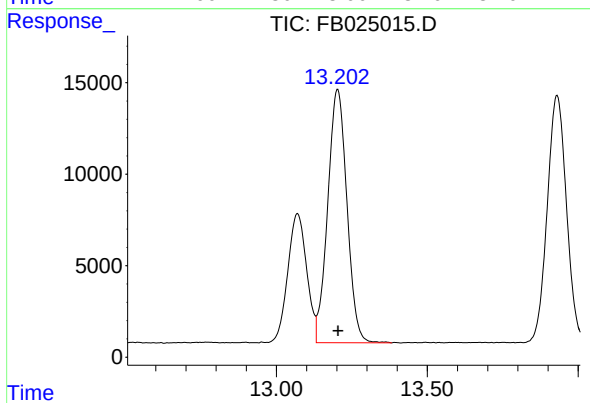

#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: -0.001 min
Response: 613325
Conc: 19.31 ng/ml

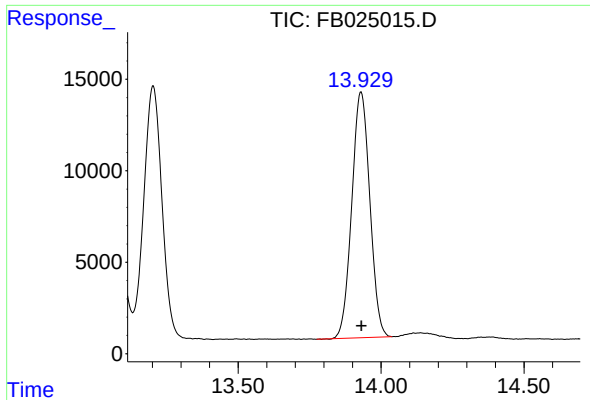


#9 O-Xylene

R.T.: 13.930 min

Delta R.T.: -0.002 min

Response: 588857

Conc: 19.38 ng/ml

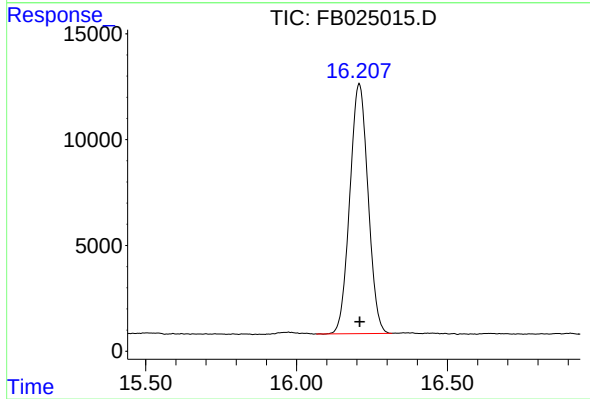

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min

Delta R.T.: -0.002 min

Response: 495596

Conc: 19.54 ng/ml