

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100520\
 Data File : FB025020.D
 Signal(s) : FID2B.CH
 Acq On : 5 Oct 2020 14:15
 Operator : DD/AJ
 Sample : L4260-03MS
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 06 01:30:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	425775	20.281 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	734442	24.422 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	659334	21.572 ng/ml
3) t n-Heptane	7.759	217886	7.162 ng/ml
4) t Benzene	7.893	345497	9.275 ng/ml
6) t Toluene	10.631	943589	27.030 ng/ml
7) t Ethylbenzene	13.071	276104	8.518 ng/ml
8) t m-Xylene	13.204	551920	17.374 ng/ml
9) t O-Xylene	13.932	540628	17.791 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	424449	16.735 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100520\
Data File : FB025020.D
Signal(s) : FID2B.CH
Acq On : 5 Oct 2020 14:15
Operator : DD/AJ
Sample : L4260-03MS
Misc : 5.01/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 06 01:30:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

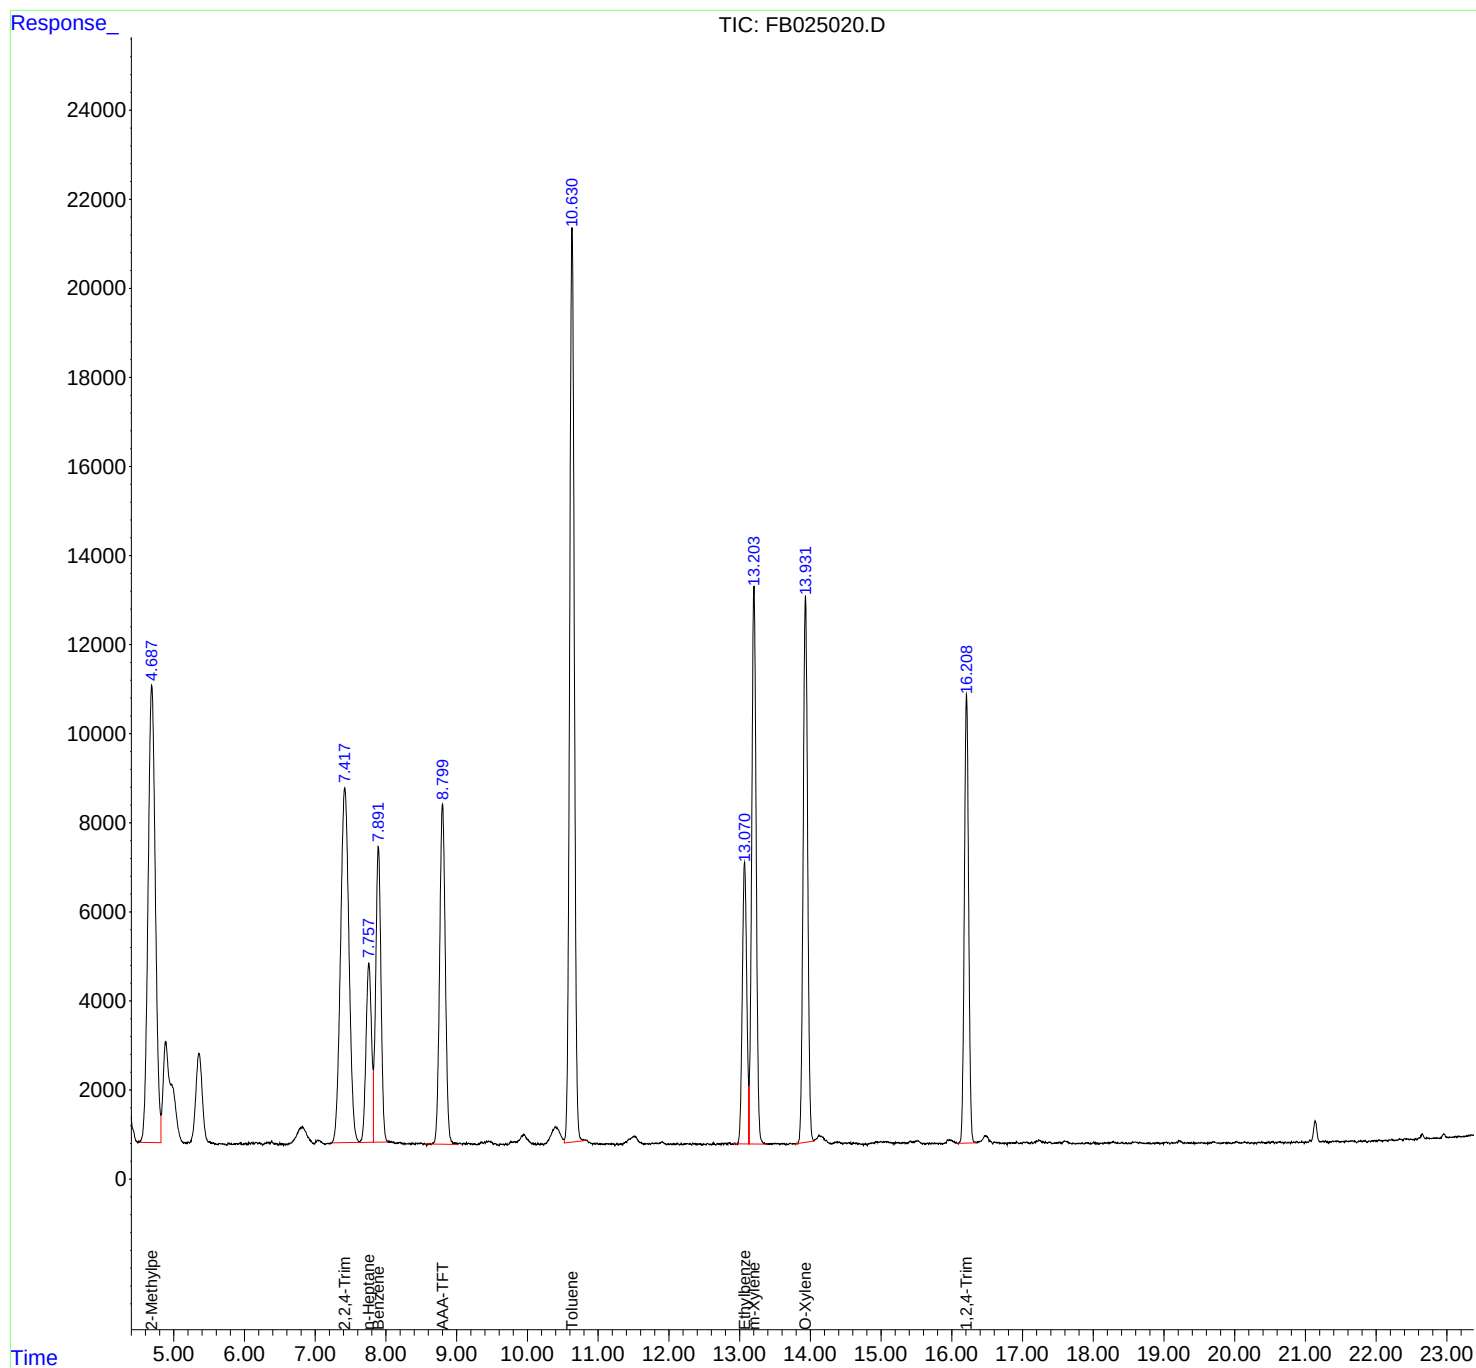

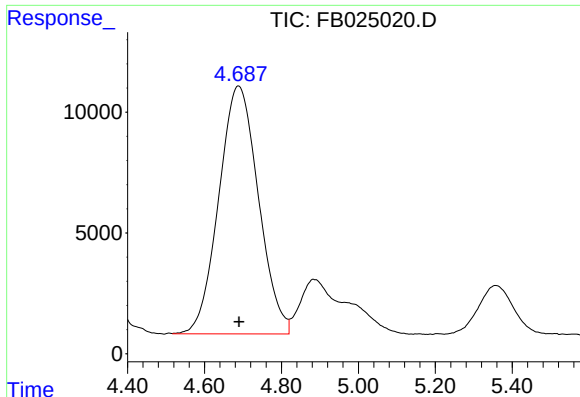


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: -0.001 min
Response: 734442
Conc: 24.42 ng/ml

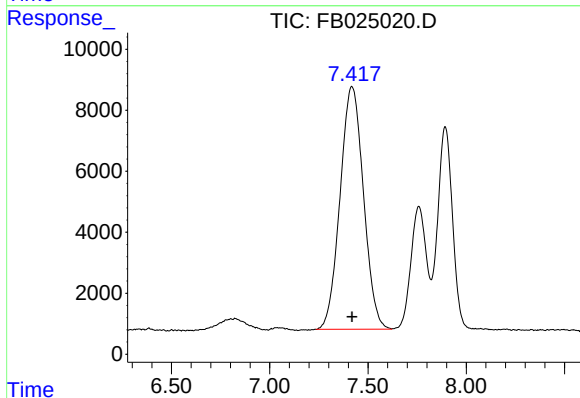


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 659334
Conc: 21.57 ng/ml

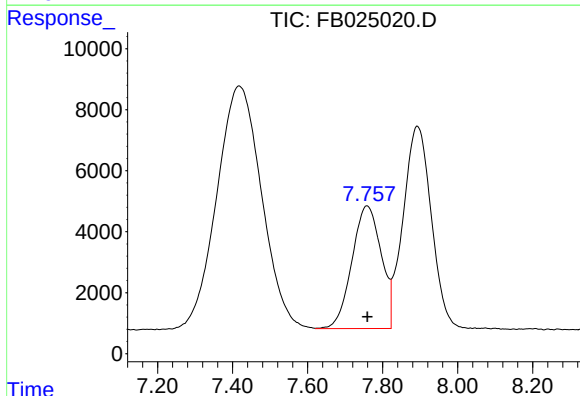


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 217886
Conc: 7.16 ng/ml

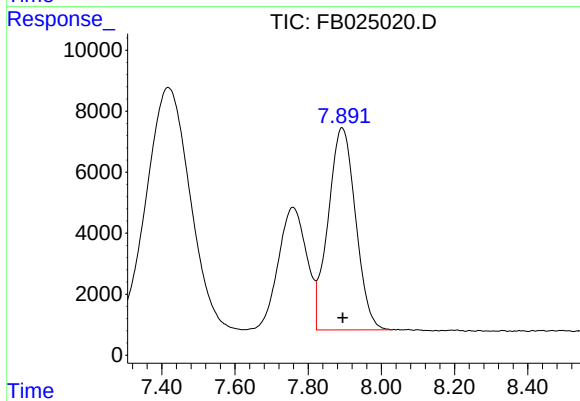


#4 Benzene

R.T.: 7.893 min
Delta R.T.: -0.002 min
Response: 345497
Conc: 9.27 ng/ml

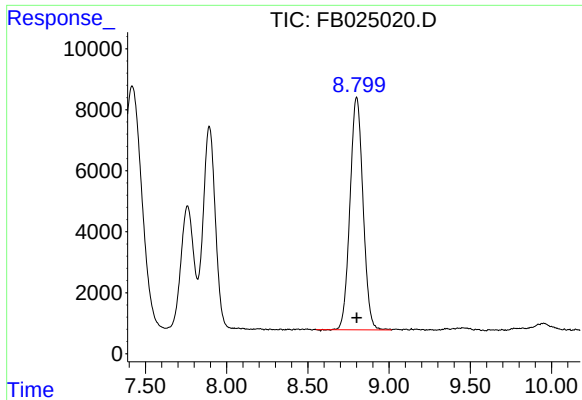


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 425775
Conc: 20.28 ng/ml

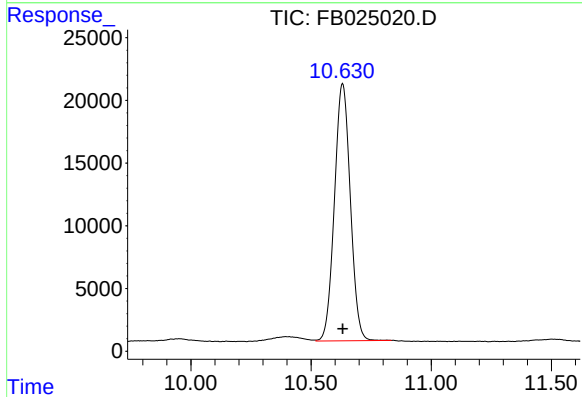


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 943589
Conc: 27.03 ng/ml

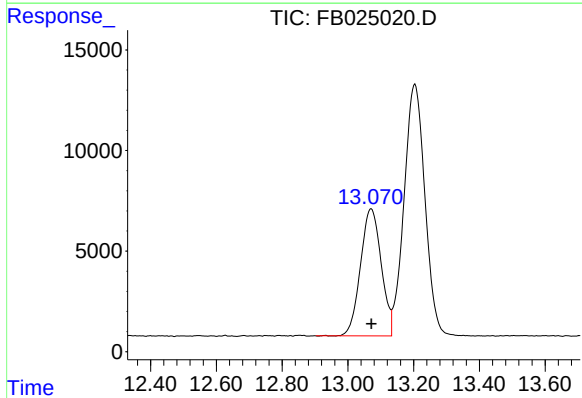


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 276104
Conc: 8.52 ng/ml

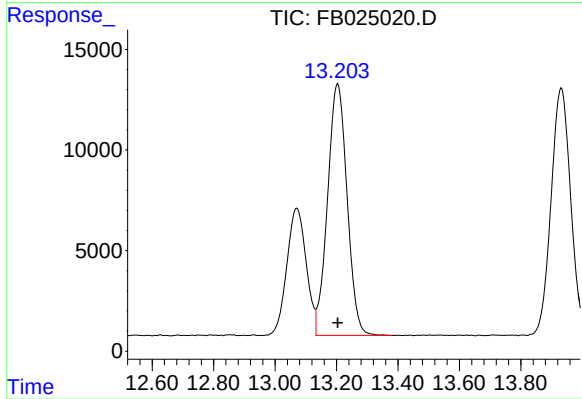

#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 551920
Conc: 17.37 ng/ml

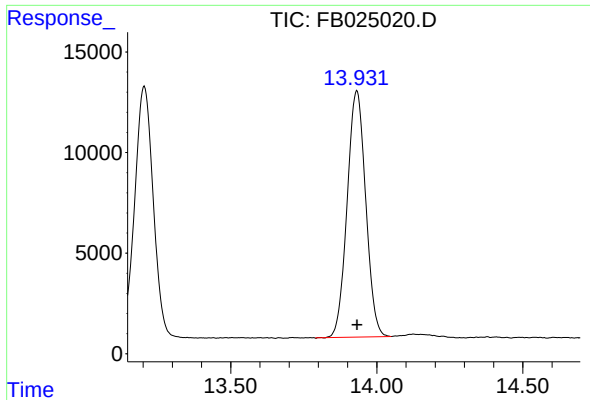


#9 O-Xylene

R.T.: 13.932 min

Delta R.T.: 0.000 min

Response: 540628

Conc: 17.79 ng/ml

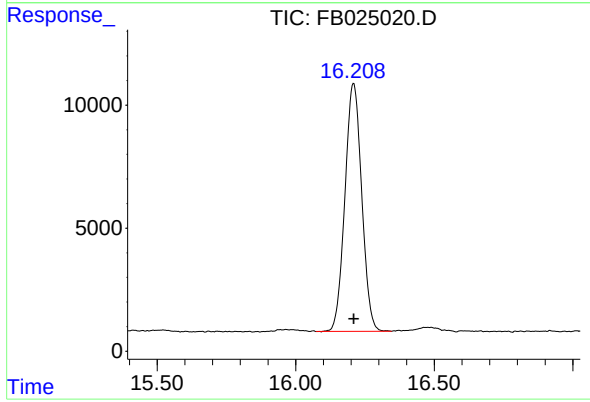

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min

Delta R.T.: 0.000 min

Response: 424449

Conc: 16.74 ng/ml