

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100520\
 Data File : FB025021.D
 Signal(s) : FID2B.CH
 Acq On : 5 Oct 2020 14:46
 Operator : DD/AJ
 Sample : L4260-03MSD
 Misc : 5.03/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 06 01:30:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.801	434970	20.719 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.689	742683	24.696 ng/ml
2) t	2,2,4-Trimethylpentane	7.419	680112	22.252 ng/ml
3) t	n-Heptane	7.759	225421	7.410 ng/ml
4) t	Benzene	7.894	356849	9.579 ng/ml
6) t	Toluene	10.632	956344	27.395 ng/ml
7) t	Ethylbenzene	13.071	286501	8.838 ng/ml
8) t	m-Xylene	13.204	568391	17.893 ng/ml
9) t	O-Xylene	13.932	553253	18.207 ng/ml
10) t	1,2,4-Trimethylbenzene	16.209	440605	17.372 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100520\
Data File : FB025021.D
Signal(s) : FID2B.CH
Acq On : 5 Oct 2020 14:46
Operator : DD/AJ
Sample : L4260-03MSD
Misc : 5.03/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 06 01:30:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

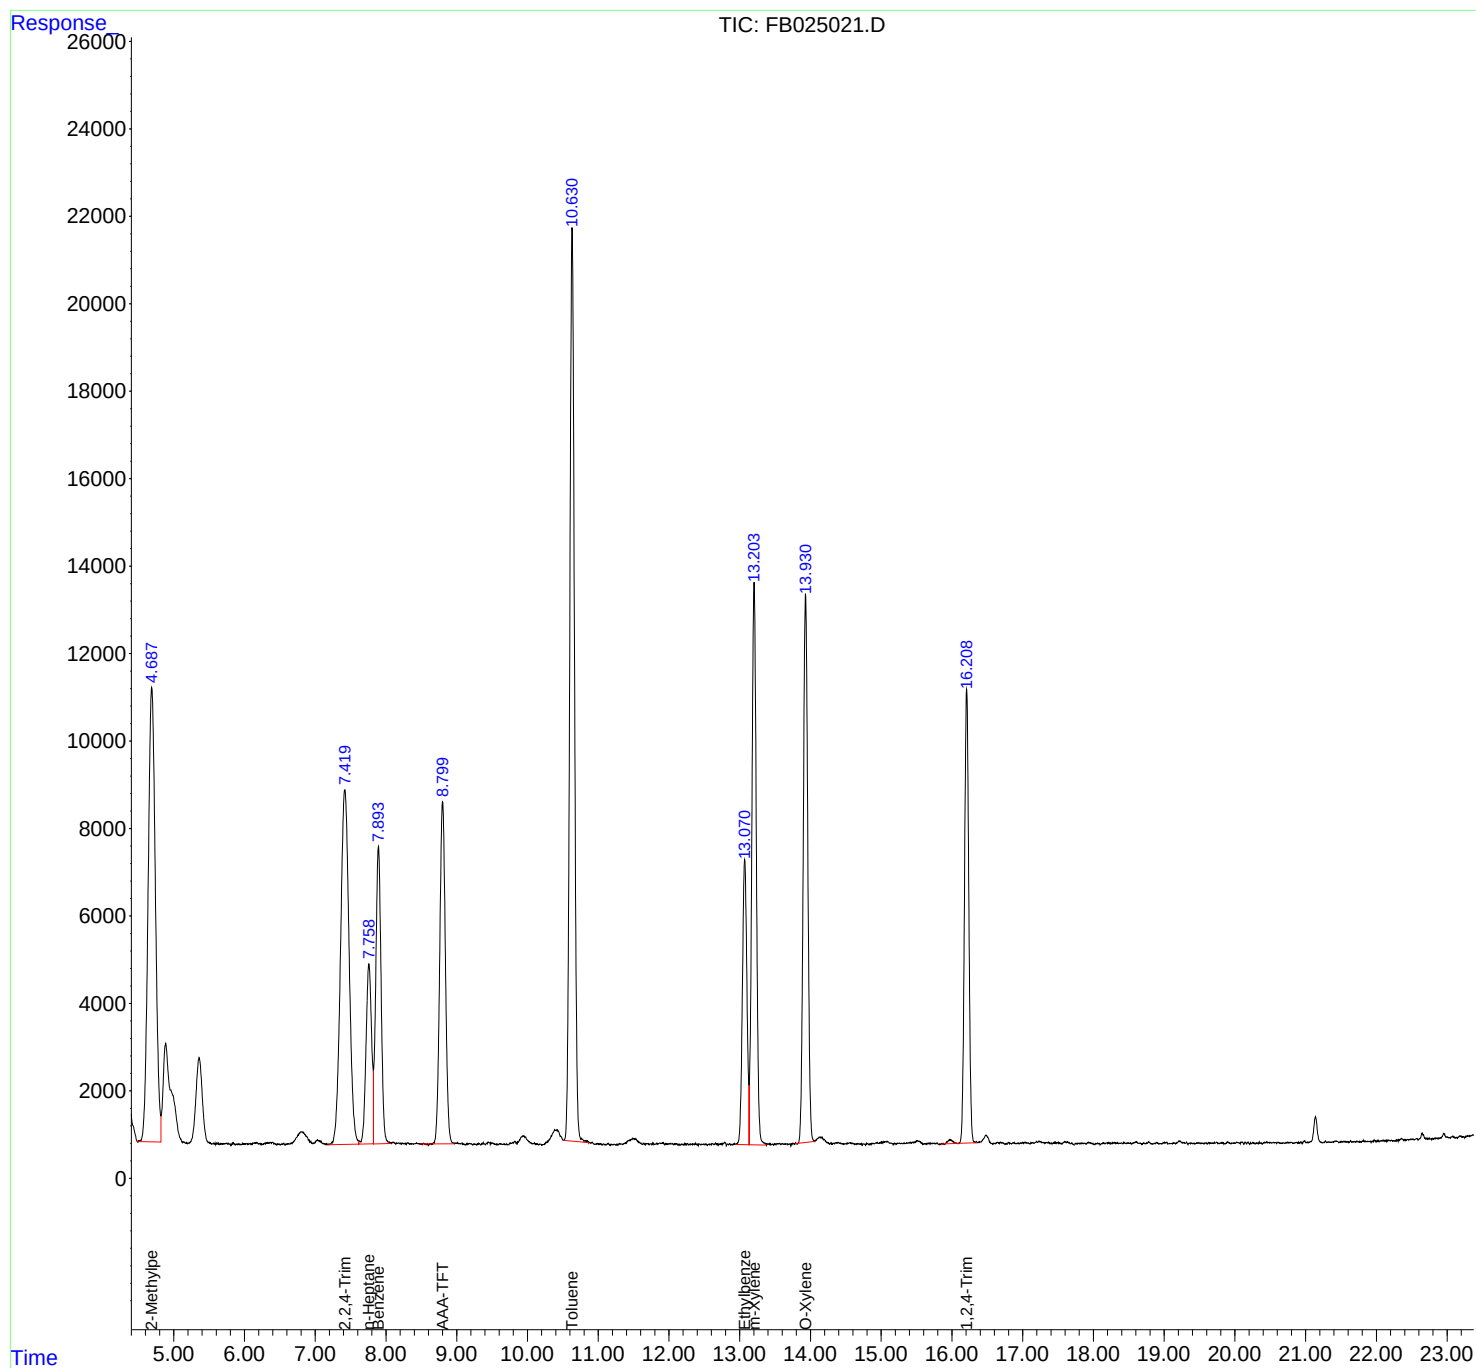

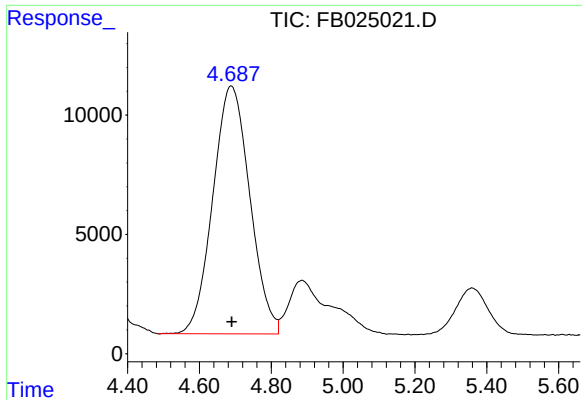


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: -0.001 min
Response: 742683
Conc: 24.70 ng/ml

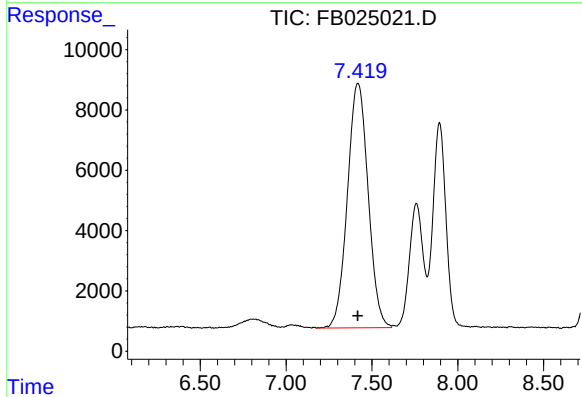


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 680112
Conc: 22.25 ng/ml

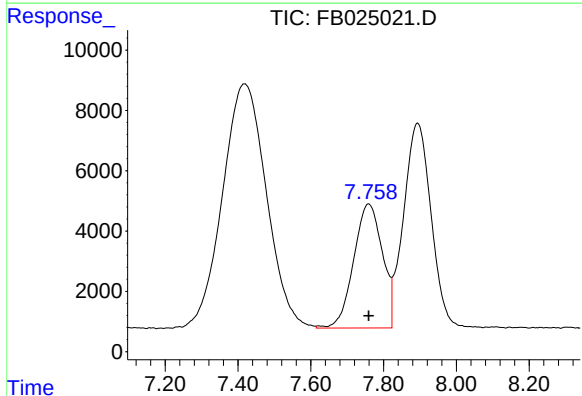


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 225421
Conc: 7.41 ng/ml

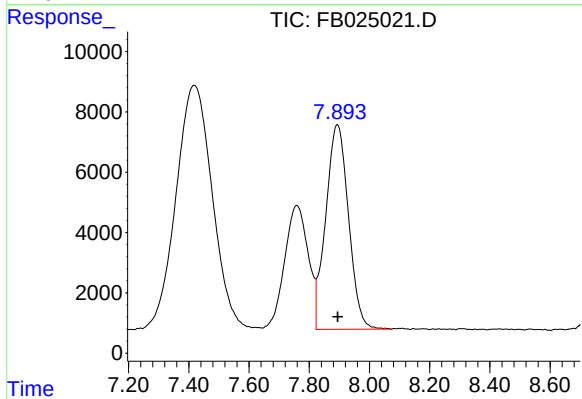


#4 Benzene

R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 356849
Conc: 9.58 ng/ml

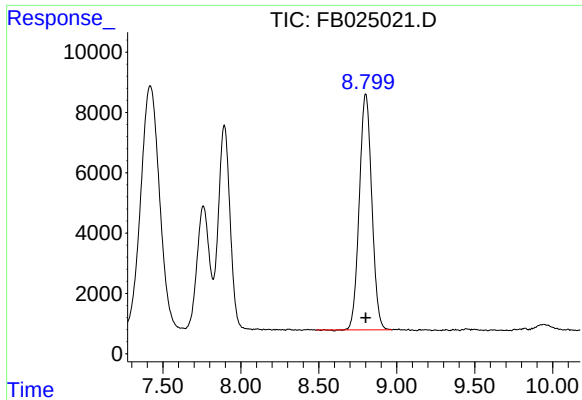


#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.000 min
Response: 434970
Conc: 20.72 ng/ml

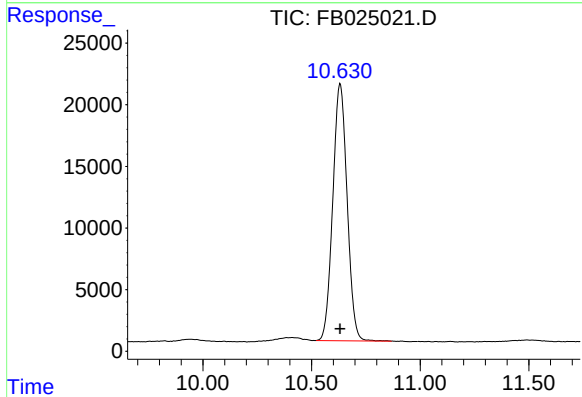


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 956344
Conc: 27.39 ng/ml

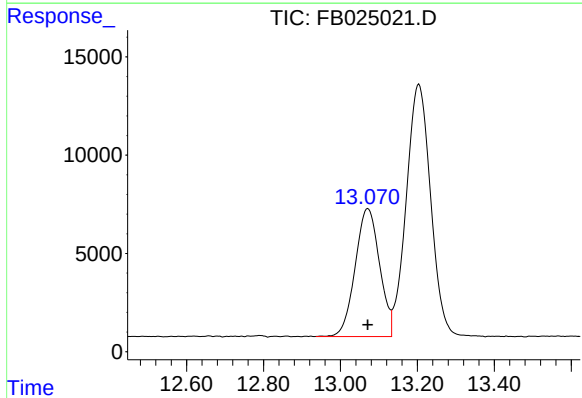


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 286501
Conc: 8.84 ng/ml

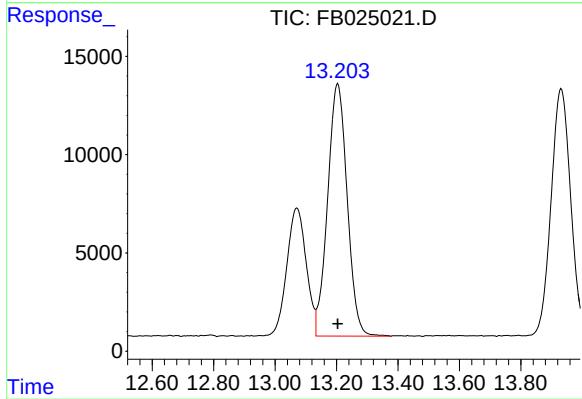


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 568391
Conc: 17.89 ng/ml

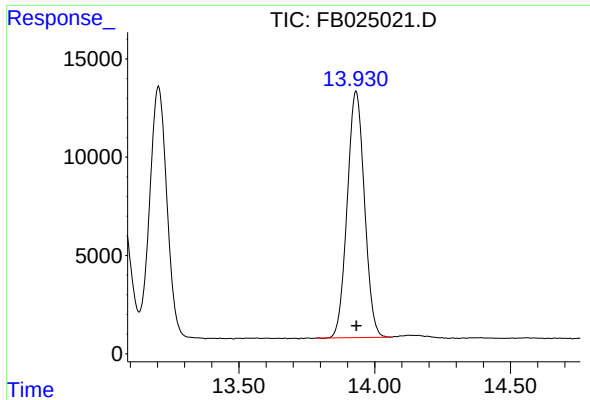

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 553253
Conc: 18.21 ng/ml

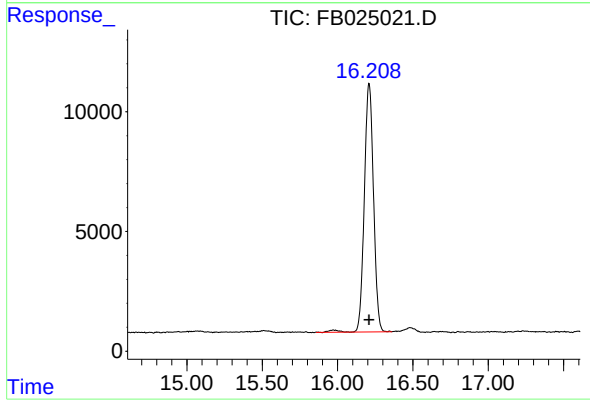

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 440605
Conc: 17.37 ng/ml