

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100521\
 Data File : FB026256.D
 Signal(s) : FID2B.CH
 Acq On : 5 Oct 2021 13:37
 Operator : AJ/MA
 Sample : M4005-18MS
 Misc : 5.04G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 06 16:09:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091621.M
 Quant Title :
 QLast Update : Thu Sep 16 16:24:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.838	229618	13.482 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.837	346472	15.594 ng/ml
2) t 2,2,4-Trimethylpentane	7.493	315136	14.178 ng/ml
3) t n-Heptane	7.813	121136	4.691 ng/ml
4) t Benzene	7.951	228944	8.406 ng/ml
6) t Toluene	10.648	629172	24.006 ng/ml
7) t Ethylbenzene	13.068	171067	7.502 ng/ml
8) t m-Xylene	13.200	331493	14.787 ng/ml
9) t O-Xylene	13.924	314057	14.790 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	282136	12.512 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100521\
Data File : FB026256.D
Signal(s) : FID2B.CH
Acq On : 5 Oct 2021 13:37
Operator : AJ/MA
Sample : M4005-18MS
Misc : 5.04G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 06 16:09:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091621.M
Quant Title :
QLast Update : Thu Sep 16 16:24:36 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

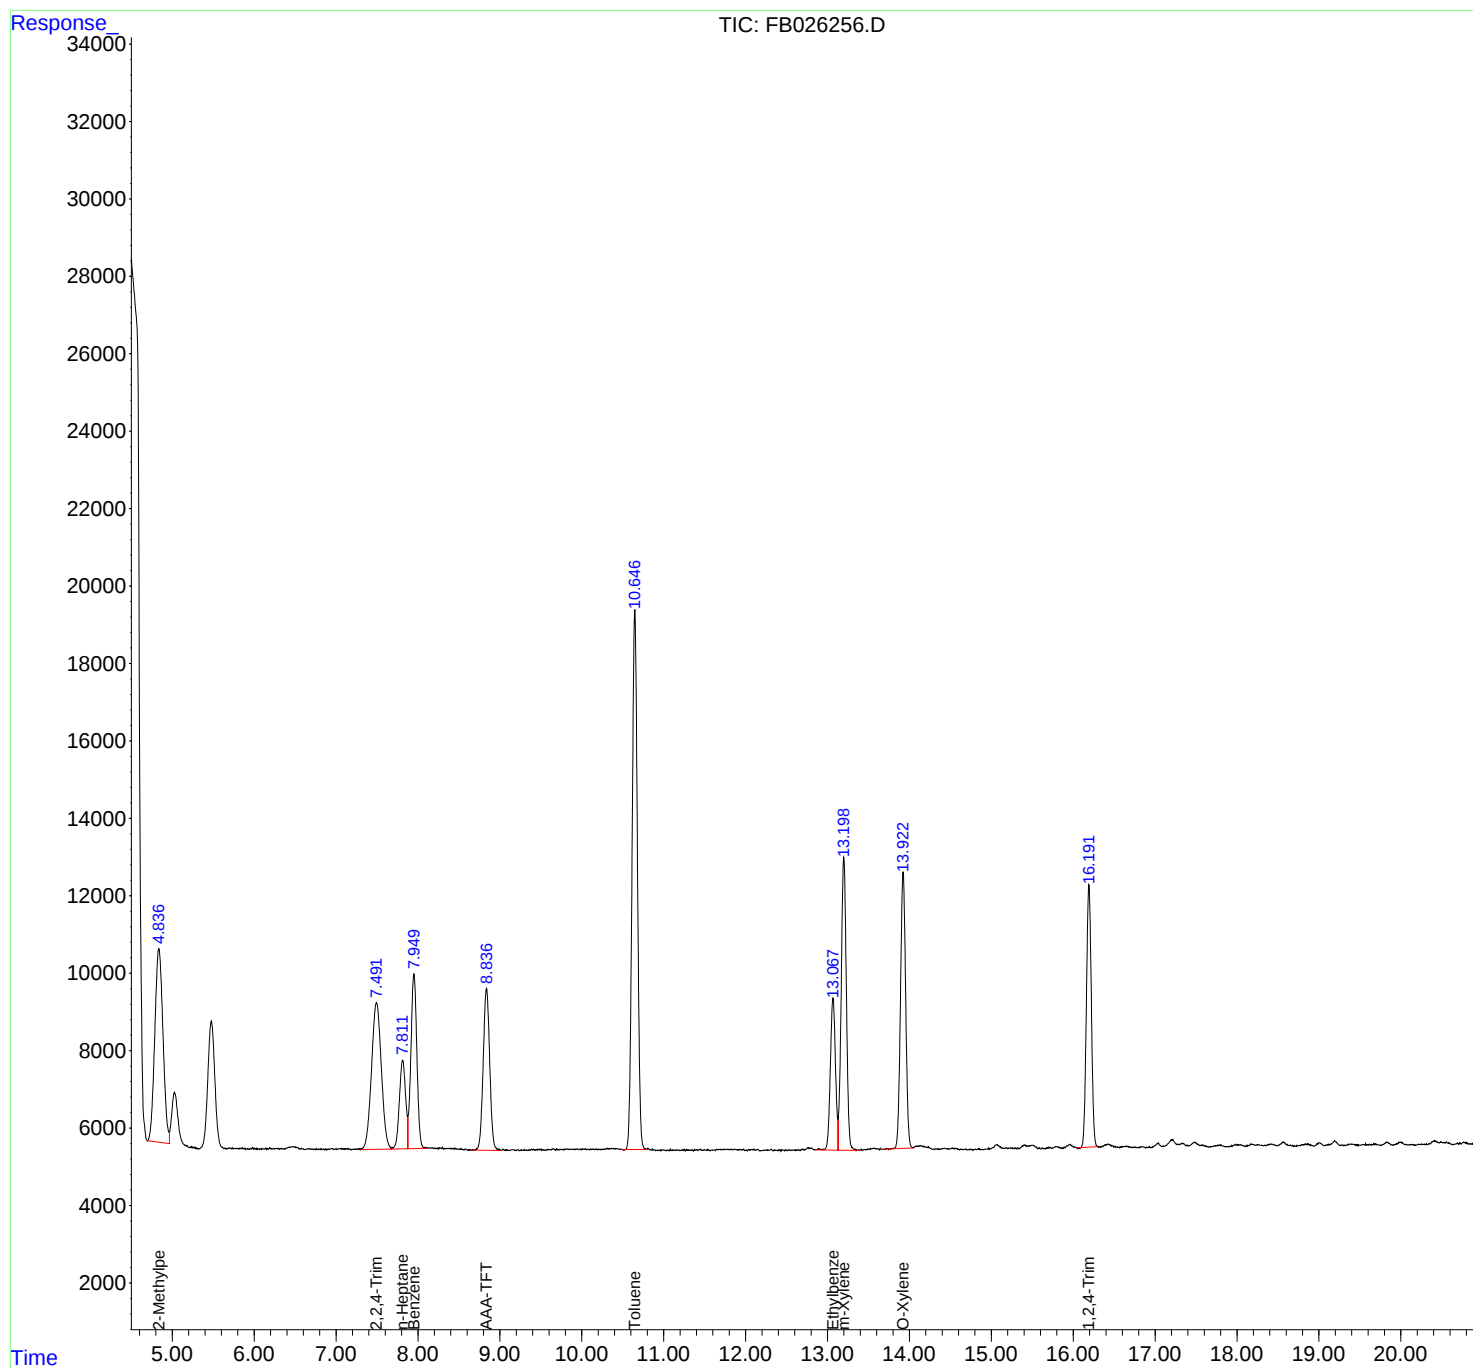

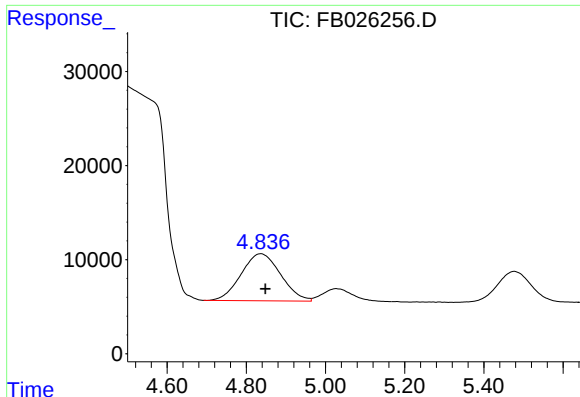


#1 2-Methylpentane

R.T.: 4.837 min
Delta R.T.: -0.011 min
Response: 346472
Conc: 15.59 ng/ml

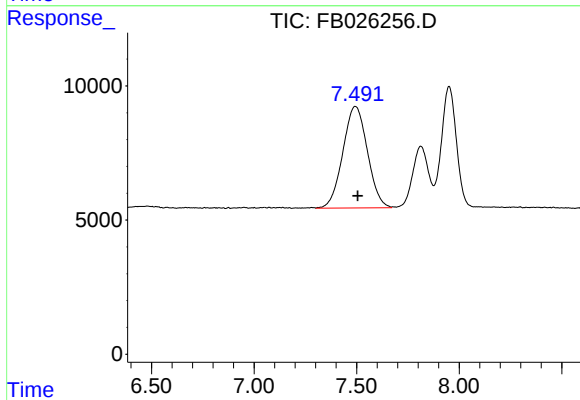


#2 2,2,4-Trimethylpentane

R.T.: 7.493 min
Delta R.T.: -0.014 min
Response: 315136
Conc: 14.18 ng/ml

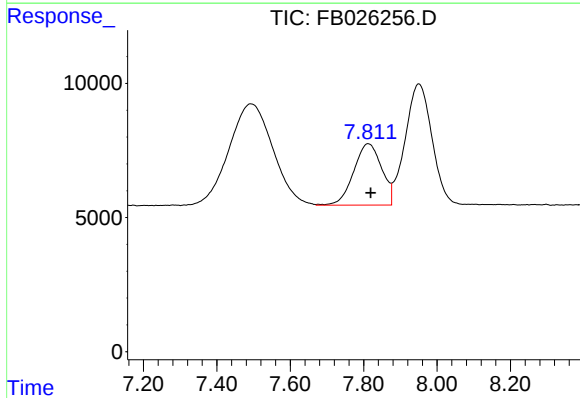


#3 n-Heptane

R.T.: 7.813 min
Delta R.T.: -0.006 min
Response: 121136
Conc: 4.69 ng/ml

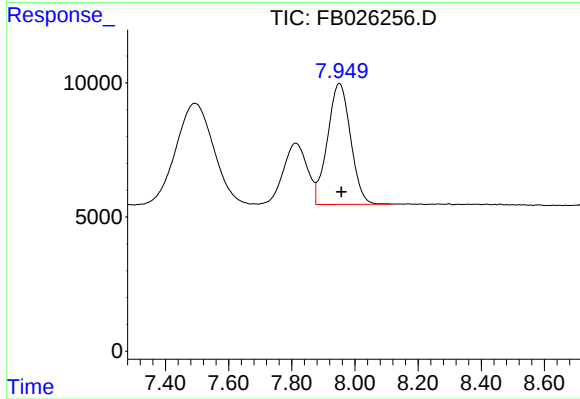


#4 Benzene

R.T.: 7.951 min
Delta R.T.: -0.006 min
Response: 228944
Conc: 8.41 ng/ml

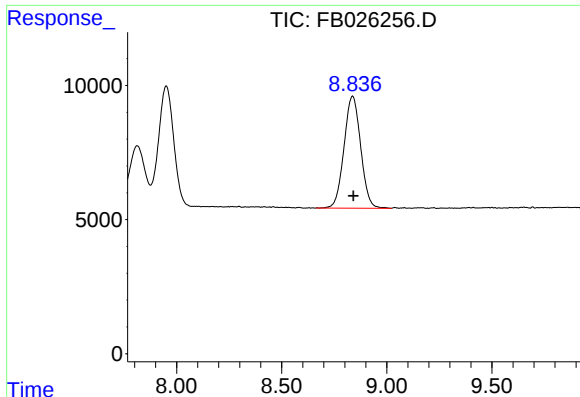


#5 AAA-TFT

R.T.: 8.838 min
Delta R.T.: -0.004 min
Response: 229618
Conc: 13.48 ng/ml

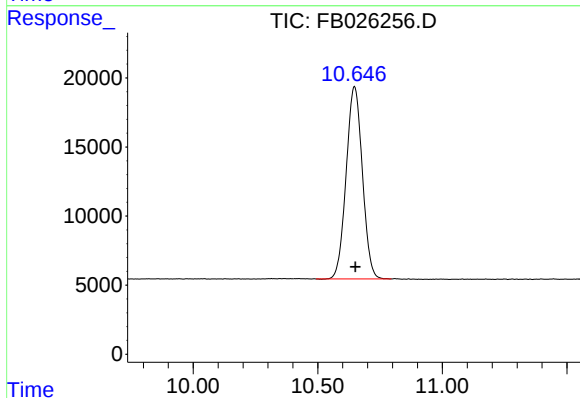


#6 Toluene

R.T.: 10.648 min
Delta R.T.: -0.004 min
Response: 629172
Conc: 24.01 ng/ml

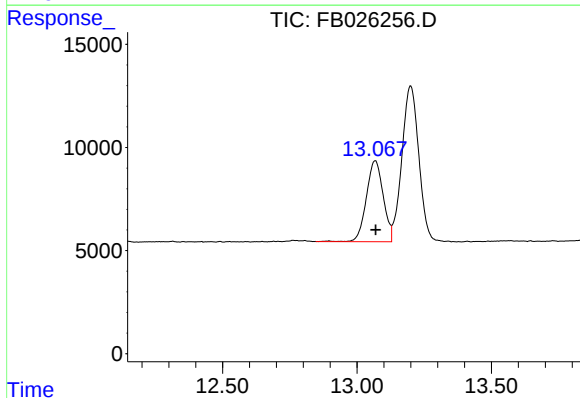


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.002 min
Response: 171067
Conc: 7.50 ng/ml

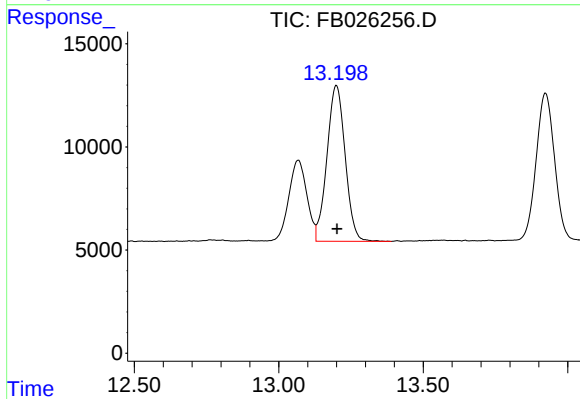


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.002 min
Response: 331493
Conc: 14.79 ng/ml

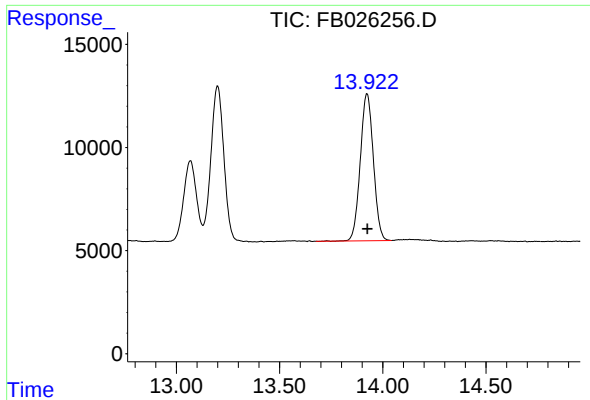

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: -0.002 min
Response: 314057
Conc: 14.79 ng/ml

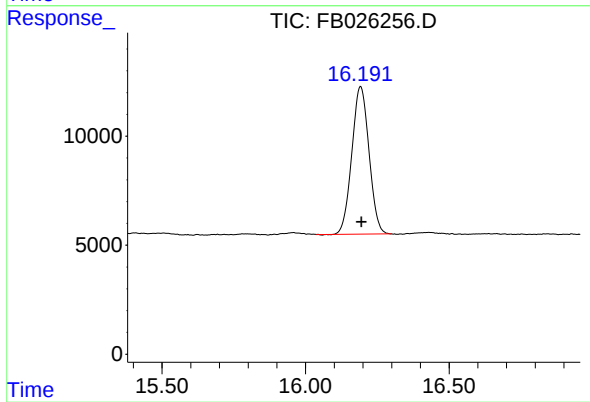

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: -0.002 min
Response: 282136
Conc: 12.51 ng/ml