

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100521\
 Data File : FB026257.D
 Signal(s) : FID2B.CH
 Acq On : 5 Oct 2021 14:23
 Operator : AJ/MA
 Sample : M4005-18MSD
 Misc : 5.06G/5.00 ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 06 16:09:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091621.M
 Quant Title :
 QLast Update : Thu Sep 16 16:24:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.841	253565	14.888 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.846	523764	23.574 ng/ml
2) t 2,2,4-Trimethylpentane	7.500	599878	26.989 ng/ml
3) t n-Heptane	7.819	232199	8.991 ng/ml
4) t Benzene	7.956	254619	9.349 ng/ml
6) t Toluene	10.650	721556	27.530 ng/ml
7) t Ethylbenzene	13.069	208040	9.123 ng/ml
8) t m-Xylene	13.201	411311	18.347 ng/ml
9) t O-Xylene	13.925	385567	18.158 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	416767	18.482 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100521\
Data File : FB026257.D
Signal(s) : FID2B.CH
Acq On : 5 Oct 2021 14:23
Operator : AJ/MA
Sample : M4005-18MSD
Misc : 5.06G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 06 16:09:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091621.M
Quant Title :
QLast Update : Thu Sep 16 16:24:36 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

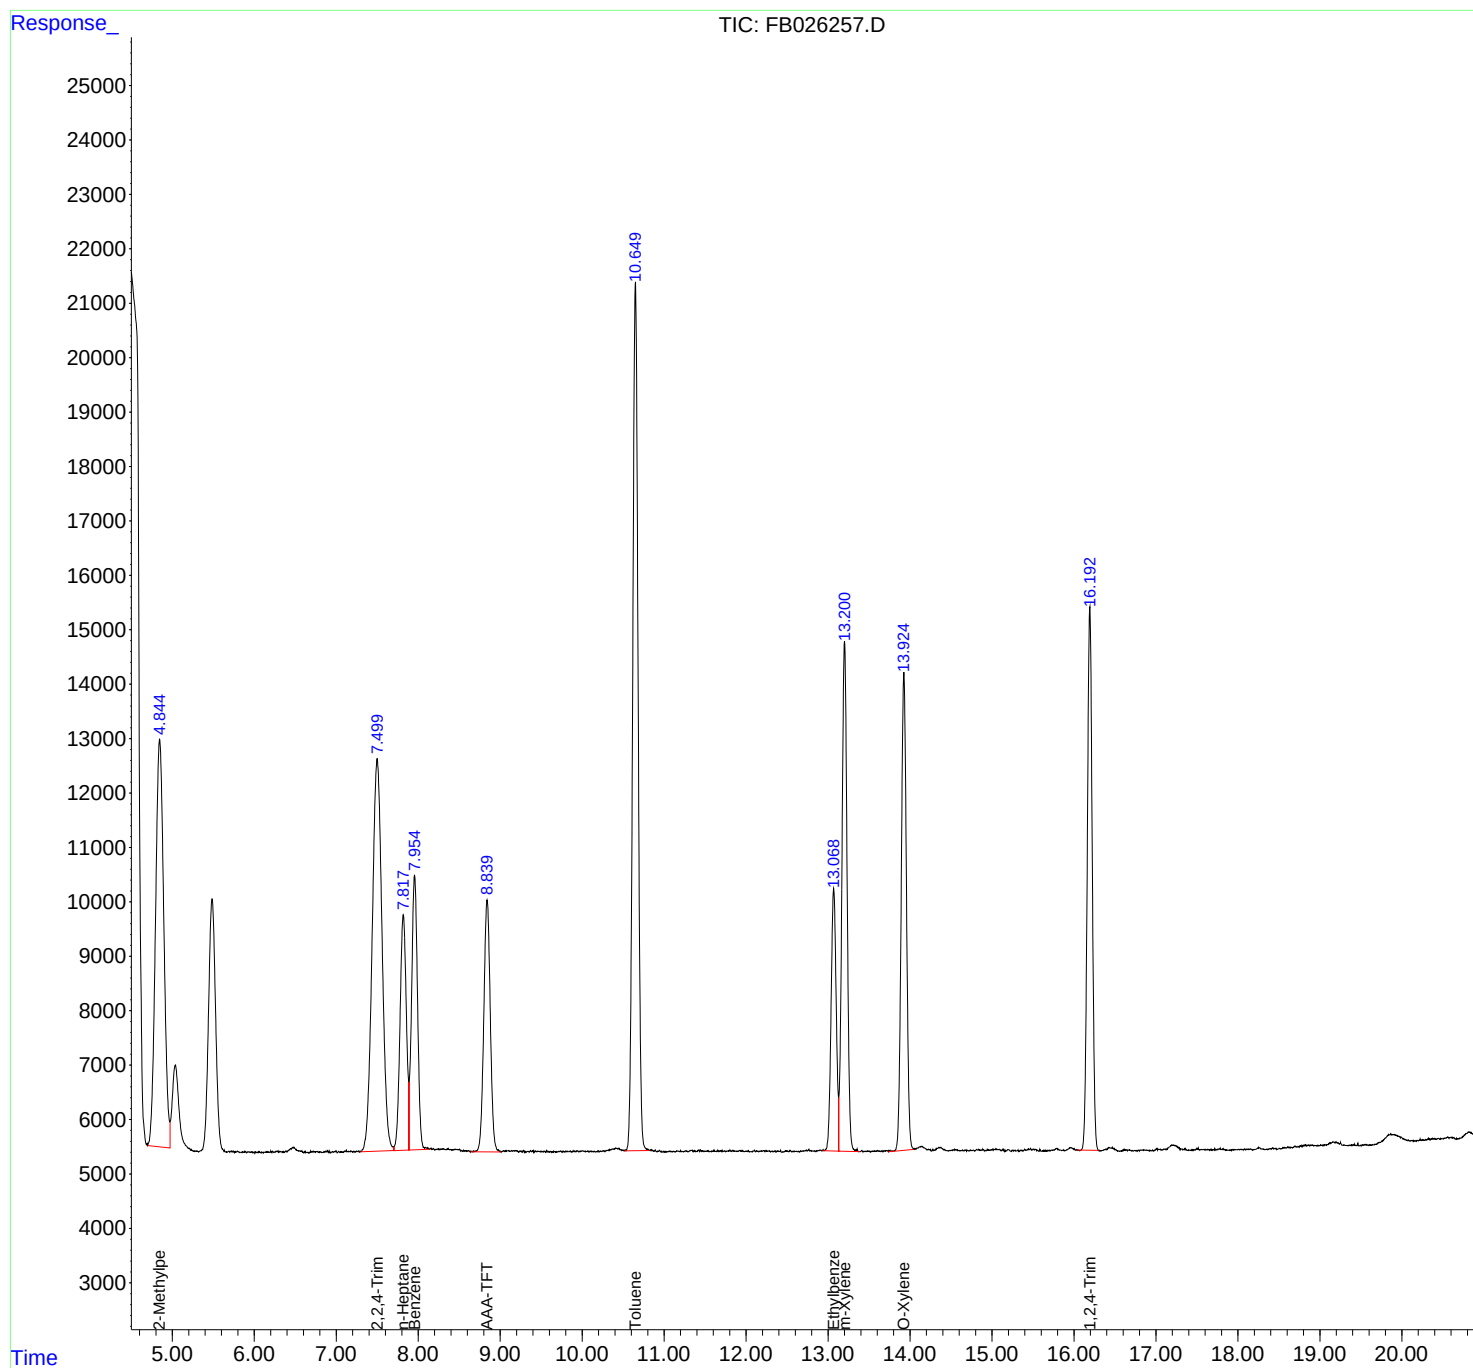

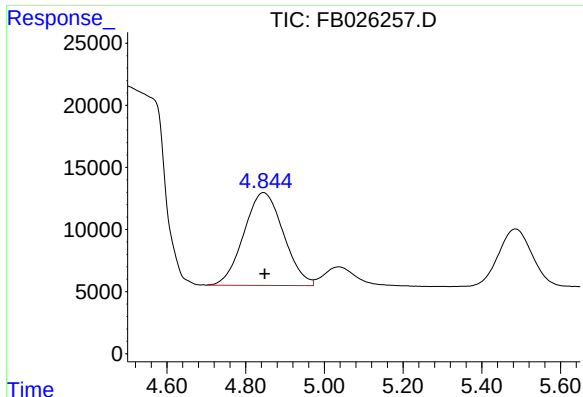


#1 2-Methylpentane

R.T.: 4.846 min
Delta R.T.: -0.002 min
Response: 523764
Conc: 23.57 ng/ml

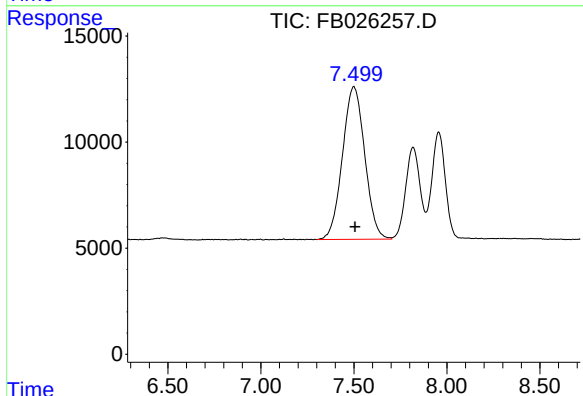


#2 2,2,4-Trimethylpentane

R.T.: 7.500 min
Delta R.T.: -0.007 min
Response: 599878
Conc: 26.99 ng/ml

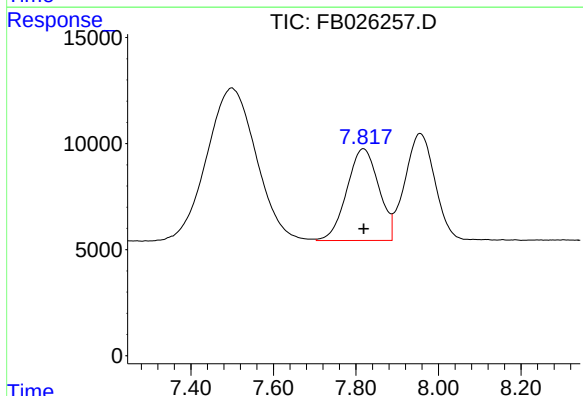


#3 n-Heptane

R.T.: 7.819 min
Delta R.T.: 0.000 min
Response: 232199
Conc: 8.99 ng/ml

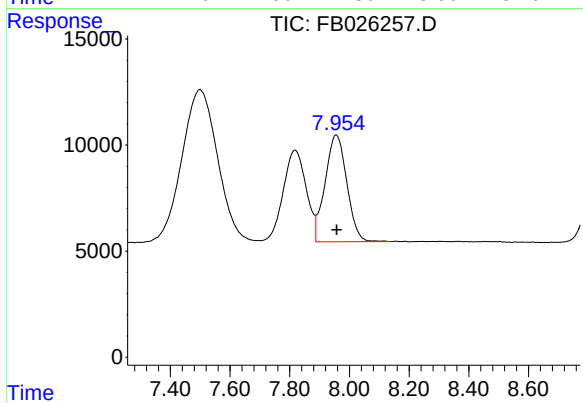


#4 Benzene

R.T.: 7.956 min
Delta R.T.: -0.001 min
Response: 254619
Conc: 9.35 ng/ml

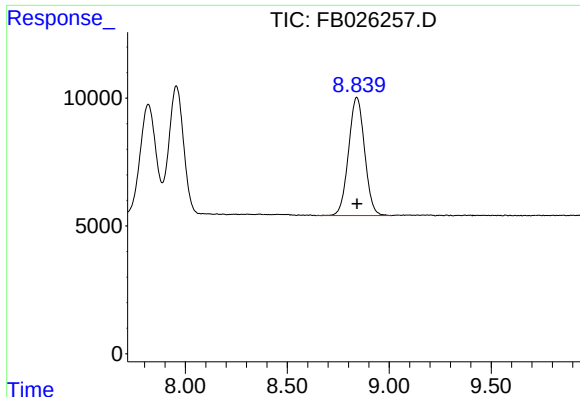


#5 AAA-TFT

R.T.: 8.841 min
Delta R.T.: -0.001 min
Response: 253565
Conc: 14.89 ng/ml

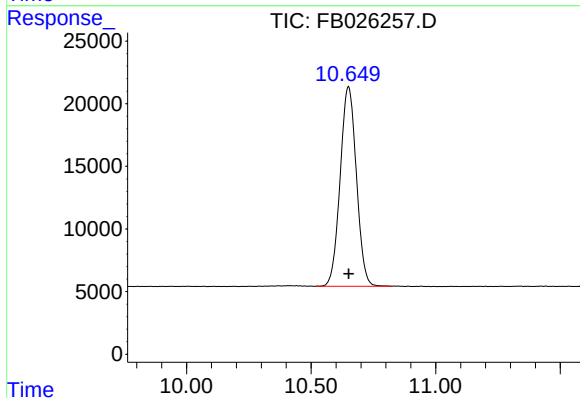


#6 Toluene

R.T.: 10.650 min
Delta R.T.: 0.000 min
Response: 721556
Conc: 27.53 ng/ml

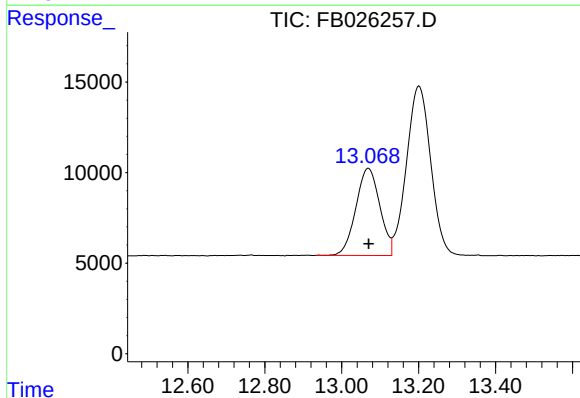


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: 0.000 min
Response: 208040
Conc: 9.12 ng/ml

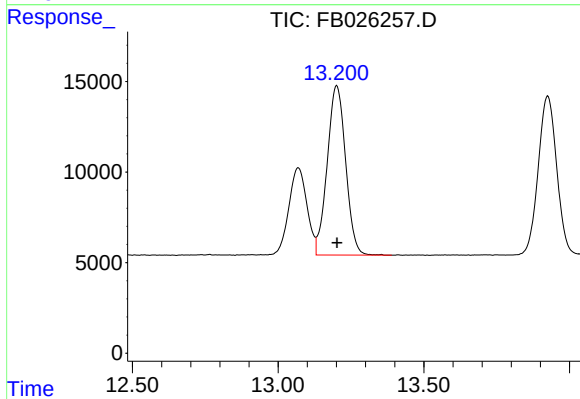

#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: 0.000 min
Response: 411311
Conc: 18.35 ng/ml

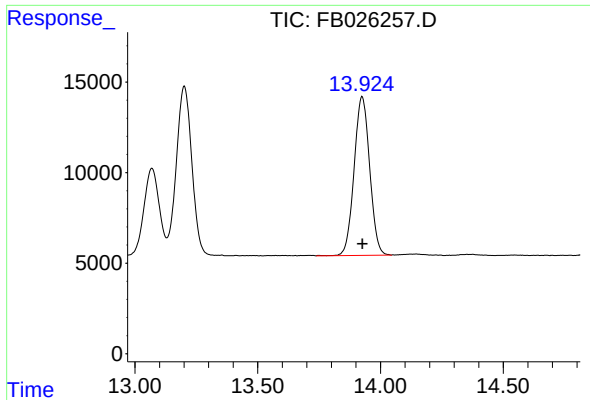


#9 O-Xylene

R.T.: 13.925 min

Delta R.T.: 0.000 min

Response: 385567

Conc: 18.16 ng/ml

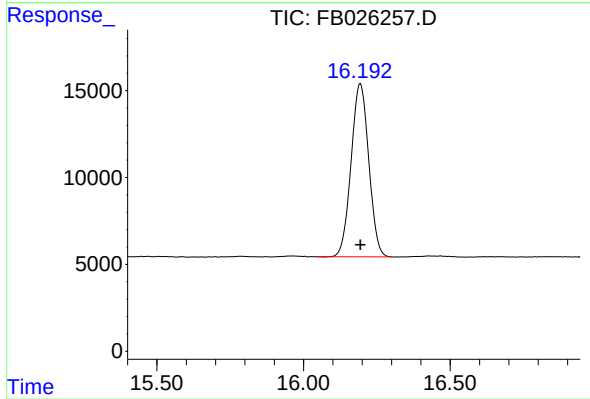

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min

Delta R.T.: 0.000 min

Response: 416767

Conc: 18.48 ng/ml