

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100521\
 Data File : FB026252.D
 Signal(s) : FID2B.CH
 Acq On : 5 Oct 2021 10:40
 Operator : AJ/MA
 Sample : BSF100551
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: SAMPLE.e
 Quant Time: Oct 05 12:19:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091621.M
 Quant Title :
 QLast Update : Thu Sep 16 16:24:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.841	288284	16.927 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.855	527041	23.721 ng/ml
2) t 2,2,4-Trimethylpentane	7.503	657120	29.564 ng/ml
3) t n-Heptane	7.820	245385	9.502 ng/ml
4) t Benzene	7.958	270305	9.925 ng/ml
6) t Toluene	10.650	788668	30.091 ng/ml
7) t Ethylbenzene	13.067	233679	10.248 ng/ml
8) t m-Xylene	13.199	461075	20.567 ng/ml
9) t O-Xylene	13.923	445932	21.001 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	490257	21.741 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100521\
Data File : FB026252.D
Signal(s) : FID2B.CH
Acq On : 5 Oct 2021 10:40
Operator : AJ/MA
Sample : BSF1005S1
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: SAMPLE.e
Quant Time: Oct 05 12:19:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091621.M
Quant Title :
QLast Update : Thu Sep 16 16:24:36 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

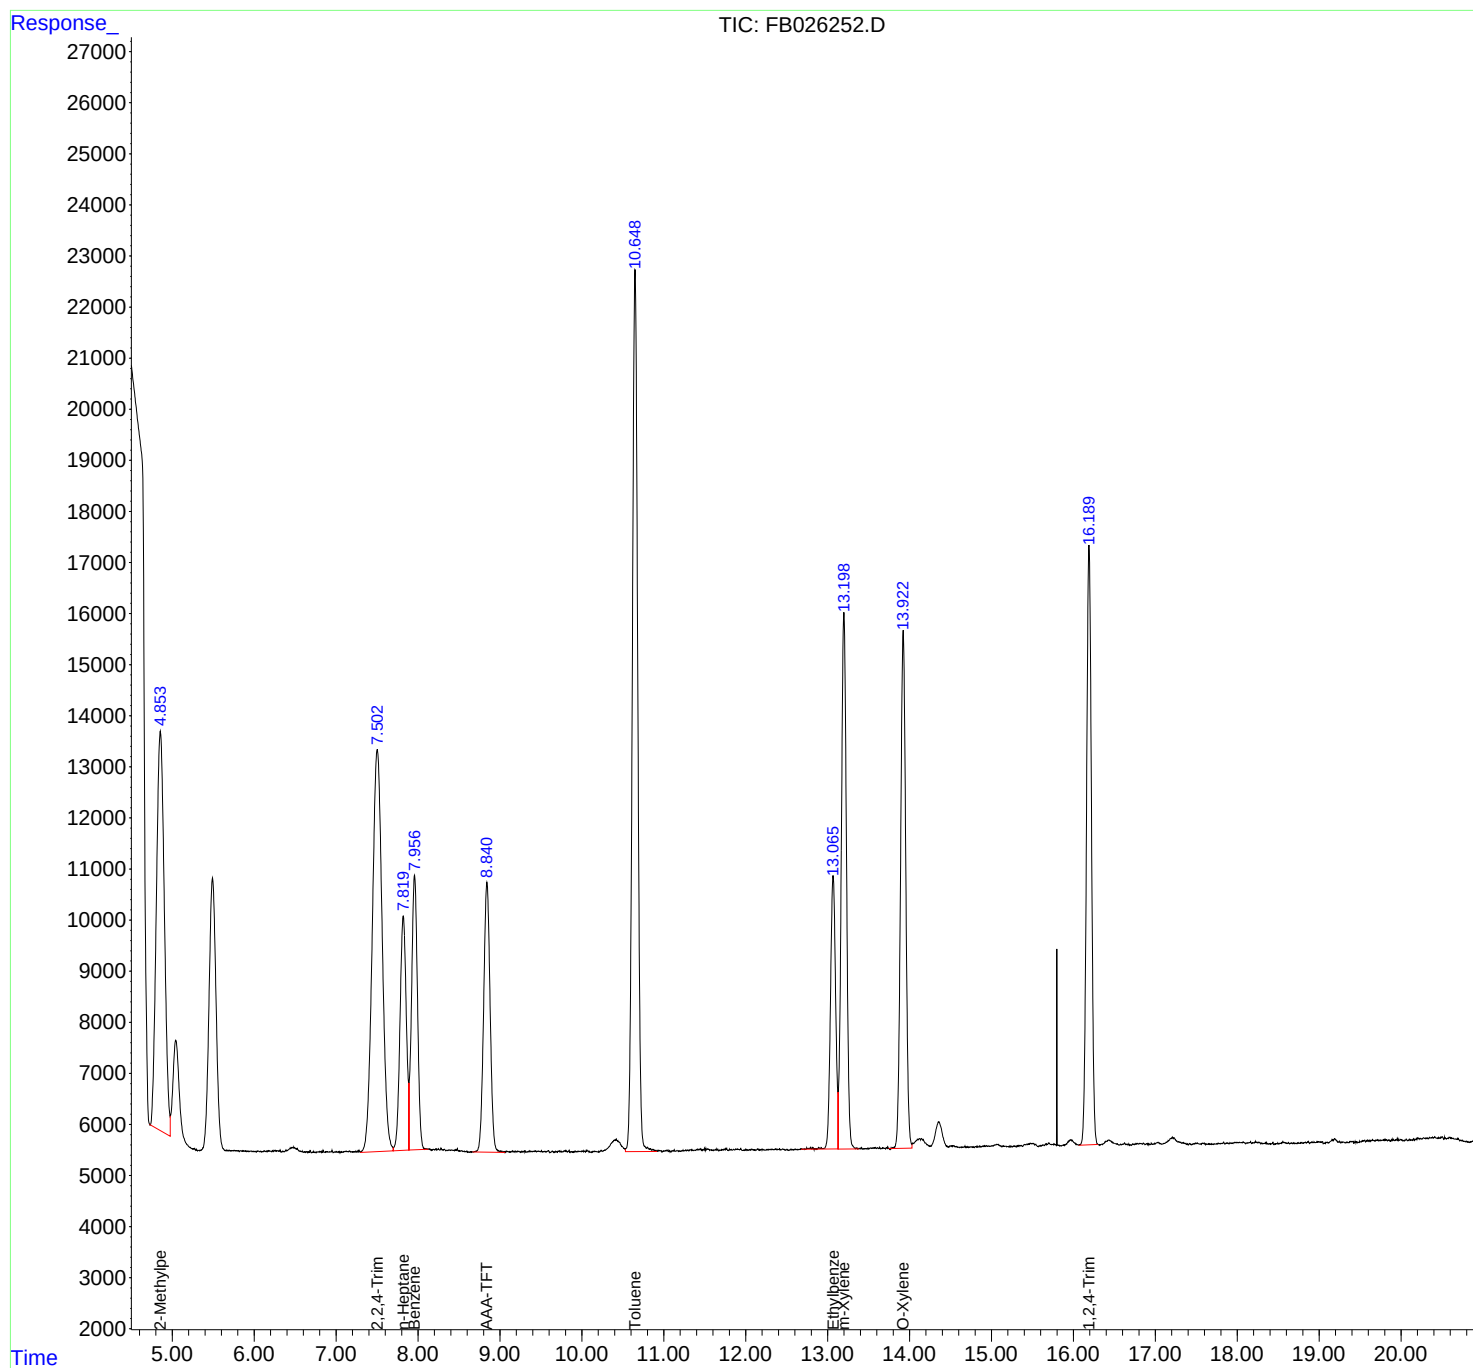

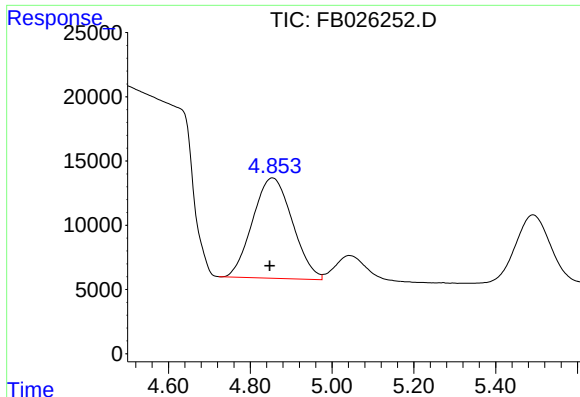


#1 2-Methylpentane

R.T.: 4.855 min
Delta R.T.: 0.007 min
Response: 527041
Conc: 23.72 ng/ml

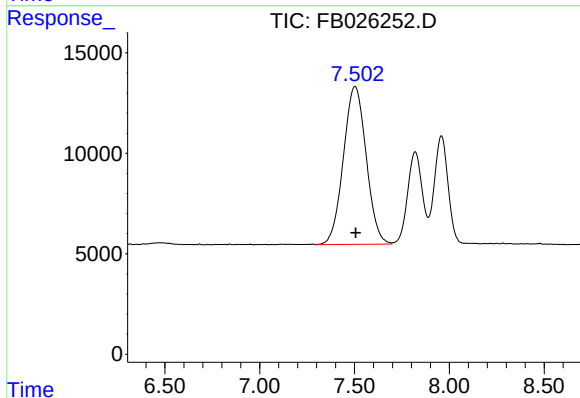


#2 2,2,4-Trimethylpentane

R.T.: 7.503 min
Delta R.T.: -0.004 min
Response: 657120
Conc: 29.56 ng/ml

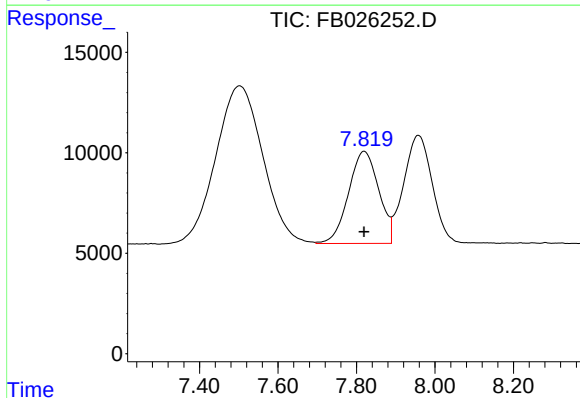


#3 n-Heptane

R.T.: 7.820 min
Delta R.T.: 0.000 min
Response: 245385
Conc: 9.50 ng/ml

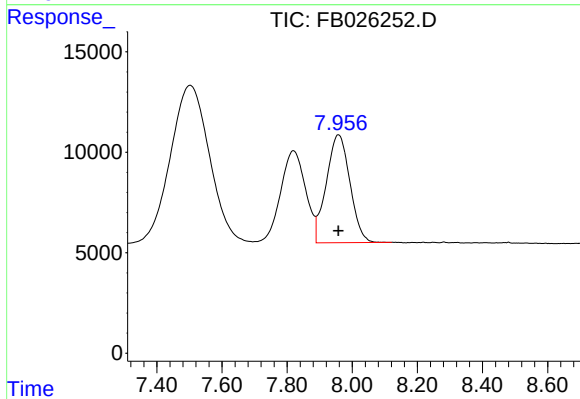


#4 Benzene

R.T.: 7.958 min
Delta R.T.: 0.000 min
Response: 270305
Conc: 9.92 ng/ml

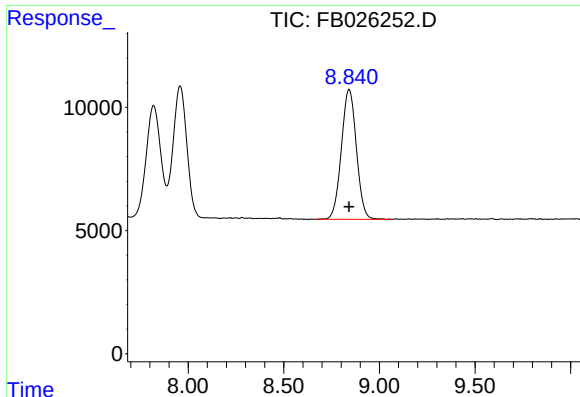


#5 AAA-TFT

R.T.: 8.841 min
Delta R.T.: 0.000 min
Response: 288284
Conc: 16.93 ng/ml

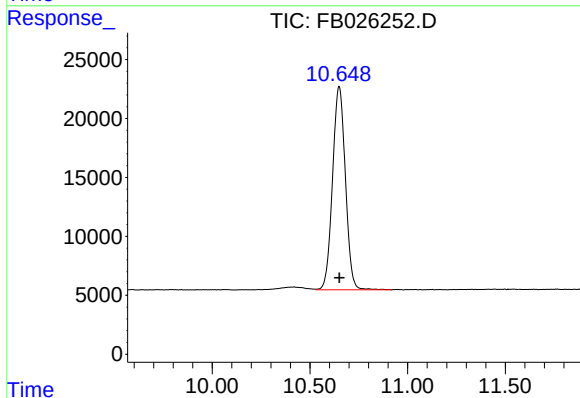


#6 Toluene

R.T.: 10.650 min
Delta R.T.: -0.002 min
Response: 788668
Conc: 30.09 ng/ml

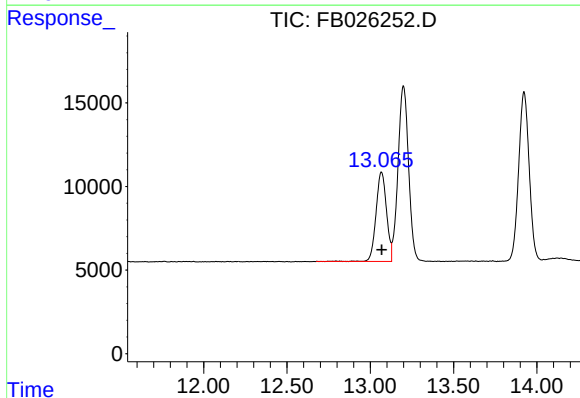


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.003 min
Response: 233679
Conc: 10.25 ng/ml

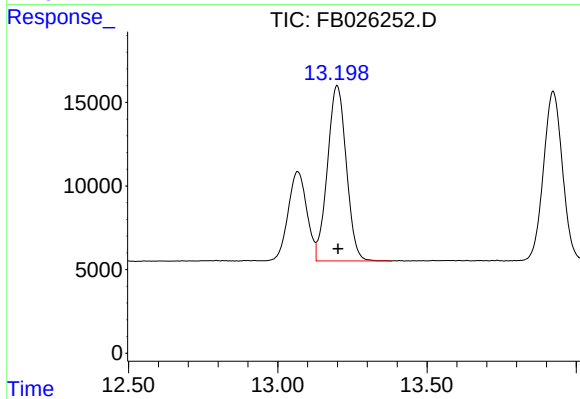


#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: -0.003 min
Response: 461075
Conc: 20.57 ng/ml

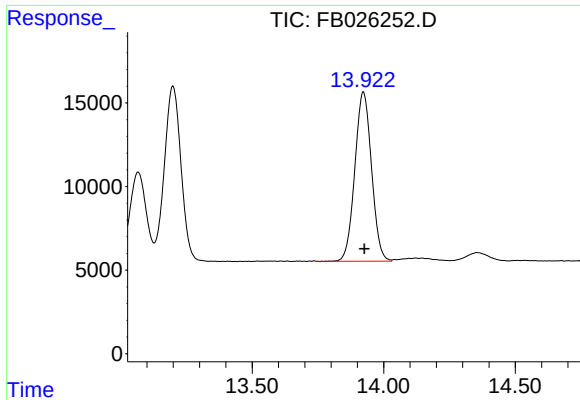

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: -0.003 min
Response: 445932
Conc: 21.00 ng/ml

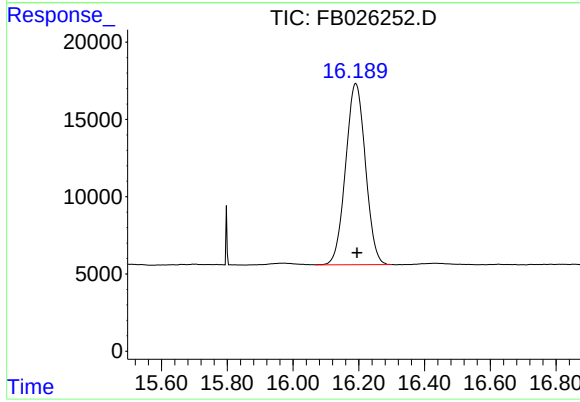

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: -0.003 min
Response: 490257
Conc: 21.74 ng/ml