

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100622\
 Data File : FB028537.D
 Signal(s) : FID2B.CH
 Acq On : 6 Oct 2022 11:41
 Operator : AJ/MA
 Sample : BSF1006S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1006S1

Integration File: Calibration.e
 Quant Time: Oct 07 06:25:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	277732	21.468 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.714	509765	31.161 ng/ml
2) t 2,2,4-Trimethylpentane	7.430	588832	32.582 ng/ml
3) t n-Heptane	7.753	178765	10.554 ng/ml
4) t Benzene	7.890	236342	10.760 ng/ml
6) t Toluene	10.624	691205	32.977 ng/ml
7) t Ethylbenzene	13.060	212628	10.714 ng/ml
8) t m-Xylene	13.193	422531	21.447 ng/ml
9) t O-Xylene	13.920	417405	21.455 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	407458	21.047 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100622\
Data File : FB028537.D
Signal(s) : FID2B.CH
Acq On : 6 Oct 2022 11:41
Operator : AJ/MA
Sample : BSF1006S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1006S1

Integration File: Calibration.e
Quant Time: Oct 07 06:25:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

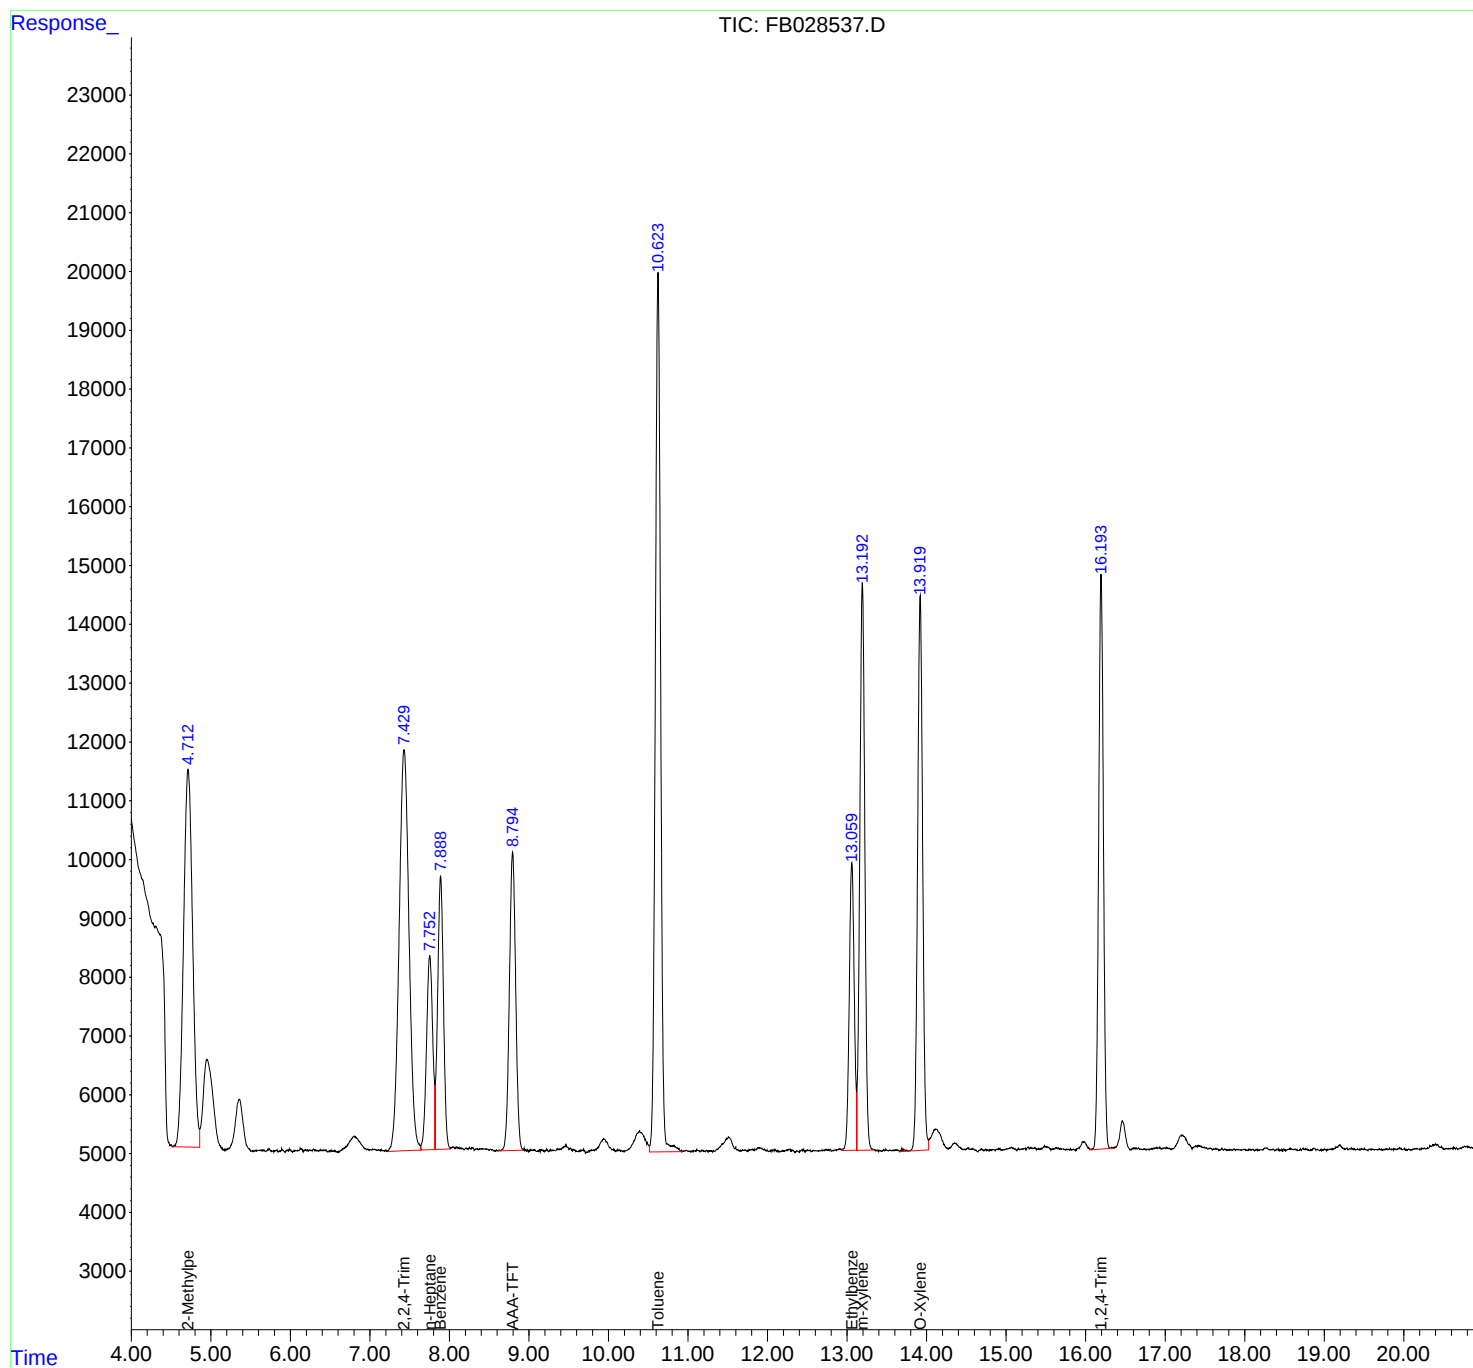


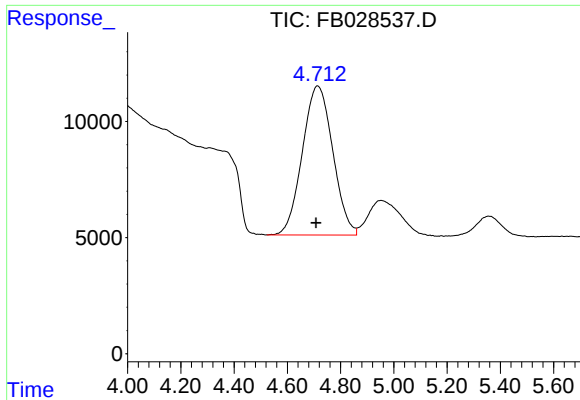

#1 2-Methylpentane


R.T.: 4.714 min
Delta R.T.: 0.006 min
Response: 509765
Conc: 31.16 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1006S1

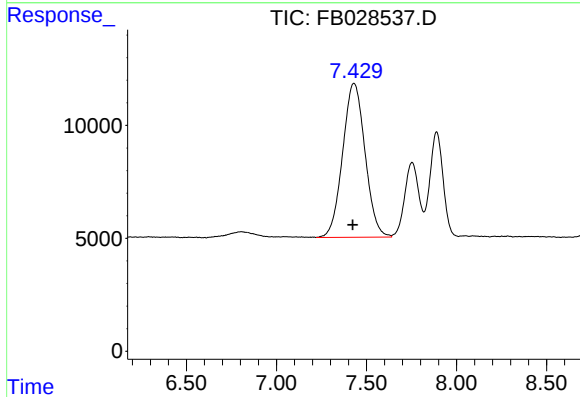


#2 2,2,4-Trimethylpentane

R.T.: 7.430 min
Delta R.T.: 0.007 min
Response: 588832
Conc: 32.58 ng/ml

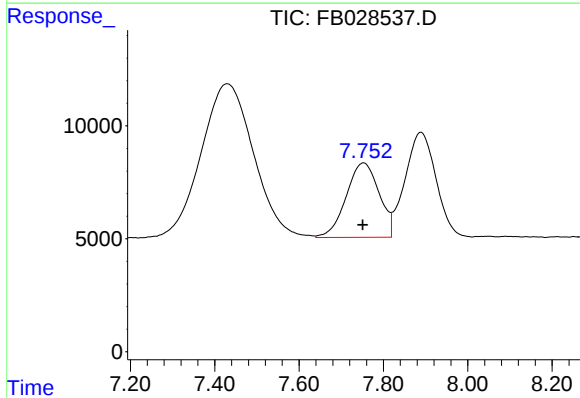


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.002 min
Response: 178765
Conc: 10.55 ng/ml

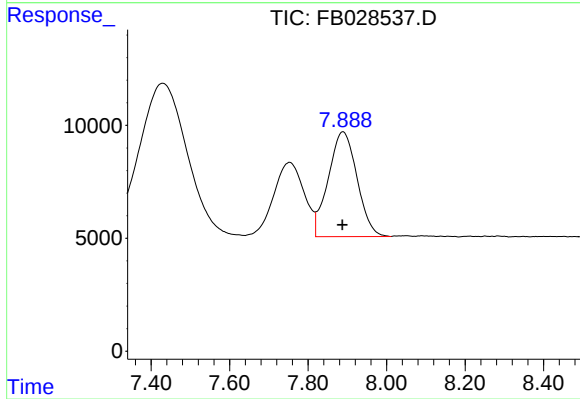

#4 Benzene


R.T.: 7.890 min
Delta R.T.: 0.002 min
Response: 236342
Conc: 10.76 ng/ml

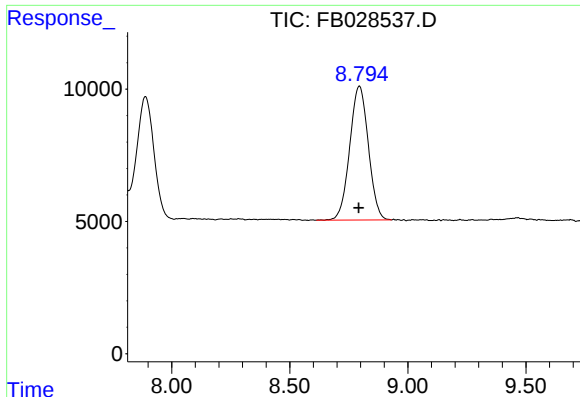

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.003 min
Response: 277732
Conc: 21.47 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1006S1

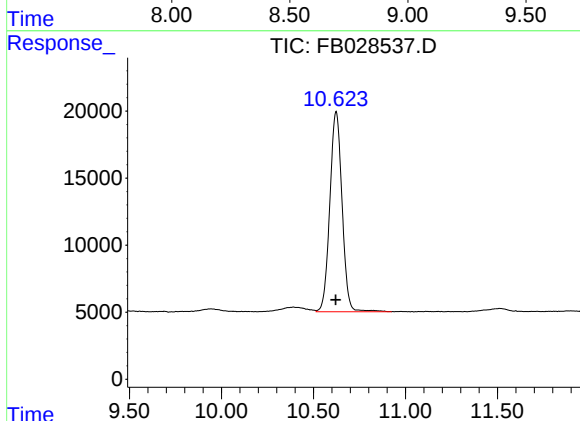


#6 Toluene

R.T.: 10.624 min
Delta R.T.: 0.003 min
Response: 691205
Conc: 32.98 ng/ml

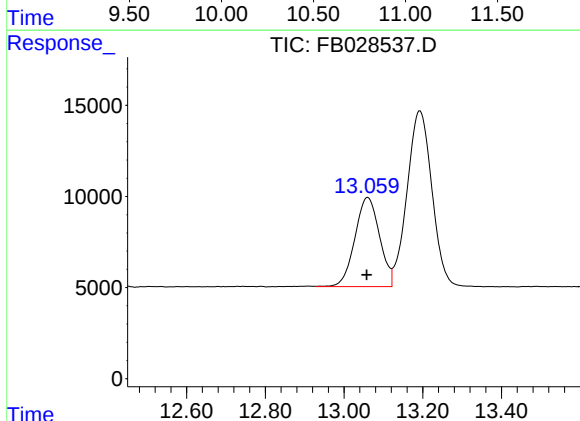


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.002 min
Response: 212628
Conc: 10.71 ng/ml

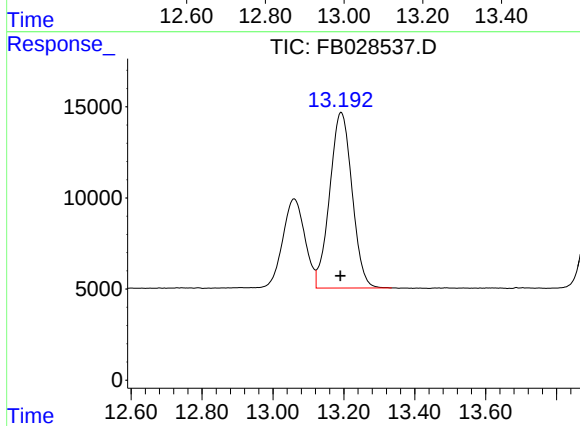

#8 m-Xylene


R.T.: 13.193 min
Delta R.T.: 0.002 min
Response: 422531
Conc: 21.45 ng/ml

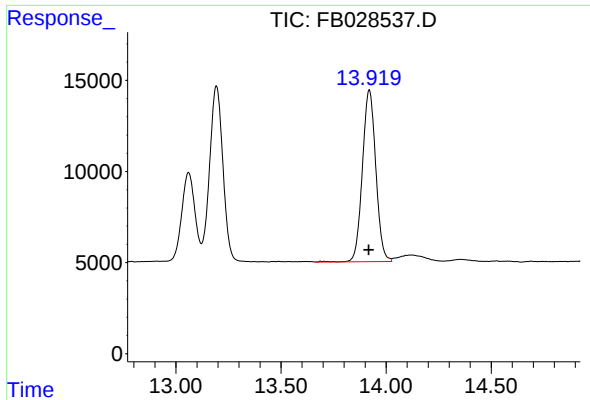

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.003 min
Response: 417405
Conc: 21.46 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1006S1

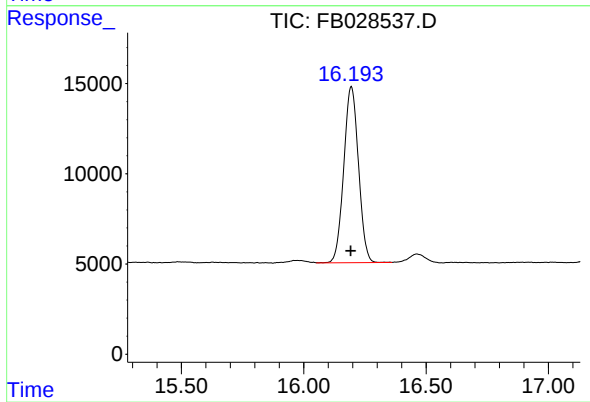

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: 0.002 min
Response: 407458
Conc: 21.05 ng/ml