

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB100622\  
Data File : FB028538.D  
Signal(s) : FID2B.CH  
Acq On : 6 Oct 2022 12:22  
Operator : AJ/MA  
Sample : N4988-01  
Misc : 5.01G/5.00 ML DI WATER  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
AU-5-100422

Integration File: Calibration.e  
Quant Time: Oct 07 06:25:57 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB100522.M  
Quant Title :  
QLast Update : Wed Oct 05 12:47:25 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound | R.T. | Response | Conc Units |
|----------|------|----------|------------|
|----------|------|----------|------------|

-----  
System Monitoring Compounds

Target Compounds  
-----

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB100622\  
Data File : FB028538.D  
Signal(s) : FID2B.CH  
Acq On : 6 Oct 2022 12:22  
Operator : AJ/MA  
Sample : N4988-01  
Misc : 5.01G/5.00 ML DI WATER  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
AU-5-100422

Integration File: Calibration.e  
Quant Time: Oct 07 06:25:57 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB100522.M  
Quant Title :  
QLast Update : Wed Oct 05 12:47:25 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

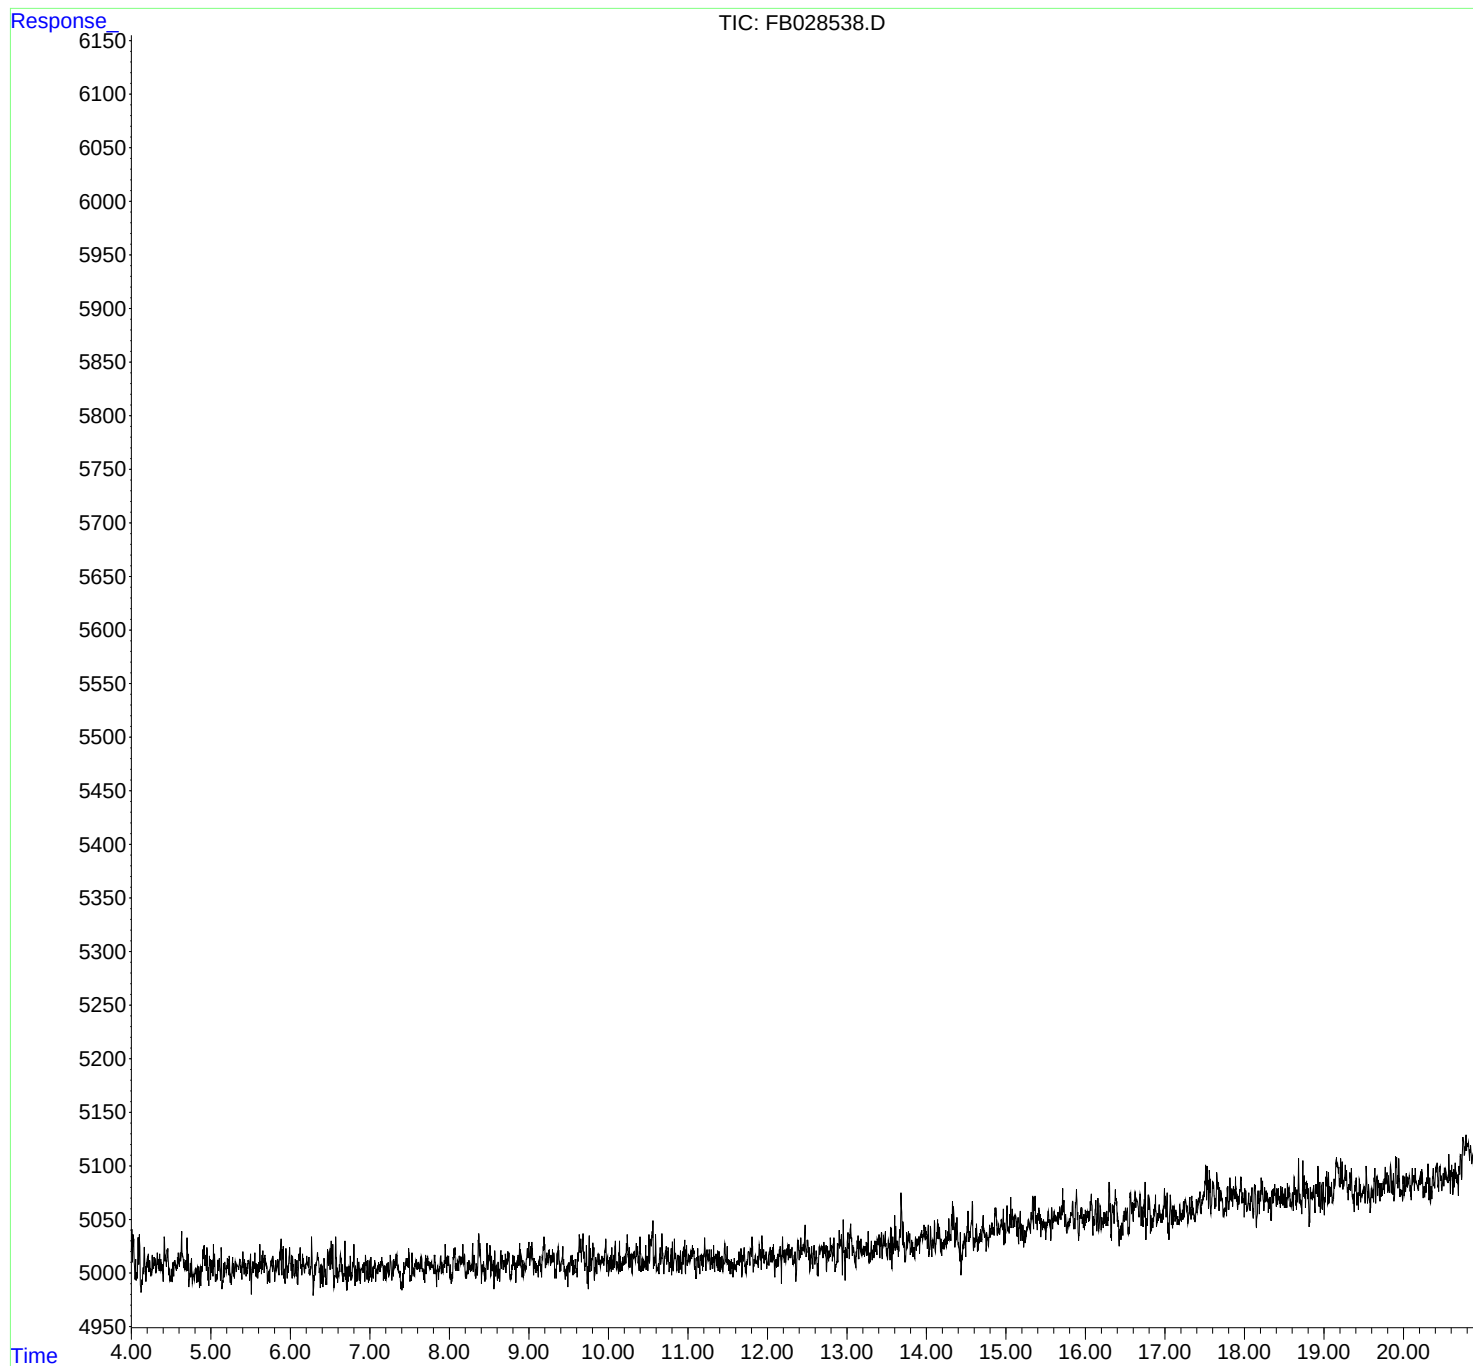

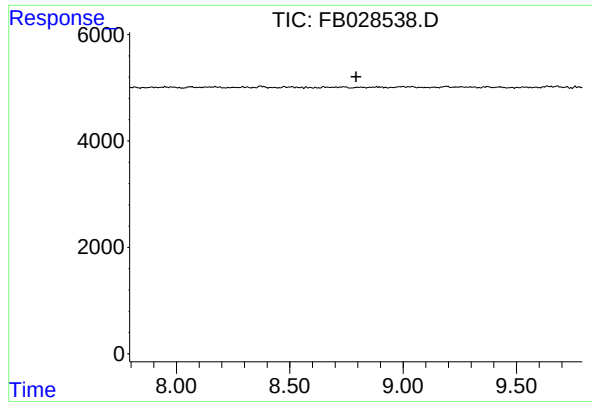

#5 AAA-TFT

R.T.: 0.000 min  
Exp R.T.: 8.793 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_B  
ClientSampleId :  
AU-5-100422