

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100622\
 Data File : FB028542.D
 Signal(s) : FID2B.CH
 Acq On : 6 Oct 2022 15:04
 Operator : AJ/MA
 Sample : N4988-01MSD 50X
 Misc : 5.01G/5.00 ML MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 AU-5-100422MSD

Integration File: Calibration.e
 Quant Time: Oct 07 06:26:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	377380	29.170 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.699	449585	27.482 ng/ml
2) t 2,2,4-Trimethylpentane	7.438	624442	34.553 ng/ml
3) t n-Heptane	7.753	204477	12.072 ng/ml
4) t Benzene	7.890	298015	13.568 ng/ml
6) t Toluene	10.626	802212	38.273 ng/ml
7) t Ethylbenzene	13.064	248129	12.502 ng/ml
8) t m-Xylene	13.196	490569	24.901 ng/ml
9) t O-Xylene	13.924	473153	24.321 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	418324	21.609 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100622\
Data File : FB028542.D
Signal(s) : FID2B.CH
Acq On : 6 Oct 2022 15:04
Operator : AJ/MA
Sample : N4988-01MSD 50X
Misc : 5.01G/5.00 ML MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
AU-5-100422MSD

Integration File: Calibration.e
Quant Time: Oct 07 06:26:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

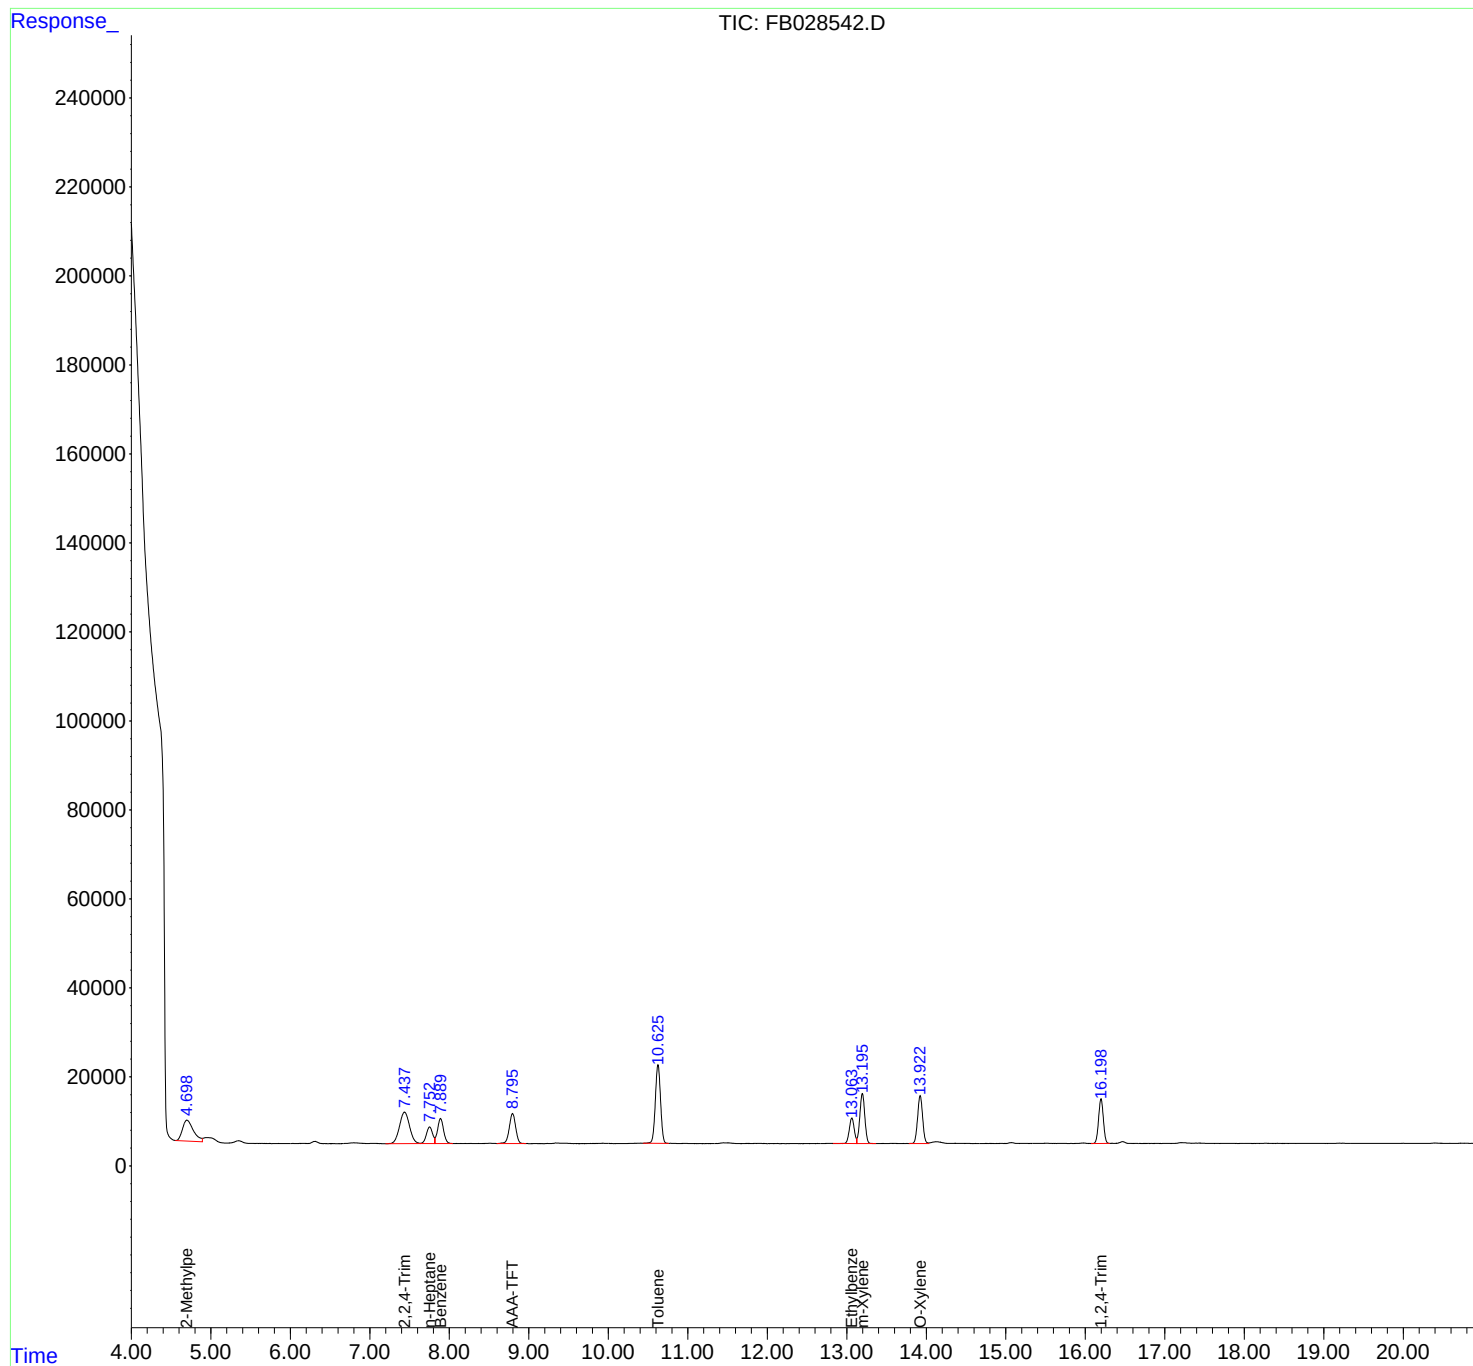


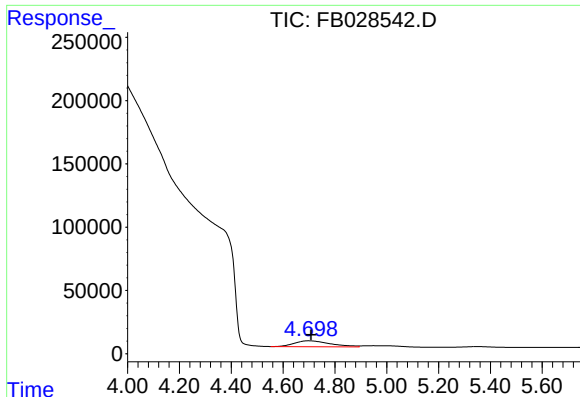

#1 2-Methylpentane


R.T.: 4.699 min
Delta R.T.: -0.009 min
Response: 449585
Conc: 27.48 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-5-100422MSD

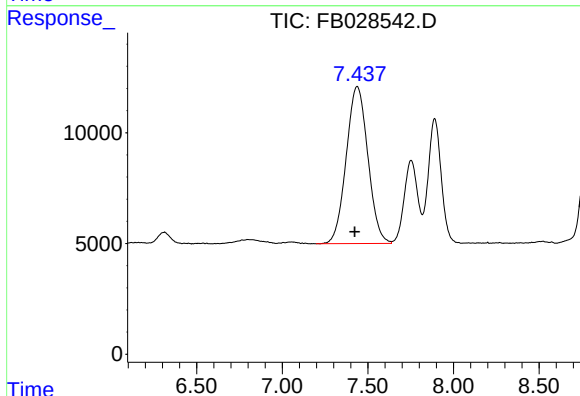


#2 2,2,4-Trimethylpentane

R.T.: 7.438 min
Delta R.T.: 0.015 min
Response: 624442
Conc: 34.55 ng/ml

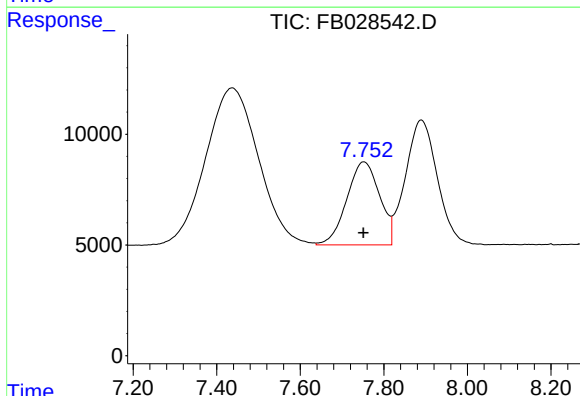


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.001 min
Response: 204477
Conc: 12.07 ng/ml

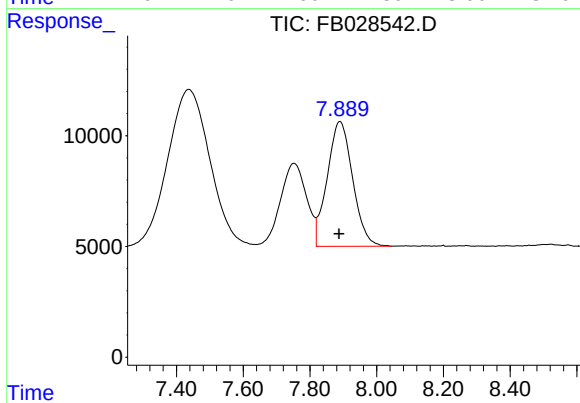

#4 Benzene


R.T.: 7.890 min
Delta R.T.: 0.002 min
Response: 298015
Conc: 13.57 ng/ml

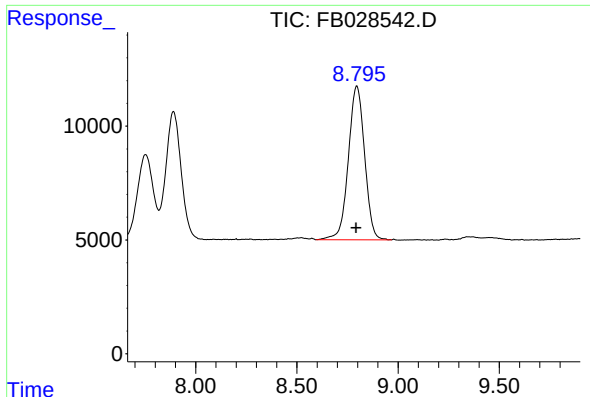

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: 0.004 min
Response: 377380
Conc: 29.17 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-5-100422MSD

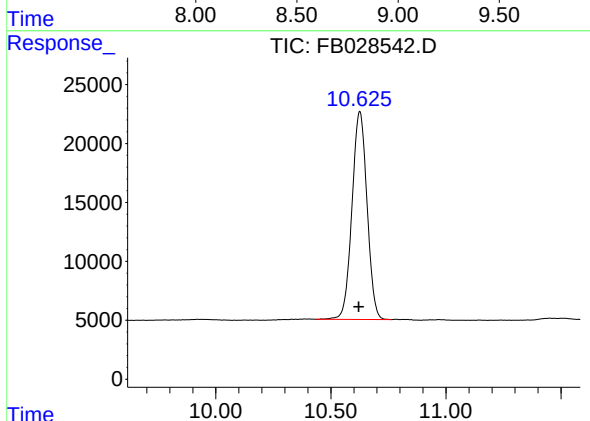


#6 Toluene

R.T.: 10.626 min
Delta R.T.: 0.005 min
Response: 802212
Conc: 38.27 ng/ml

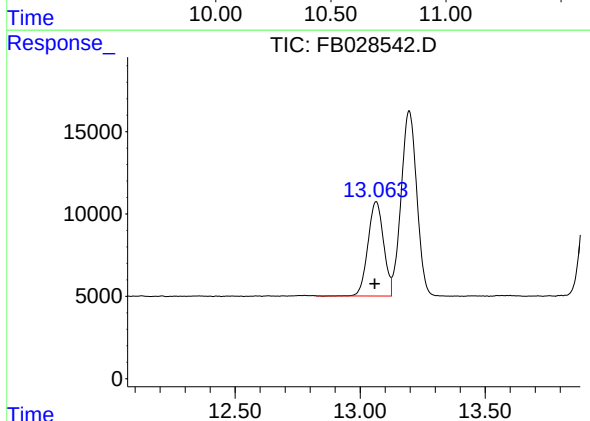


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: 0.007 min
Response: 248129
Conc: 12.50 ng/ml

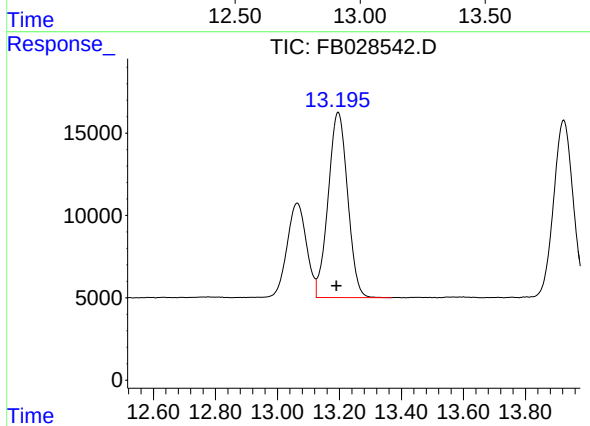

#8 m-Xylene


R.T.: 13.196 min
Delta R.T.: 0.006 min
Response: 490569
Conc: 24.90 ng/ml

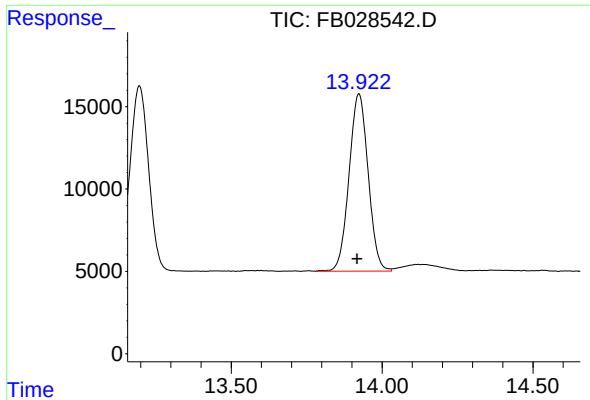

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.006 min
Response: 473153
Conc: 24.32 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-5-100422MSD

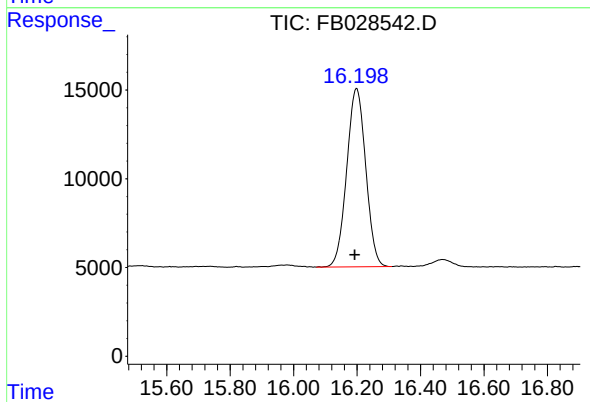

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min
Delta R.T.: 0.006 min
Response: 418324
Conc: 21.61 ng/ml