

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100622\
Data File : FB028548.D
Signal(s) : FID2B.CH
Acq On : 6 Oct 2022 19:15
Operator : AJ/MA
Sample : N5014-16 50X
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
COMP-1

Integration File: Calibration.e
Quant Time: Oct 07 06:26:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	330106	25.516 ng/ml
Target Compounds			
4) t Benzene	7.945	16770	0.763 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100622\
Data File : FB028548.D
Signal(s) : FID2B.CH
Acq On : 6 Oct 2022 19:15
Operator : AJ/MA
Sample : N5014-16 50X
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
COMP-1

Integration File: Calibration.e
Quant Time: Oct 07 06:26:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

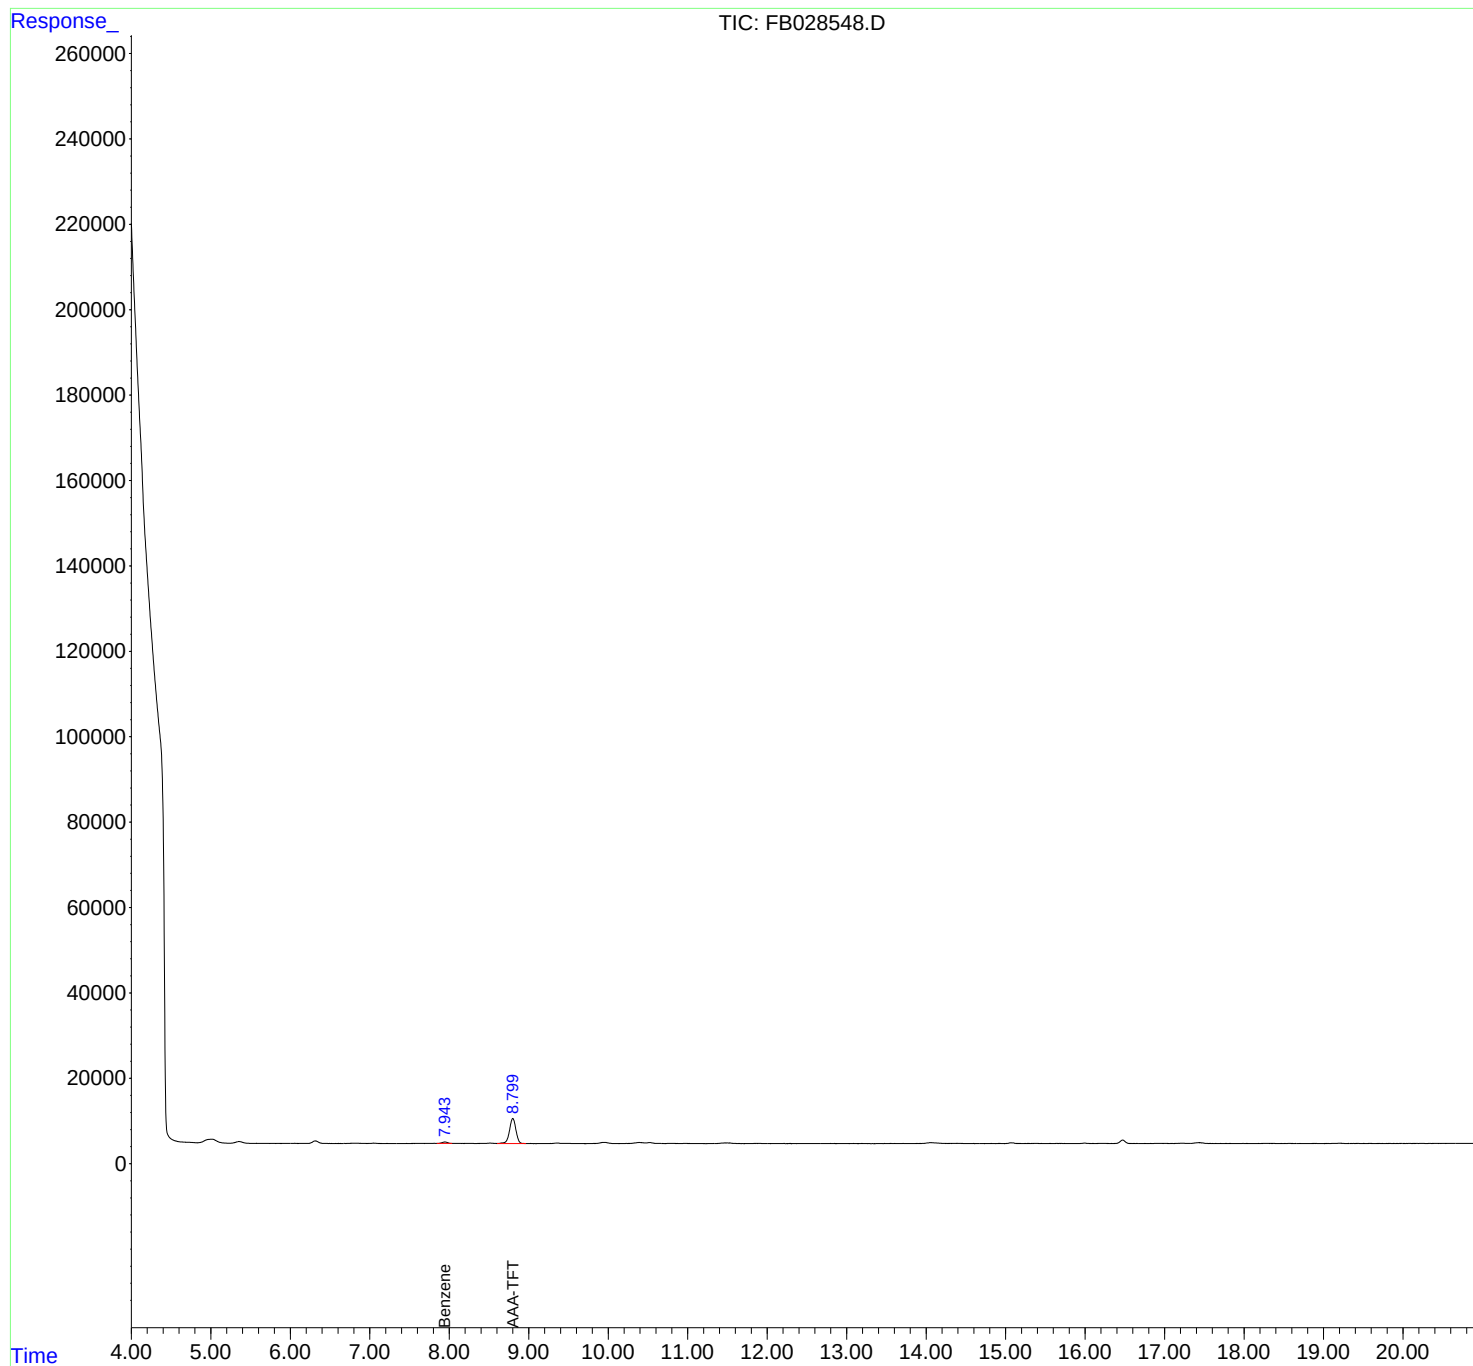


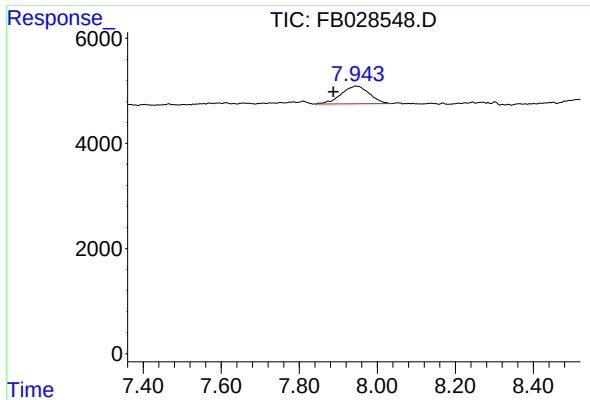

#4 Benzene

R.T.: 7.945 min
Delta R.T.: 0.057 min
Response: 16770
Conc: 0.76 ng/ml

Instrument :
FID_B
ClientSampleId :
COMP-1

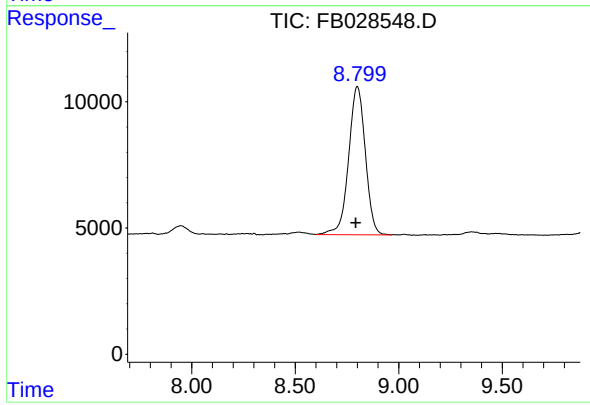

#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.008 min
Response: 330106
Conc: 25.52 ng/ml