

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100622\
Data File : FB028549.D
Signal(s) : FID2B.CH
Acq On : 6 Oct 2022 20:09
Operator : AJ/MA
Sample : N5014-17 50X
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
COMP-2

Integration File: Calibration.e
Quant Time: Oct 07 06:26:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	307509	23.769 ng/ml
Target Compounds			
4) t Benzene	7.950	18720	0.852 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100622\
Data File : FB028549.D
Signal(s) : FID2B.CH
Acq On : 6 Oct 2022 20:09
Operator : AJ/MA
Sample : N5014-17 50X
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
COMP-2

Integration File: Calibration.e
Quant Time: Oct 07 06:26:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

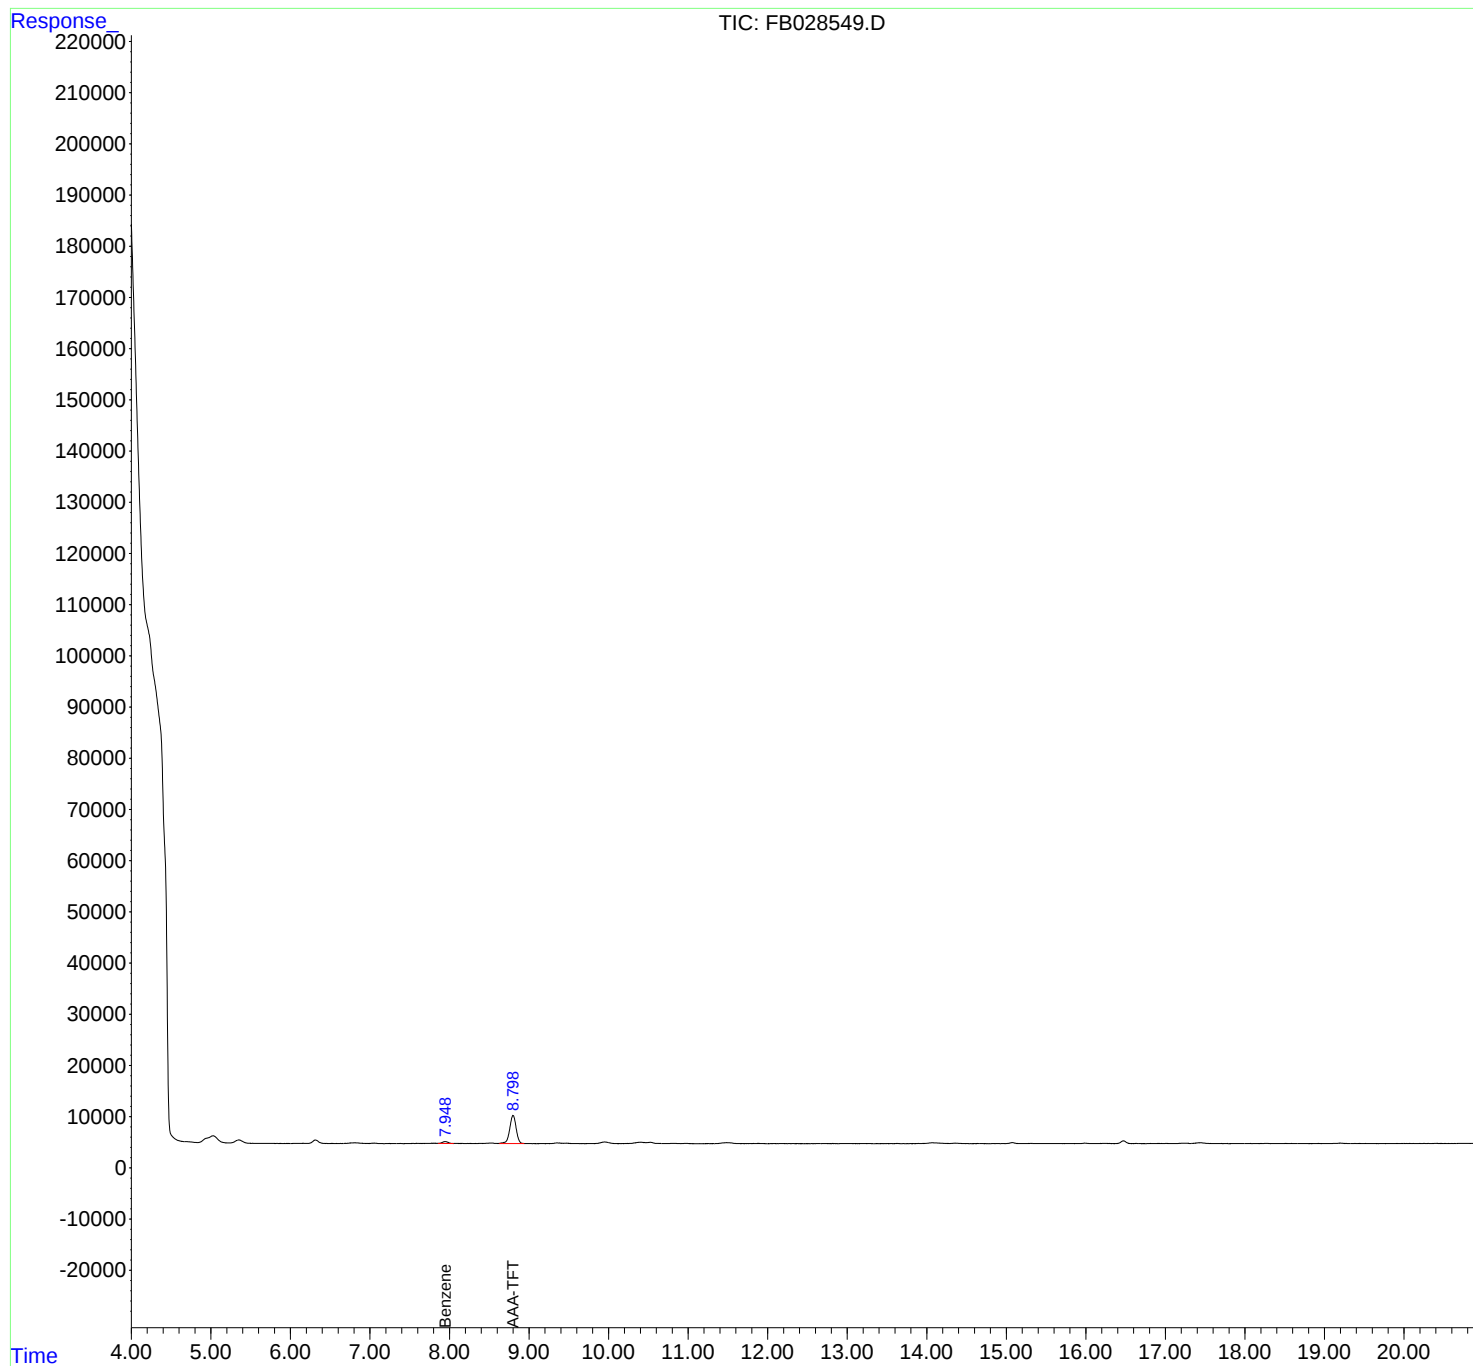


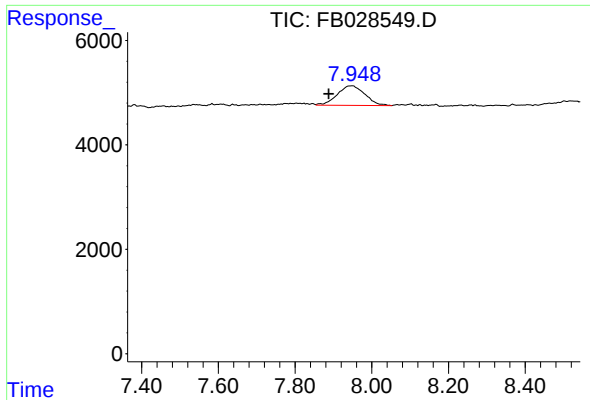

#4 Benzene

R.T.: 7.950 min
Delta R.T.: 0.062 min
Response: 18720
Conc: 0.85 ng/ml

Instrument :
FID_B
ClientSampleId :
COMP-2

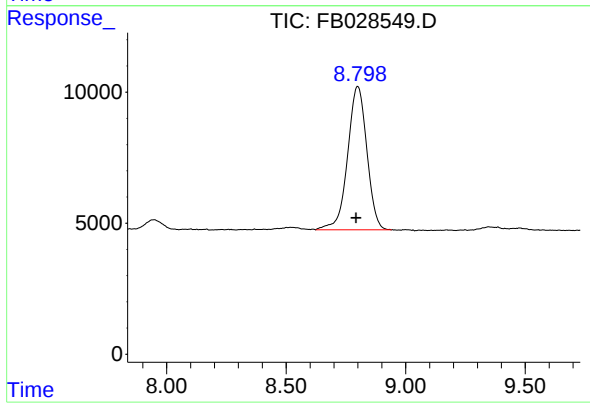

#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.007 min
Response: 307509
Conc: 23.77 ng/ml