

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100622\
 Data File : FB028550.D
 Signal(s) : FID2B.CH
 Acq On : 6 Oct 2022 20:57
 Operator : AJ/MA
 Sample : BSF1006S2
 Misc : 5.10G/5.00 ML DI WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 07 06:26:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	292503	22.610 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.723	511397	31.261 ng/ml
2) t 2,2,4-Trimethylpentane	7.439	609595	33.731 ng/ml
3) t n-Heptane	7.760	187359	11.061 ng/ml
4) t Benzene	7.898	255441	11.630 ng/ml
6) t Toluene	10.631	742382	35.419 ng/ml
7) t Ethylbenzene	13.068	229777	11.578 ng/ml
8) t m-Xylene	13.201	452349	22.961 ng/ml
9) t O-Xylene	13.928	439204	22.576 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	410252	21.192 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100622\
Data File : FB028550.D
Signal(s) : FID2B.CH
Acq On : 6 Oct 2022 20:57
Operator : AJ/MA
Sample : BSF1006S2
Misc : 5.10G/5.00 ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 07 06:26:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

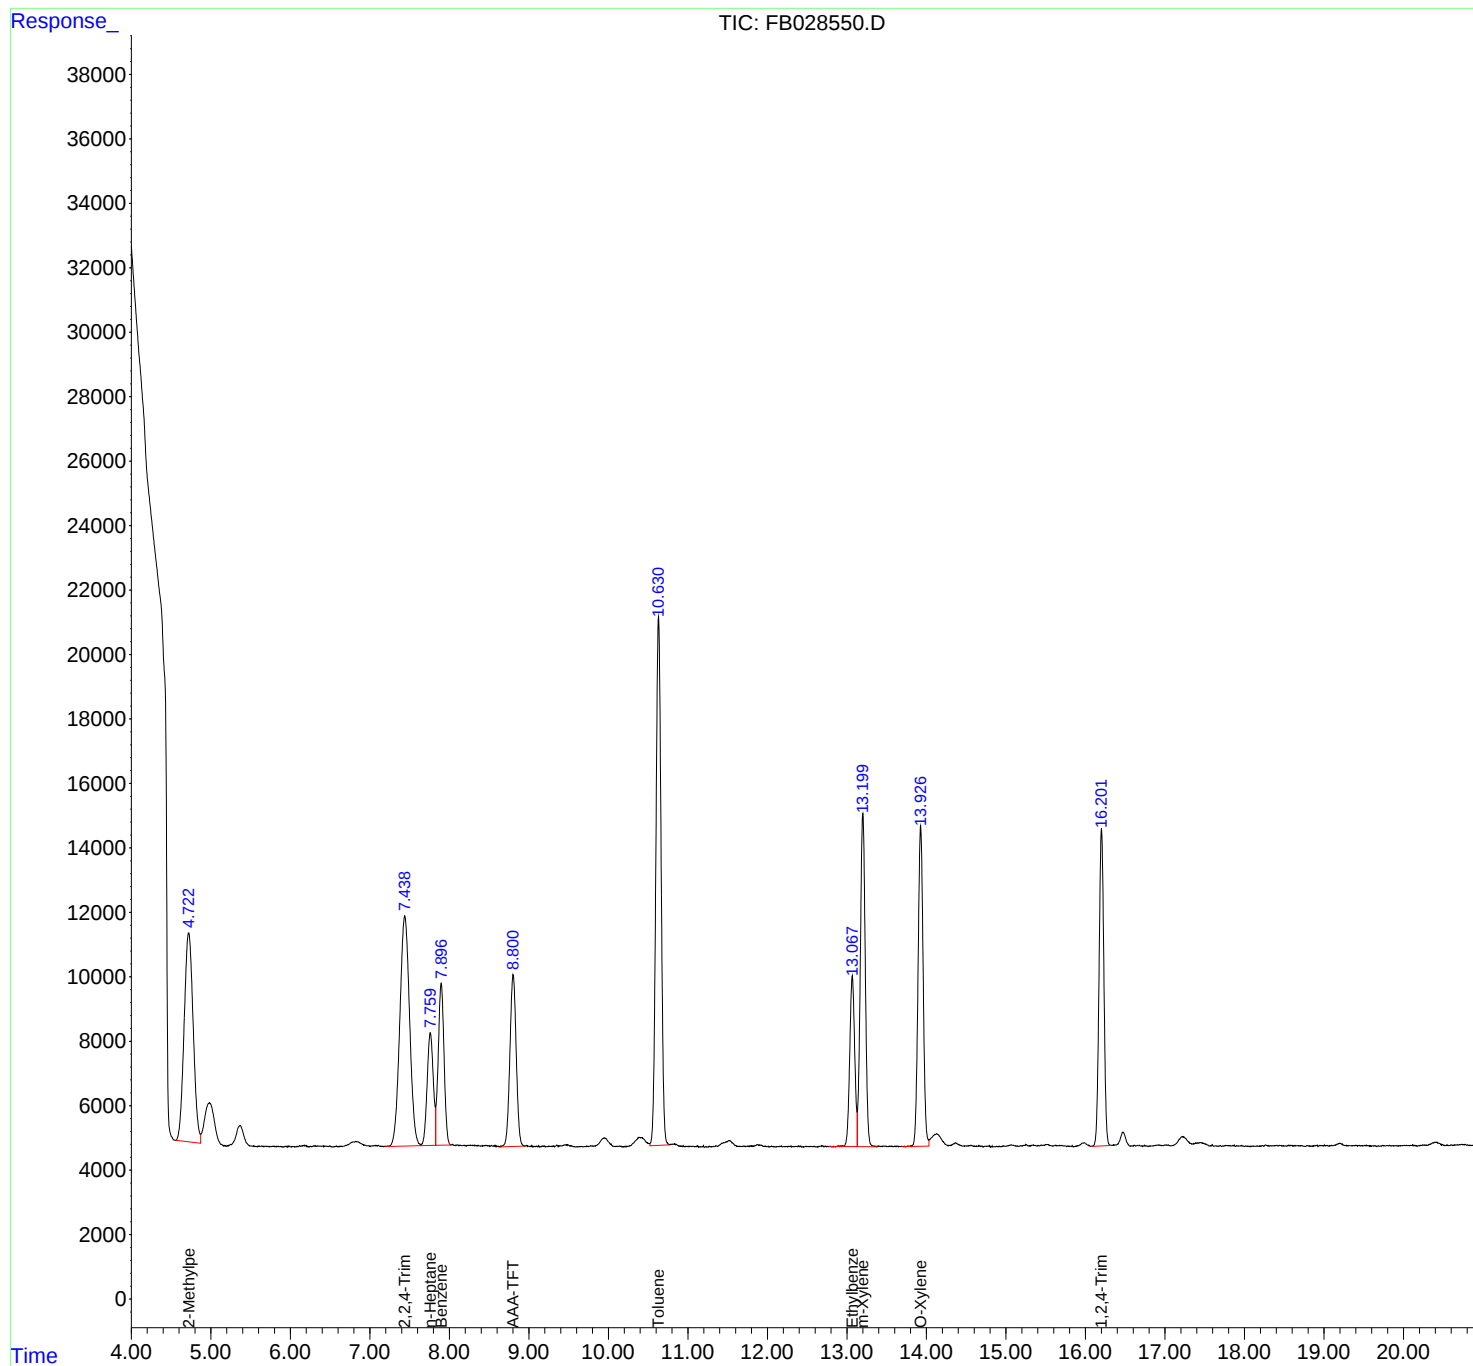


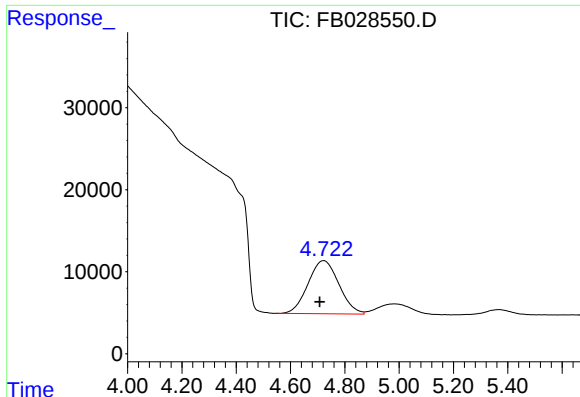

#1 2-Methylpentane


R.T.: 4.723 min
Delta R.T.: 0.015 min
Response: 511397
Conc: 31.26 ng/ml

Instrument :
FID_B
ClientSampleId :

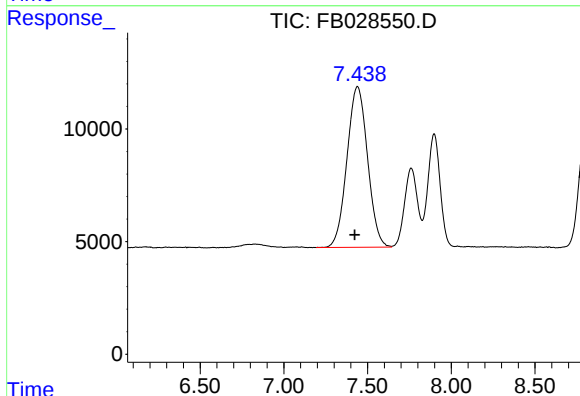


#2 2,2,4-Trimethylpentane

R.T.: 7.439 min
Delta R.T.: 0.016 min
Response: 609595
Conc: 33.73 ng/ml

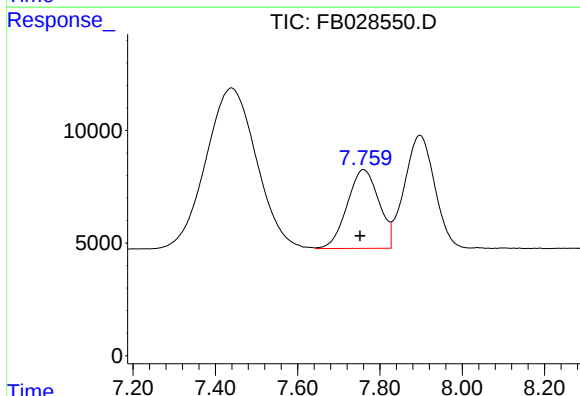


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.009 min
Response: 187359
Conc: 11.06 ng/ml

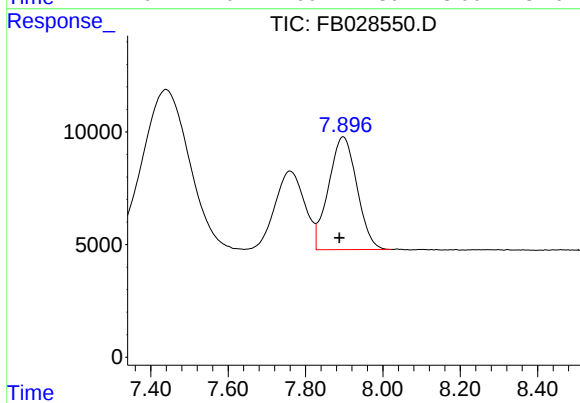

#4 Benzene


R.T.: 7.898 min
Delta R.T.: 0.010 min
Response: 255441
Conc: 11.63 ng/ml

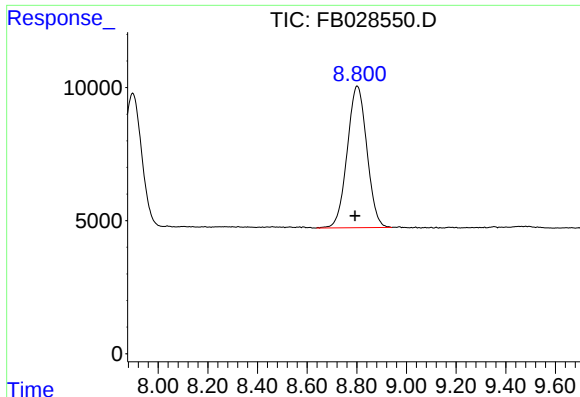

#5 AAA-TFT


R.T.: 8.802 min
Delta R.T.: 0.010 min
Response: 292503
Conc: 22.61 ng/ml

Instrument :
FID_B
ClientSampleId :

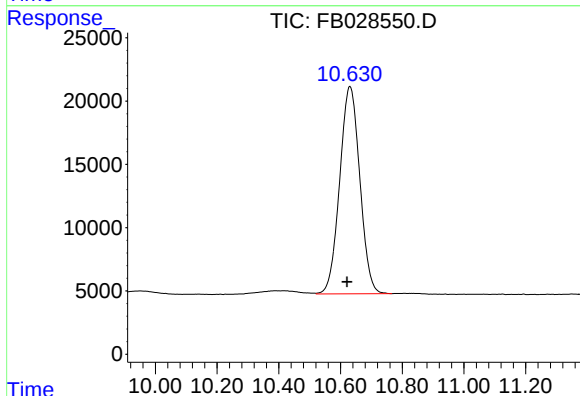


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.010 min
Response: 742382
Conc: 35.42 ng/ml

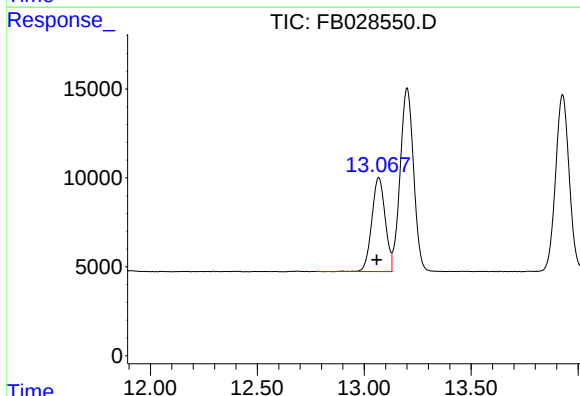


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: 0.010 min
Response: 229777
Conc: 11.58 ng/ml

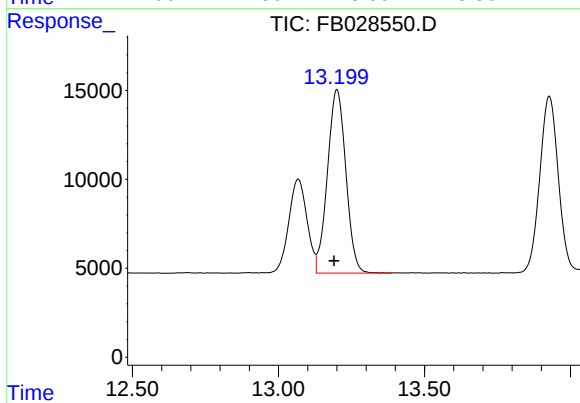

#8 m-Xylene


R.T.: 13.201 min
Delta R.T.: 0.010 min
Response: 452349
Conc: 22.96 ng/ml

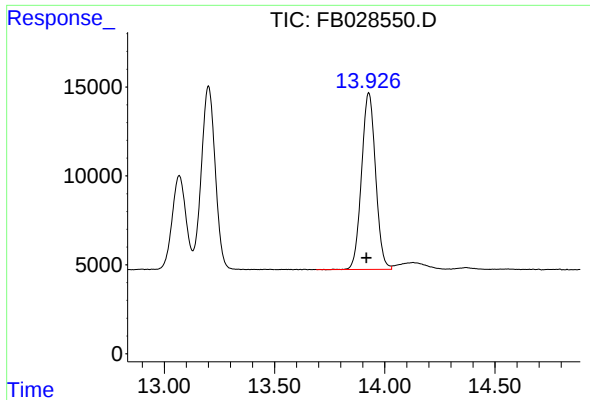

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: 0.010 min
Response: 439204
Conc: 22.58 ng/ml

Instrument :
FID_B
ClientSampleId :

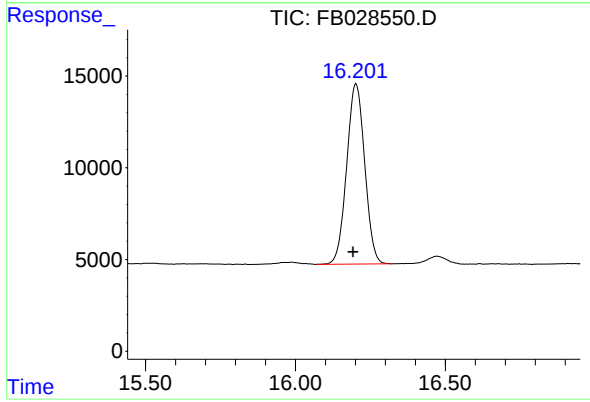

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: 0.010 min
Response: 410252
Conc: 21.19 ng/ml