

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB100622\  
 Data File : FB028550.D  
 Signal(s) : FID2B.CH  
 Acq On : 6 Oct 2022 20:57  
 Operator : AJ/MA  
 Sample : BSF1006S2  
 Misc : 5.10G/5.00 ML DI WATER  
 ALS Vial : 17 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :  
 BSF1006S2

Integration File: Calibration.e  
 Quant Time: Oct 07 06:26:48 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB100522.M  
 Quant Title :  
 QLast Update : Wed Oct 05 12:47:25 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.802  | 292503   | 22.610 ng/ml |
| Target Compounds             |        |          |              |
| 1) t 2-Methylpentane         | 4.723  | 511397   | 31.261 ng/ml |
| 2) t 2,2,4-Trimethylpentane  | 7.439  | 609595   | 33.731 ng/ml |
| 3) t n-Heptane               | 7.760  | 187359   | 11.061 ng/ml |
| 4) t Benzene                 | 7.898  | 255441   | 11.630 ng/ml |
| 6) t Toluene                 | 10.631 | 742382   | 35.419 ng/ml |
| 7) t Ethylbenzene            | 13.068 | 229777   | 11.578 ng/ml |
| 8) t m-Xylene                | 13.201 | 452349   | 22.961 ng/ml |
| 9) t O-Xylene                | 13.928 | 439204   | 22.576 ng/ml |
| 10) t 1,2,4-Trimethylbenzene | 16.202 | 410252   | 21.192 ng/ml |
| -----                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB100622\  
Data File : FB028550.D  
Signal(s) : FID2B.CH  
Acq On : 6 Oct 2022 20:57  
Operator : AJ/MA  
Sample : BSF1006S2  
Misc : 5.10G/5.00 ML DI WATER  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
BSF1006S2

Integration File: Calibration.e  
Quant Time: Oct 07 06:26:48 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB100522.M  
Quant Title :  
QLast Update : Wed Oct 05 12:47:25 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

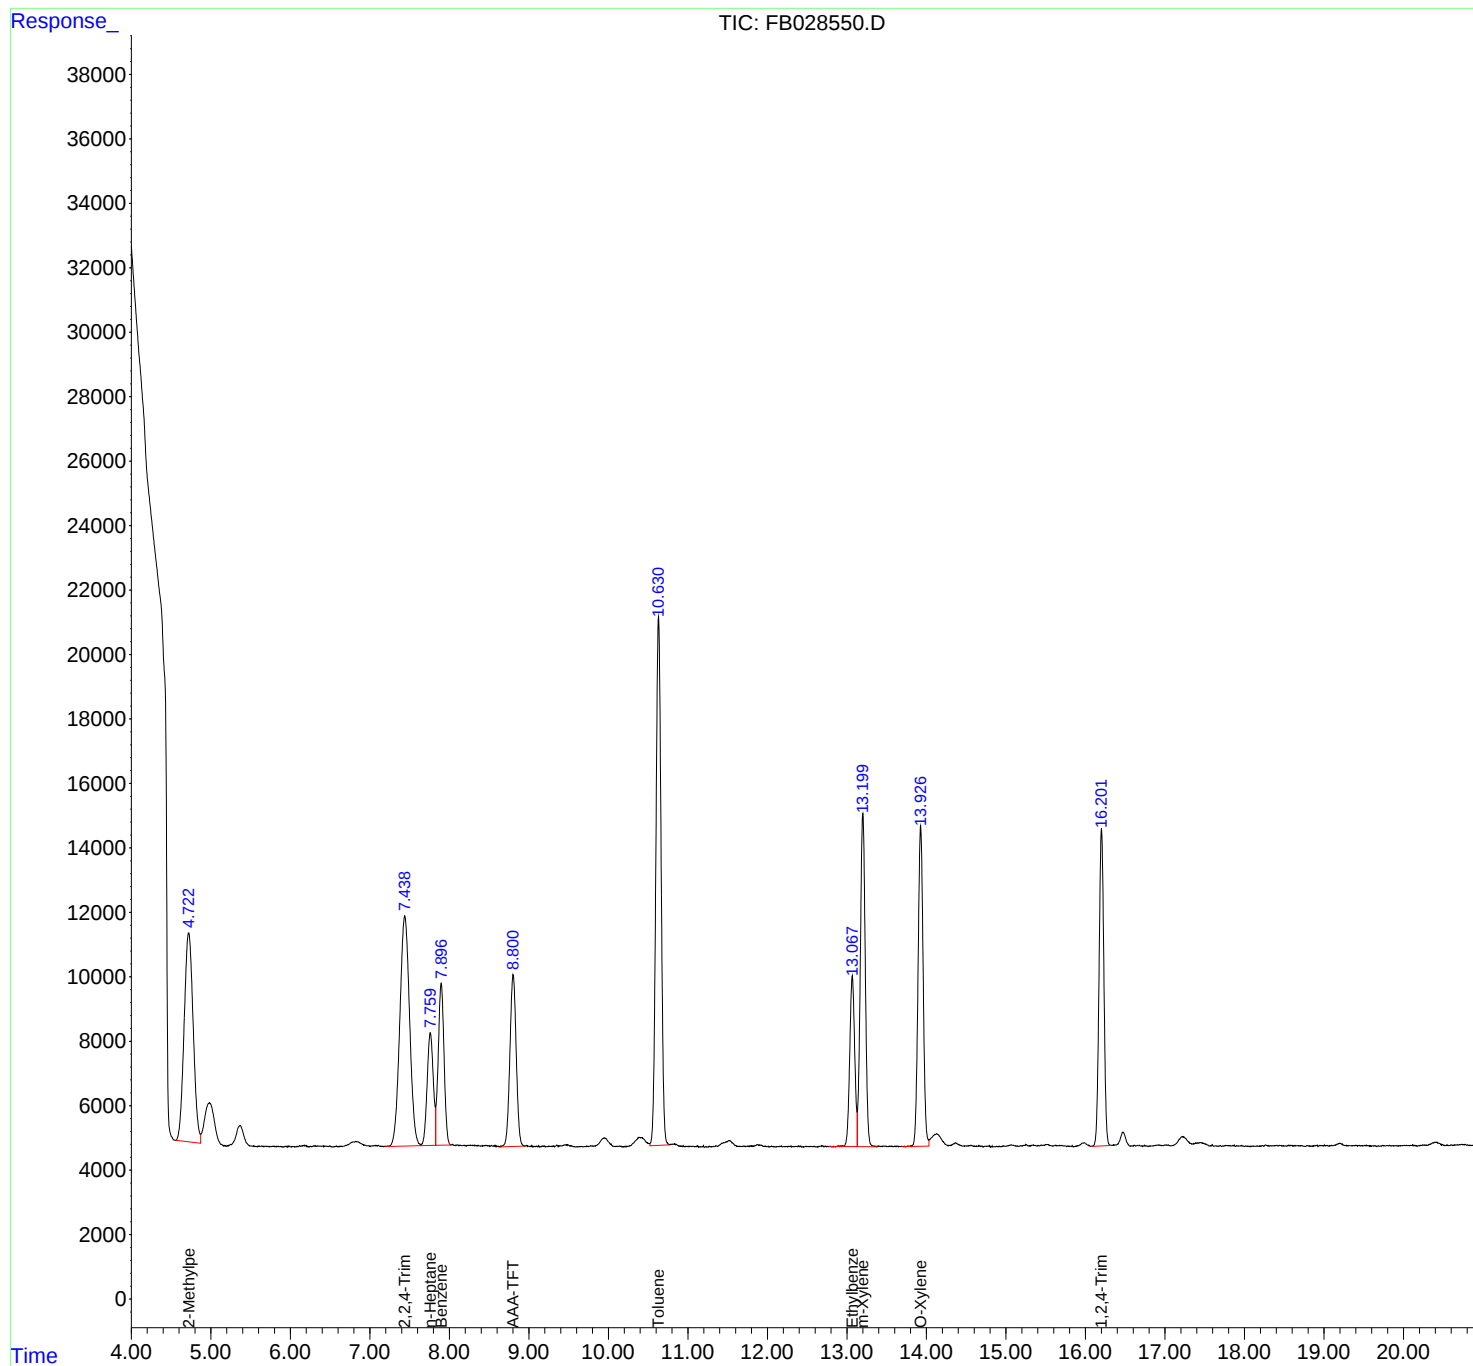


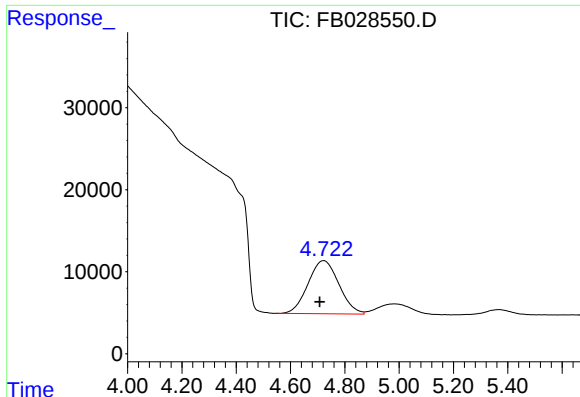

#1 2-Methylpentane


R.T.: 4.723 min  
Delta R.T.: 0.015 min  
Response: 511397  
Conc: 31.26 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
BSF1006S2

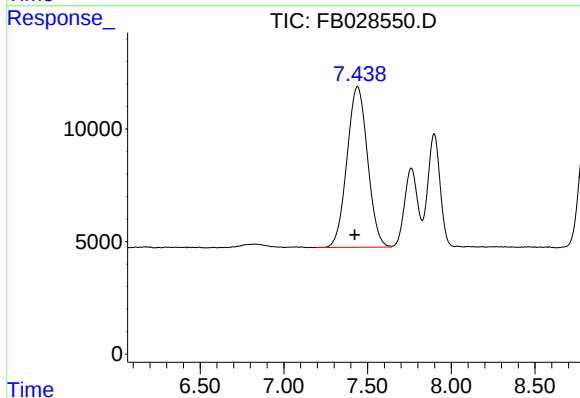


#2 2,2,4-Trimethylpentane

R.T.: 7.439 min  
Delta R.T.: 0.016 min  
Response: 609595  
Conc: 33.73 ng/ml

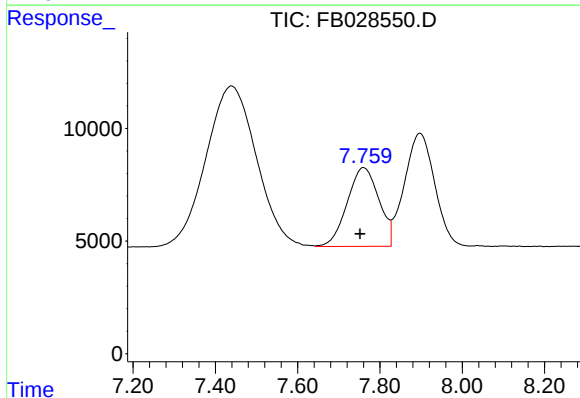


#3 n-Heptane

R.T.: 7.760 min  
Delta R.T.: 0.009 min  
Response: 187359  
Conc: 11.06 ng/ml

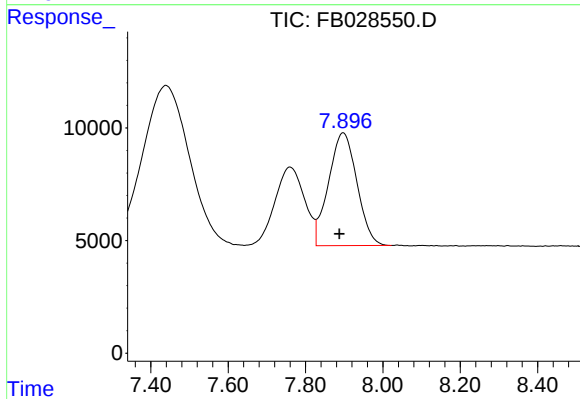

#4 Benzene


R.T.: 7.898 min  
Delta R.T.: 0.010 min  
Response: 255441  
Conc: 11.63 ng/ml

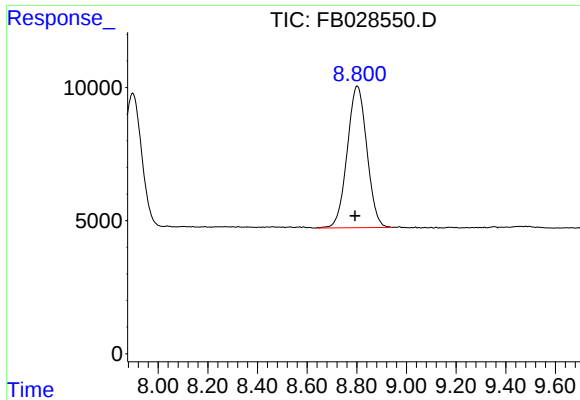

#5 AAA-TFT


R.T.: 8.802 min  
Delta R.T.: 0.010 min  
Response: 292503  
Conc: 22.61 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
BSF1006S2

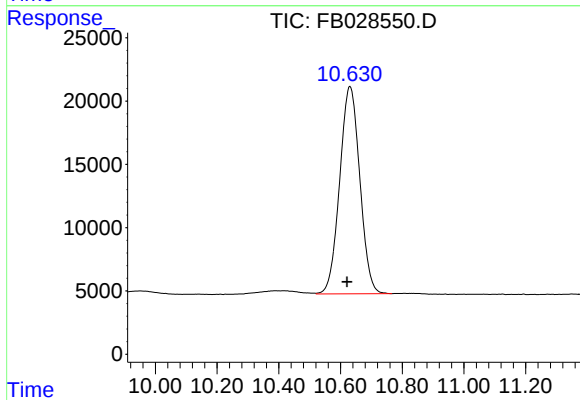


#6 Toluene

R.T.: 10.631 min  
Delta R.T.: 0.010 min  
Response: 742382  
Conc: 35.42 ng/ml

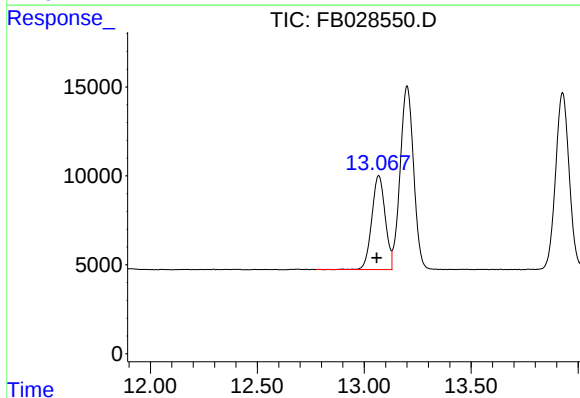


#7 Ethylbenzene

R.T.: 13.068 min  
Delta R.T.: 0.010 min  
Response: 229777  
Conc: 11.58 ng/ml

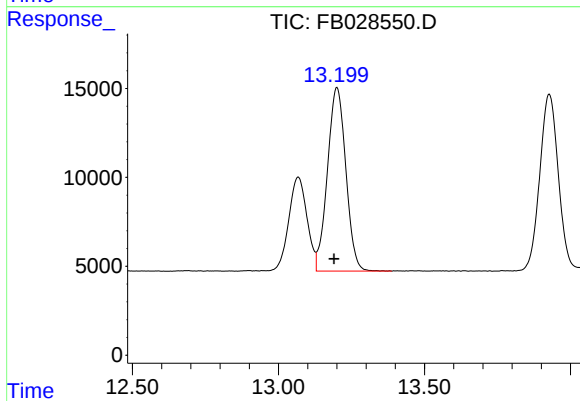

#8 m-Xylene


R.T.: 13.201 min  
Delta R.T.: 0.010 min  
Response: 452349  
Conc: 22.96 ng/ml

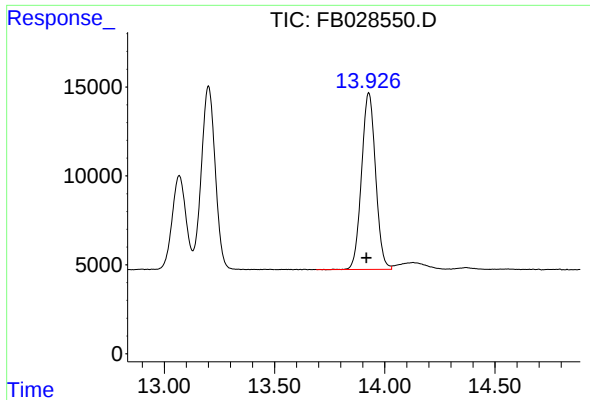

#9 O-Xylene

R.T.: 13.928 min  
Delta R.T.: 0.010 min  
Response: 439204  
Conc: 22.58 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
BSF1006S2

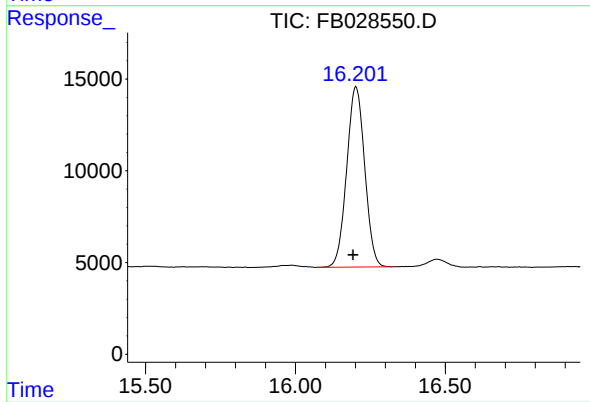

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min  
Delta R.T.: 0.010 min  
Response: 410252  
Conc: 21.19 ng/ml