

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100720\
 Data File : FB025029.D
 Signal(s) : FID2B.CH
 Acq On : 7 Oct 2020 16:15
 Operator : DD/AJ
 Sample : L4224-02MS
 Misc : 5.04/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 08 01:18:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.803	400108	19.058 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	664716	22.103 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	605469	19.810 ng/ml
3) t n-Heptane	7.761	158917	5.224 ng/ml
4) t Benzene	7.895	338747	9.093 ng/ml
6) t Toluene	10.633	876361	25.104 ng/ml
7) t Ethylbenzene	13.073	292279	9.017 ng/ml
8) t m-Xylene	13.206	486470	15.314 ng/ml
9) t O-Xylene	13.934	505472	16.634 ng/ml
10) t 1,2,4-Trimethylbenzene	16.212	359842	14.188 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100720\
Data File : FB025029.D
Signal(s) : FID2B.CH
Acq On : 7 Oct 2020 16:15
Operator : DD/AJ
Sample : L4224-02MS
Misc : 5.04/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 08 01:18:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

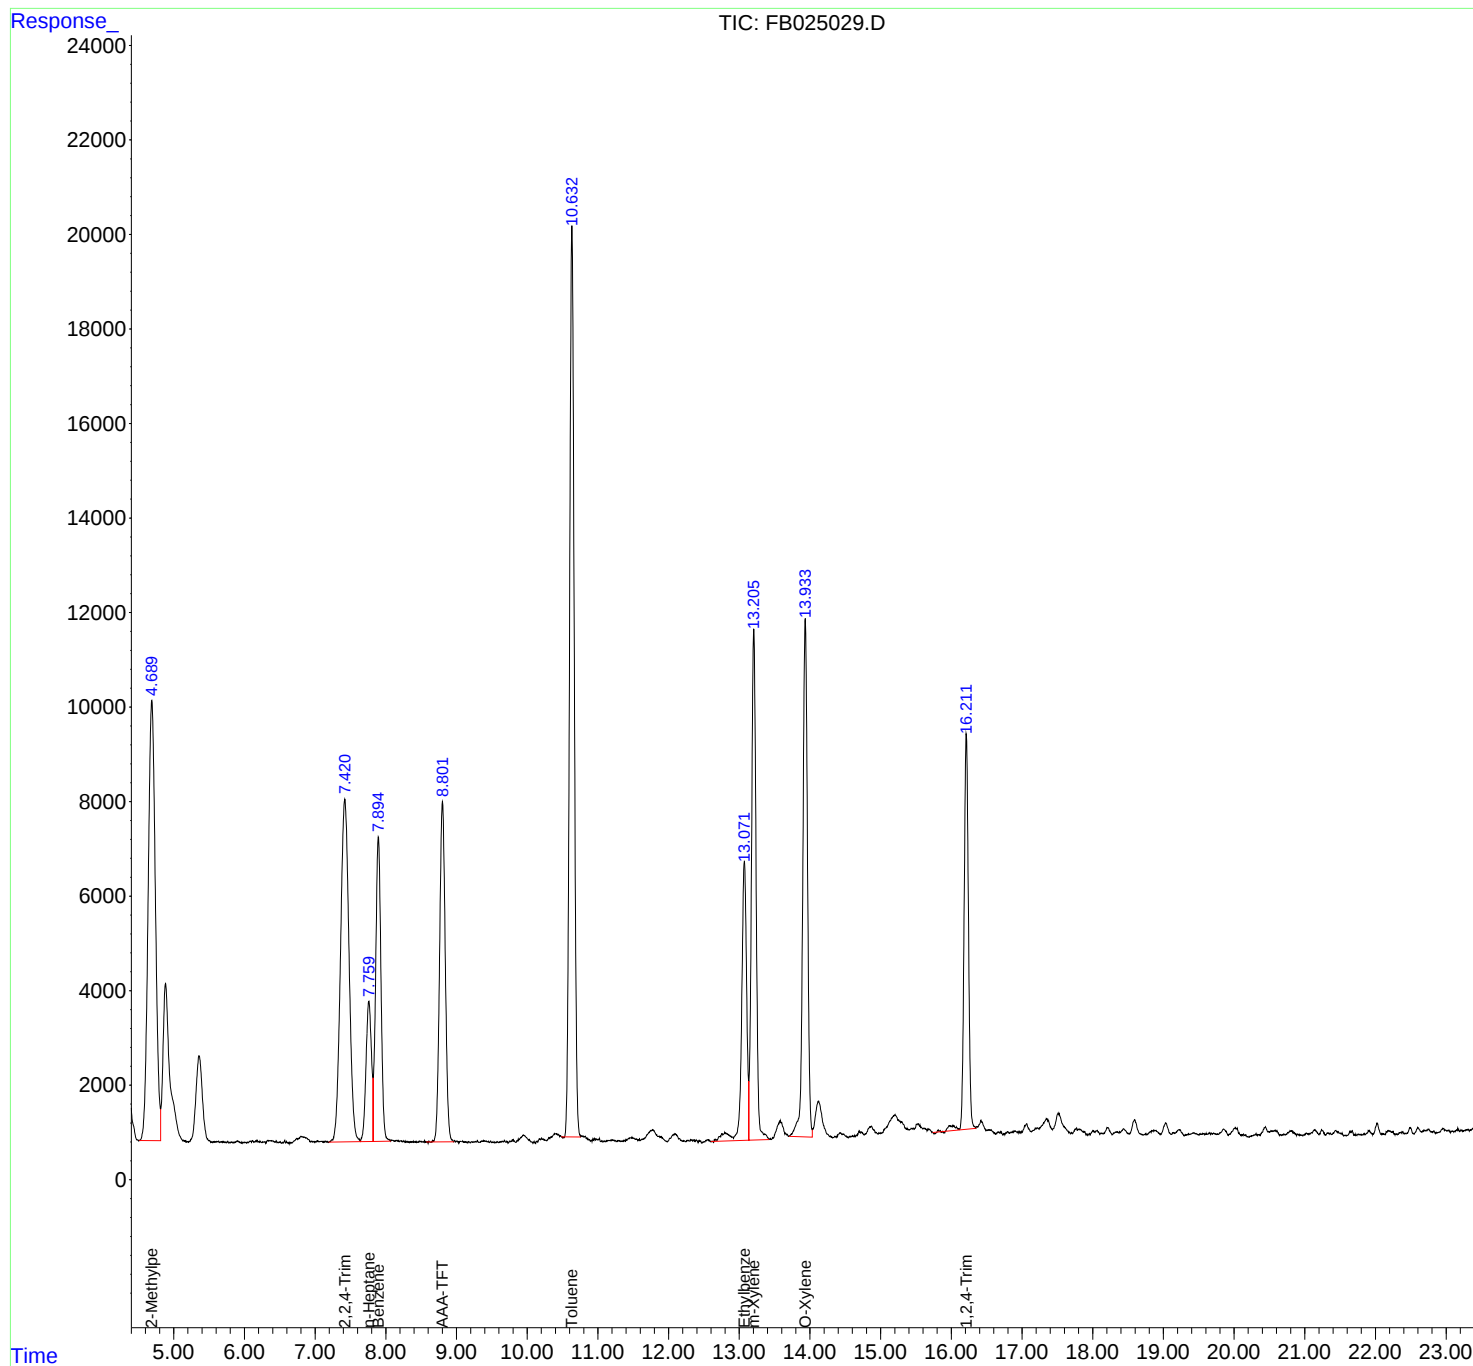

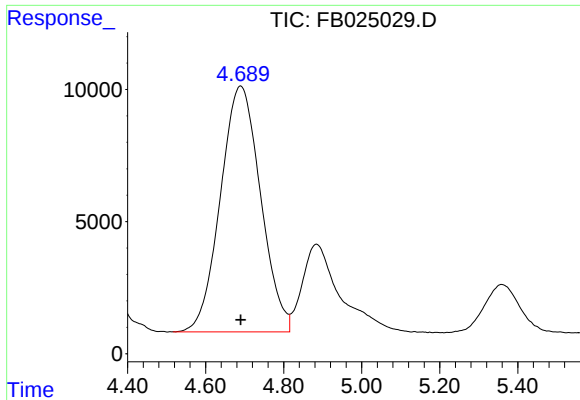


#1 2-Methylpentane

R.T.: 4.691 min
Delta R.T.: 0.000 min
Response: 664716
Conc: 22.10 ng/ml

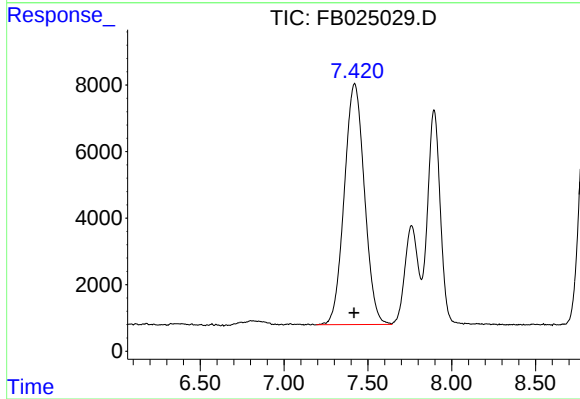


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: 0.003 min
Response: 605469
Conc: 19.81 ng/ml

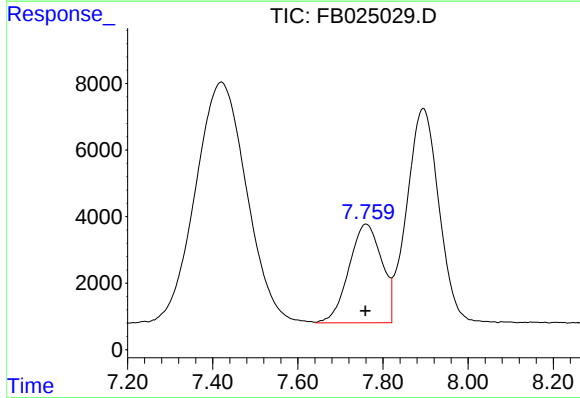


#3 n-Heptane

R.T.: 7.761 min
Delta R.T.: 0.001 min
Response: 158917
Conc: 5.22 ng/ml

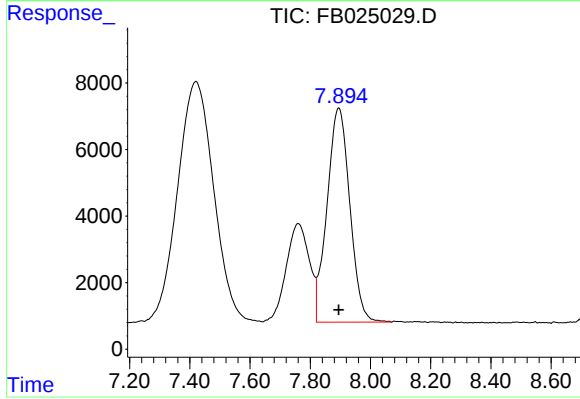


#4 Benzene

R.T.: 7.895 min
Delta R.T.: 0.000 min
Response: 338747
Conc: 9.09 ng/ml

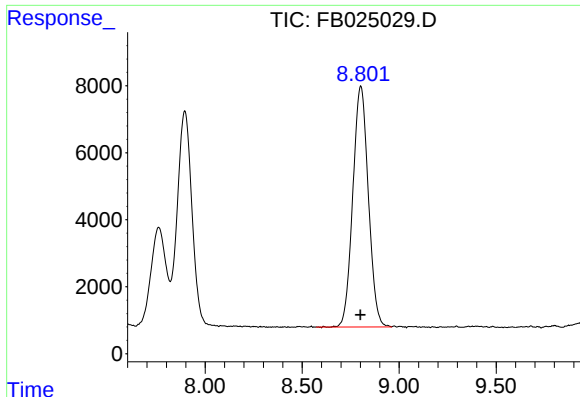


#5 AAA-TFT

R.T.: 8.803 min
Delta R.T.: 0.002 min
Response: 400108
Conc: 19.06 ng/ml

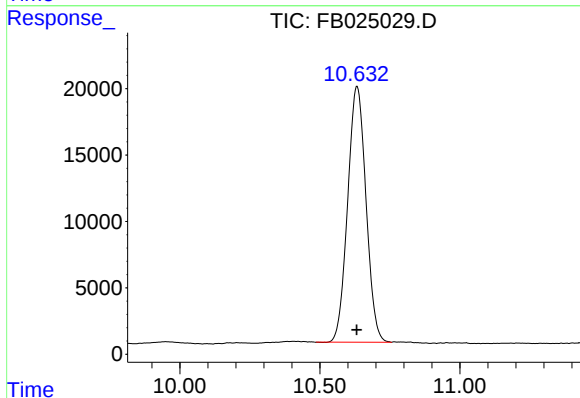


#6 Toluene

R.T.: 10.633 min
Delta R.T.: 0.002 min
Response: 876361
Conc: 25.10 ng/ml

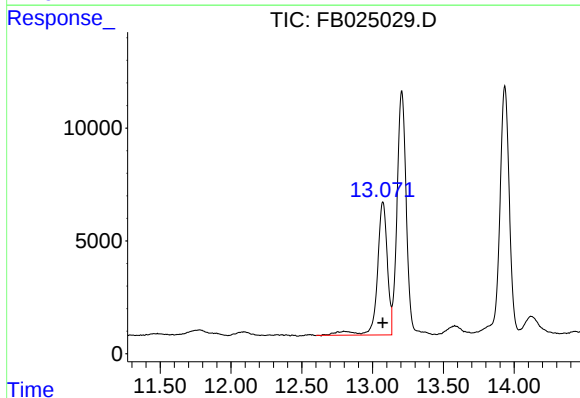


#7 Ethylbenzene

R.T.: 13.073 min
Delta R.T.: 0.002 min
Response: 292279
Conc: 9.02 ng/ml

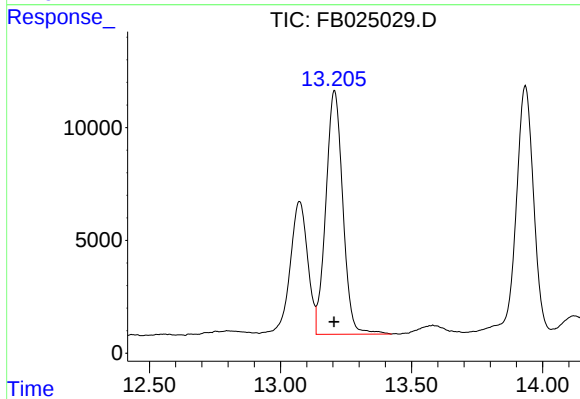


#8 m-Xylene

R.T.: 13.206 min
Delta R.T.: 0.002 min
Response: 486470
Conc: 15.31 ng/ml

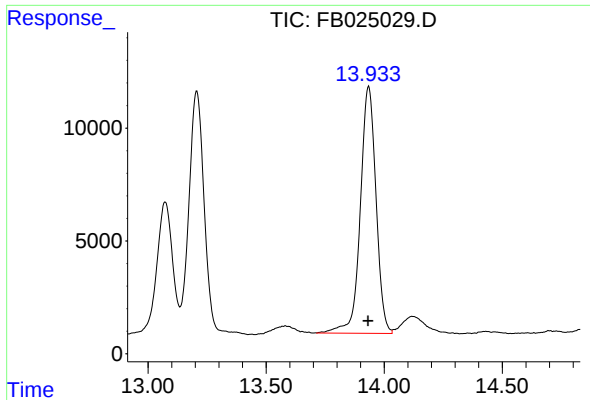

#9 O-Xylene

R.T.: 13.934 min
Delta R.T.: 0.002 min
Response: 505472
Conc: 16.63 ng/ml

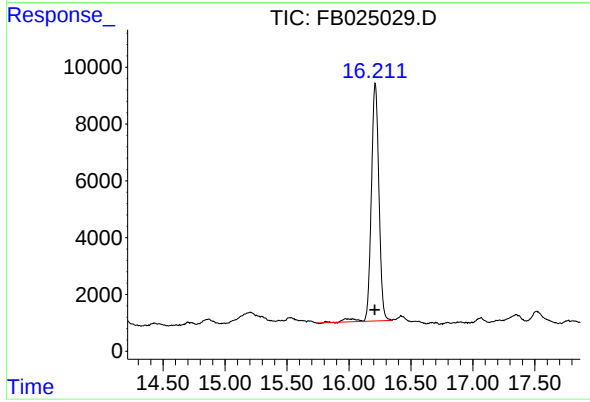

#10 1,2,4-Trimethylbenzene

R.T.: 16.212 min
Delta R.T.: 0.003 min
Response: 359842
Conc: 14.19 ng/ml