

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100722\
 Data File : FB028556.D
 Signal(s) : FID2B.CH
 Acq On : 7 Oct 2022 12:06
 Operator : AJ/MA
 Sample : BSF1007S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1007S1

Integration File: Calibration.e
 Quant Time: Oct 08 21:54:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	288777	22.321 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	417111	25.497 ng/ml
2) t 2,2,4-Trimethylpentane	7.434	530782	29.370 ng/ml
3) t n-Heptane	7.756	159452	9.414 ng/ml
4) t Benzene	7.892	224744	10.232 ng/ml
6) t Toluene	10.626	634212	30.258 ng/ml
7) t Ethylbenzene	13.063	200386	10.097 ng/ml
8) t m-Xylene	13.195	396379	20.120 ng/ml
9) t O-Xylene	13.922	389318	20.012 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	367479	18.982 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100722\
Data File : FB028556.D
Signal(s) : FID2B.CH
Acq On : 7 Oct 2022 12:06
Operator : AJ/MA
Sample : BSF1007S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1007S1

Integration File: Calibration.e
Quant Time: Oct 08 21:54:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

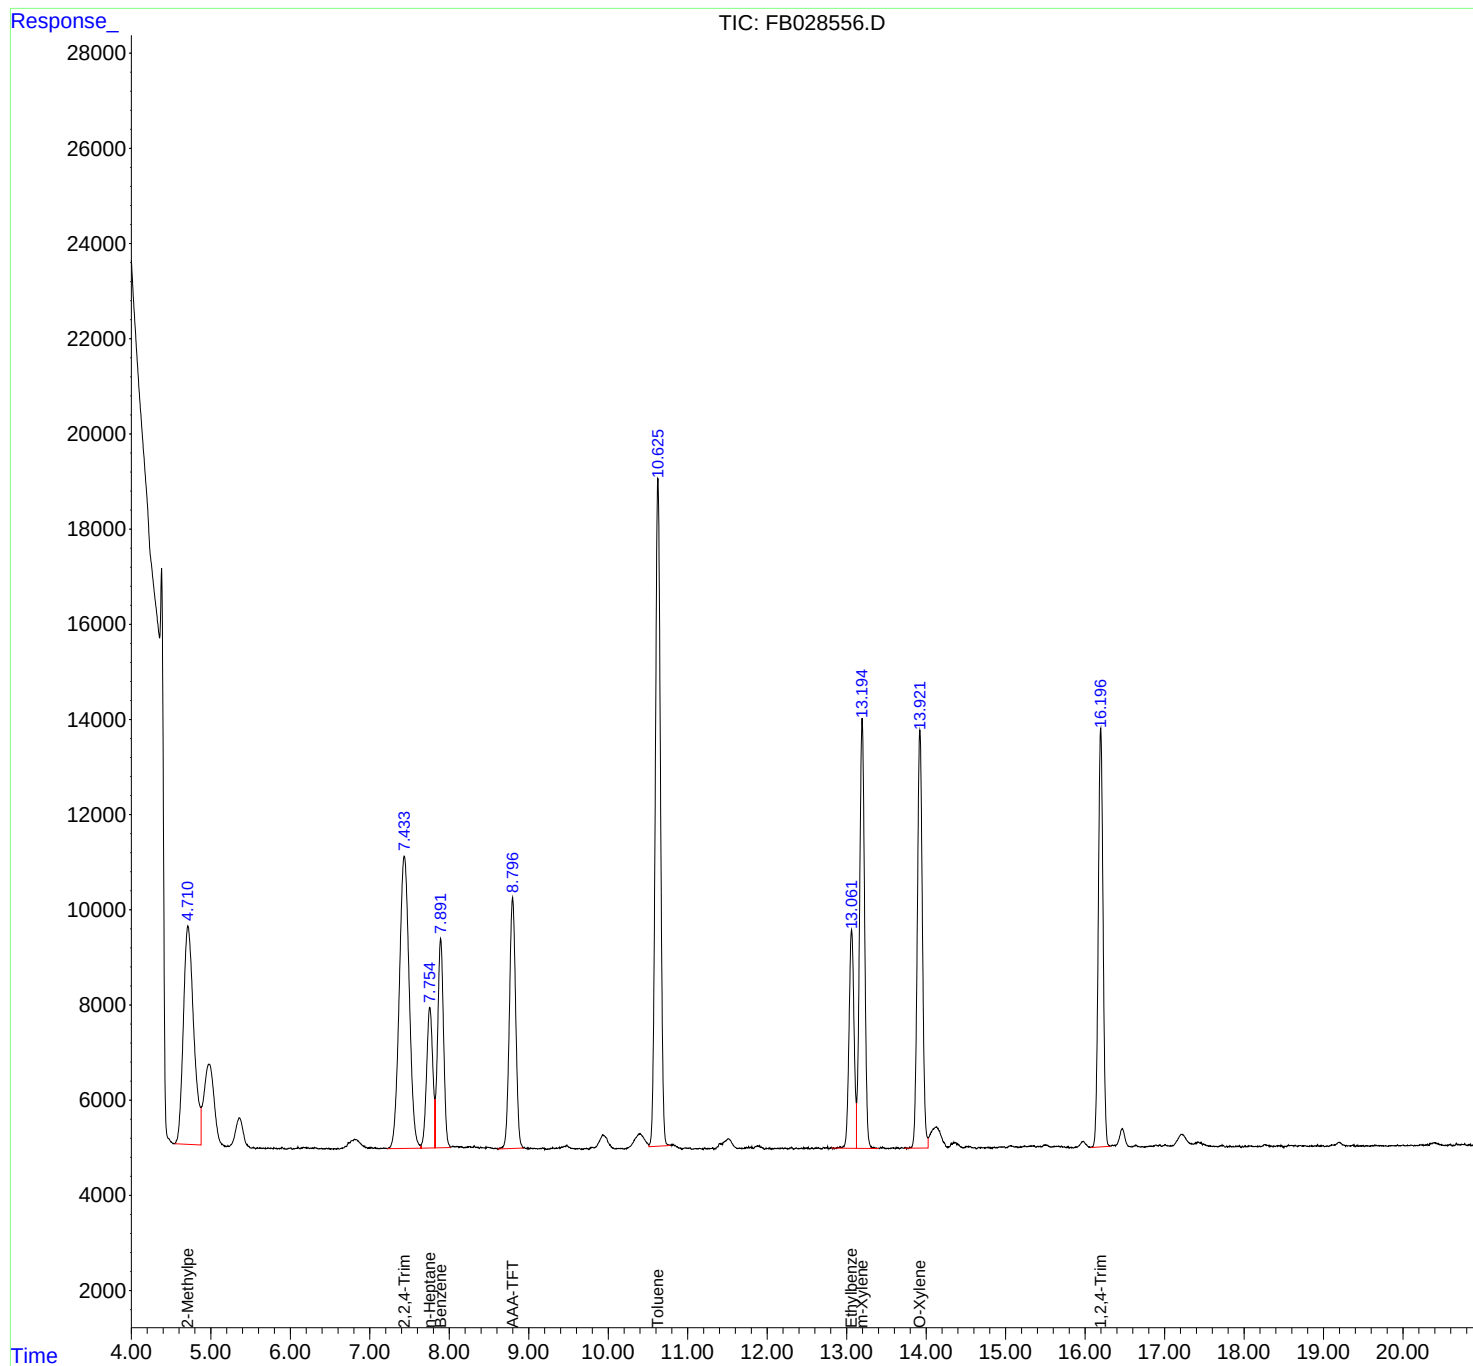


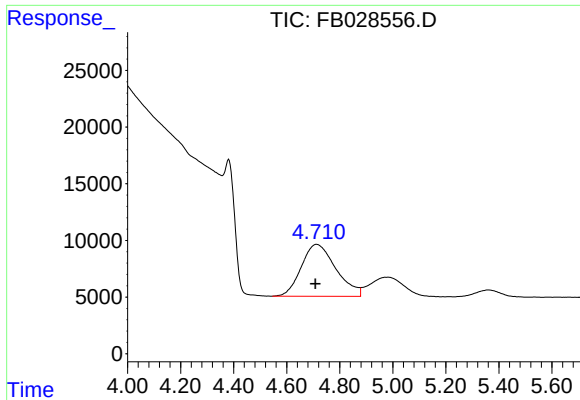

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: 0.004 min
Response: 417111
Conc: 25.50 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1007S1

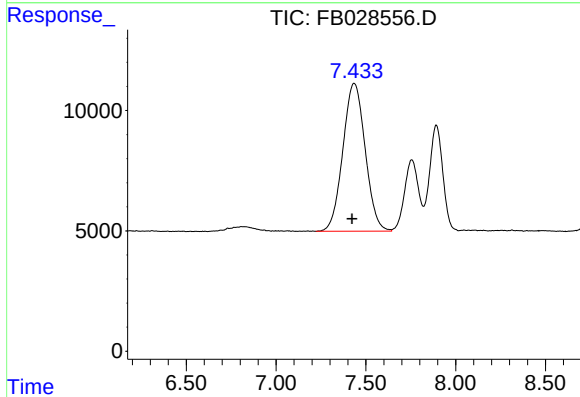


#2 2,2,4-Trimethylpentane

R.T.: 7.434 min
Delta R.T.: 0.011 min
Response: 530782
Conc: 29.37 ng/ml

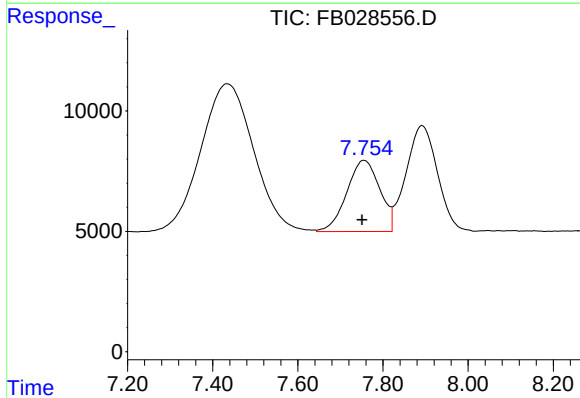


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.004 min
Response: 159452
Conc: 9.41 ng/ml

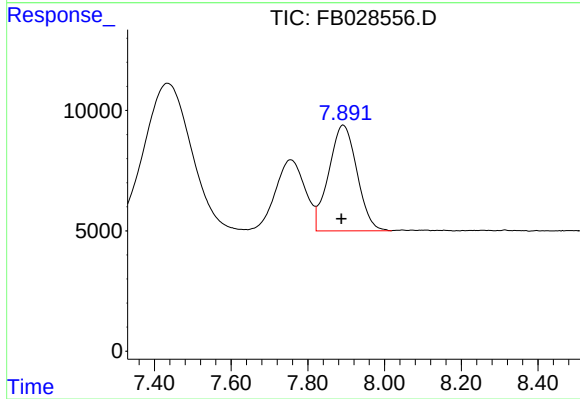

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.005 min
Response: 224744
Conc: 10.23 ng/ml

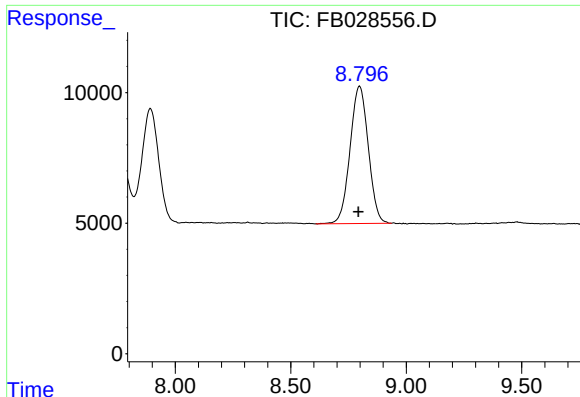

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: 0.005 min
Response: 288777
Conc: 22.32 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1007S1

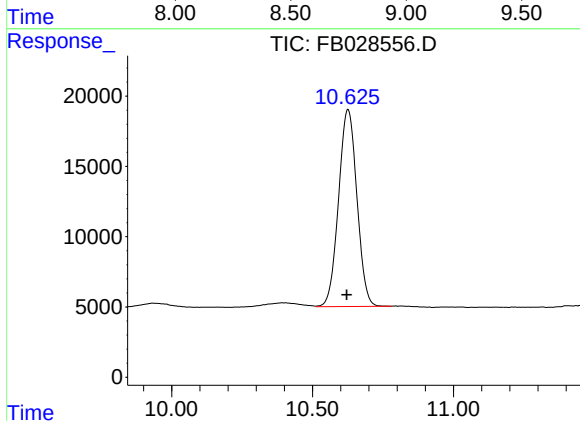


#6 Toluene

R.T.: 10.626 min
Delta R.T.: 0.005 min
Response: 634212
Conc: 30.26 ng/ml

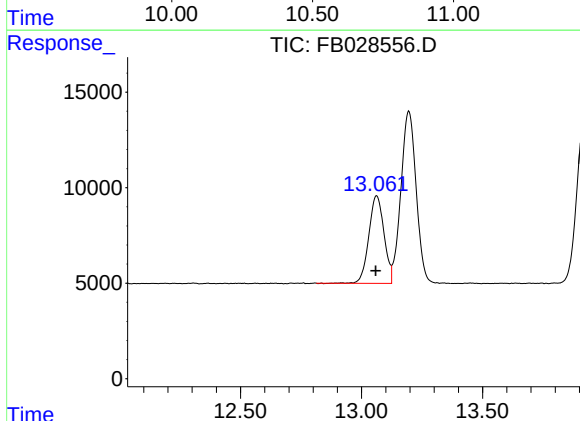


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: 0.005 min
Response: 200386
Conc: 10.10 ng/ml

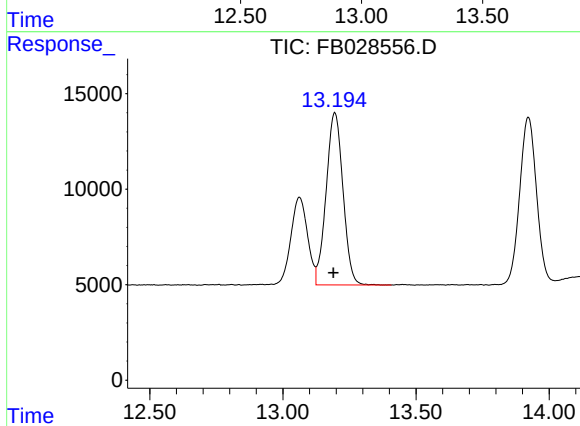

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: 0.005 min
Response: 396379
Conc: 20.12 ng/ml

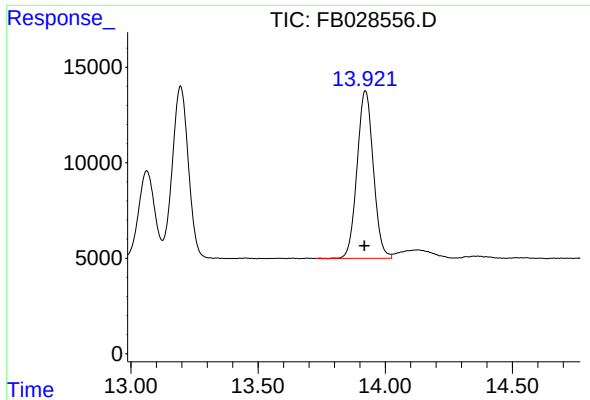

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.005 min
Response: 389318
Conc: 20.01 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1007S1

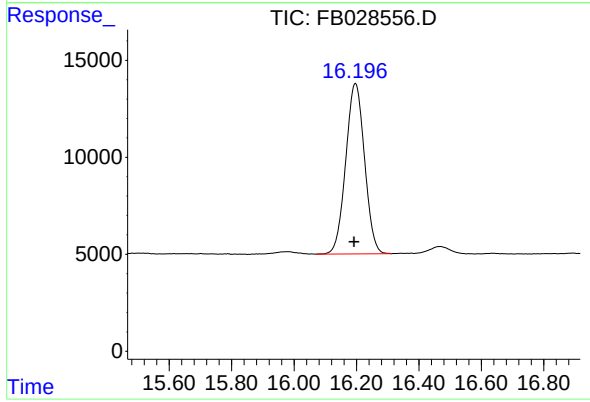

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: 0.005 min
Response: 367479
Conc: 18.98 ng/ml