

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100820\
 Data File : FB025034.D
 Signal(s) : FID2B.CH
 Acq On : 8 Oct 2020 9:40
 Operator : DD/AJ
 Sample : BSF1008S1
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 09 00:41:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	430266	20.495 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	843830	28.059 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	923414	30.213 ng/ml
3) t n-Heptane	7.758	301277	9.903 ng/ml
4) t Benzene	7.893	361962	9.717 ng/ml
6) t Toluene	10.631	1012315	28.998 ng/ml
7) t Ethylbenzene	13.071	310706	9.585 ng/ml
8) t m-Xylene	13.203	615875	19.388 ng/ml
9) t O-Xylene	13.931	591990	19.481 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	482443	19.022 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100820\
Data File : FB025034.D
Signal(s) : FID2B.CH
Acq On : 8 Oct 2020 9:40
Operator : DD/AJ
Sample : BSF1008S1
Misc : 5.01/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 09 00:41:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

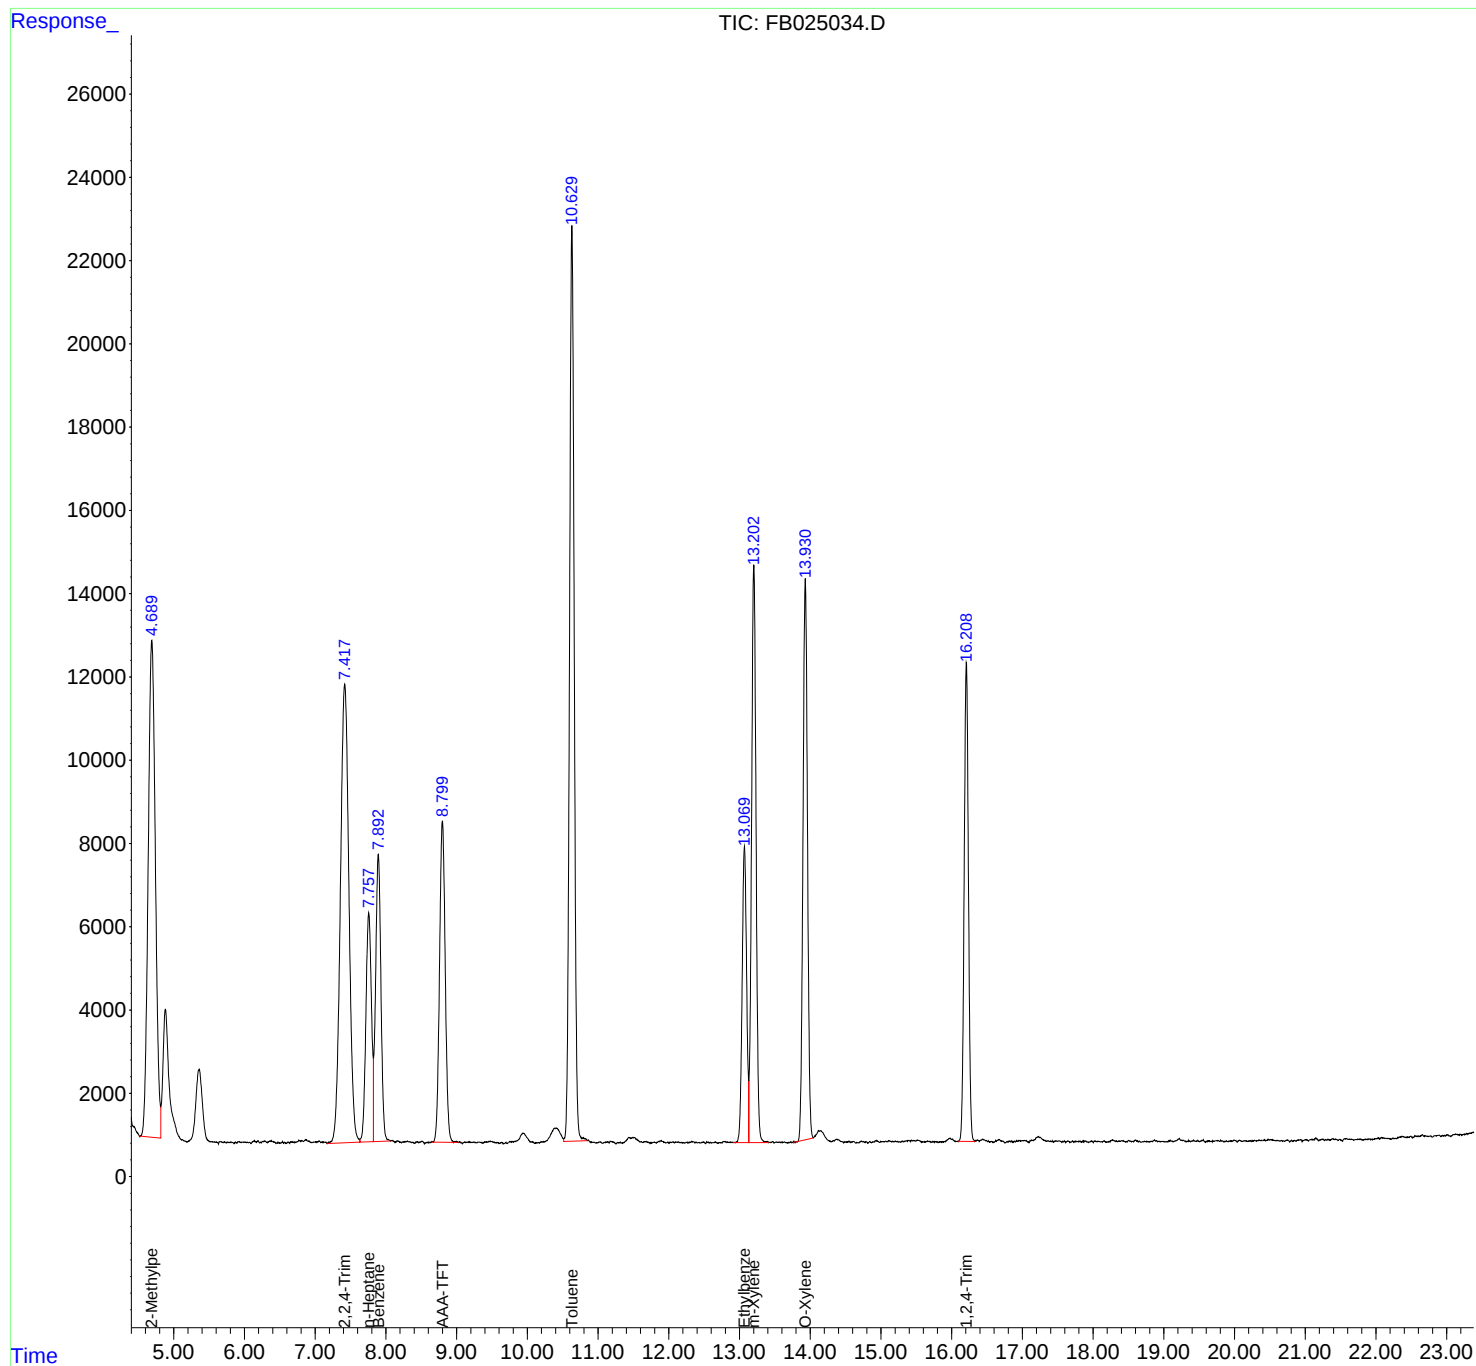

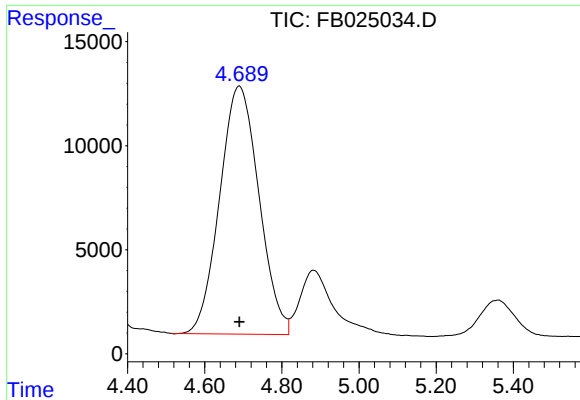


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: 0.000 min
Response: 843830
Conc: 28.06 ng/ml

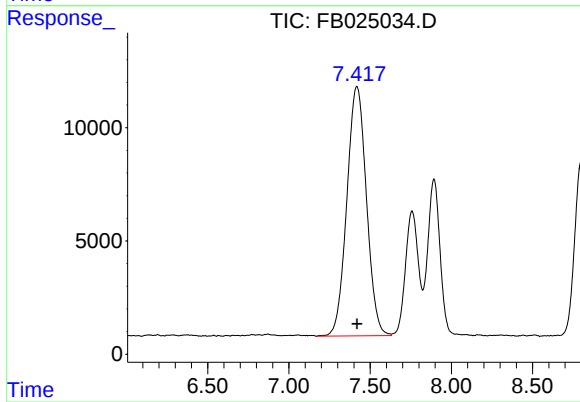


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 923414
Conc: 30.21 ng/ml

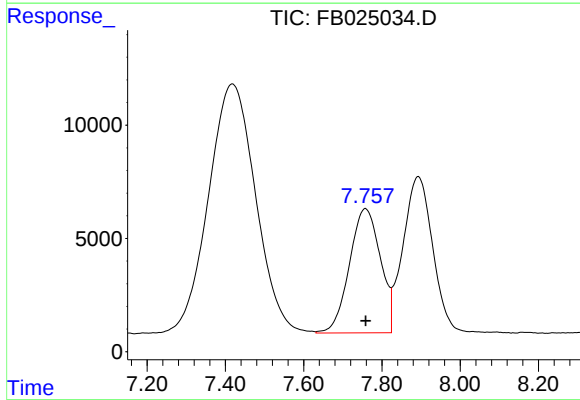


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: -0.001 min
Response: 301277
Conc: 9.90 ng/ml

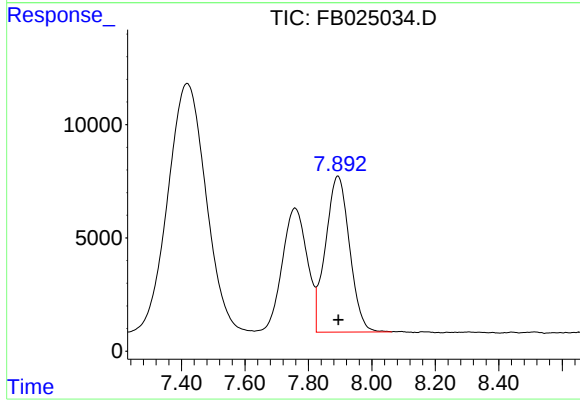


#4 Benzene

R.T.: 7.893 min
Delta R.T.: -0.002 min
Response: 361962
Conc: 9.72 ng/ml

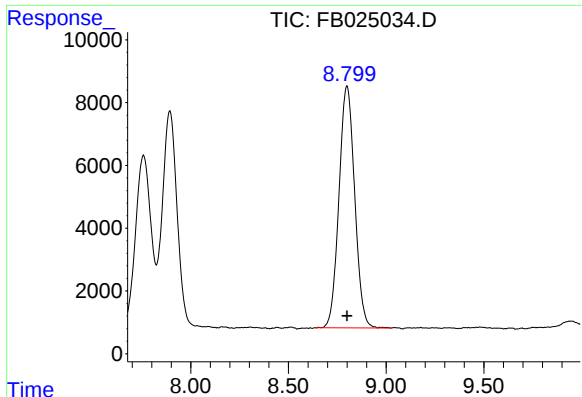


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 430266
Conc: 20.49 ng/ml

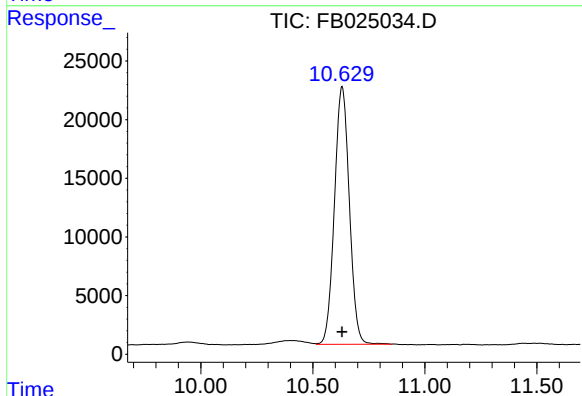


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 1012315
Conc: 29.00 ng/ml

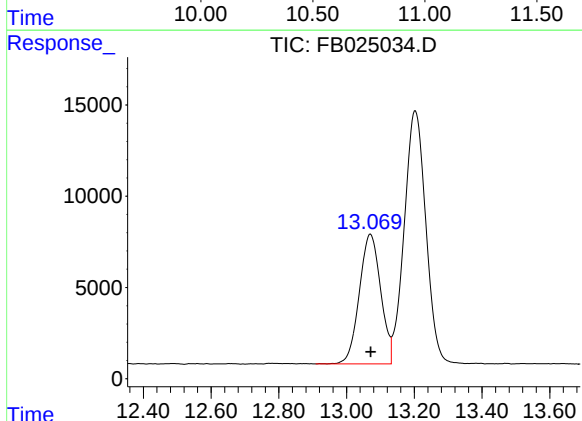


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 310706
Conc: 9.59 ng/ml

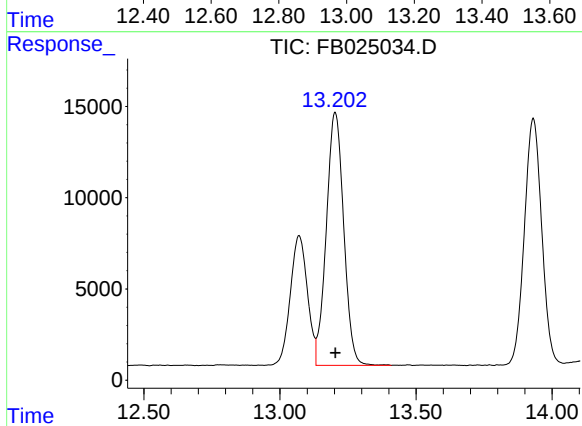


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 615875
Conc: 19.39 ng/ml

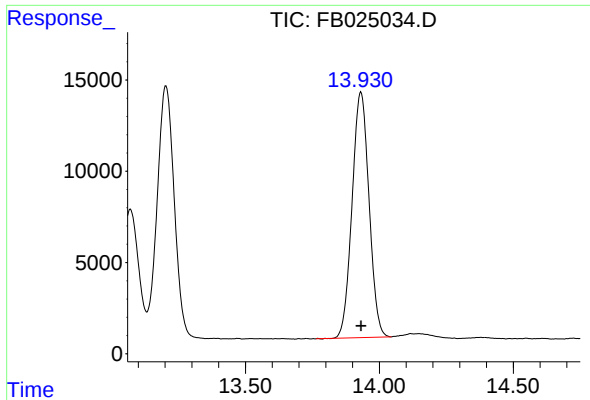

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 591990
Conc: 19.48 ng/ml

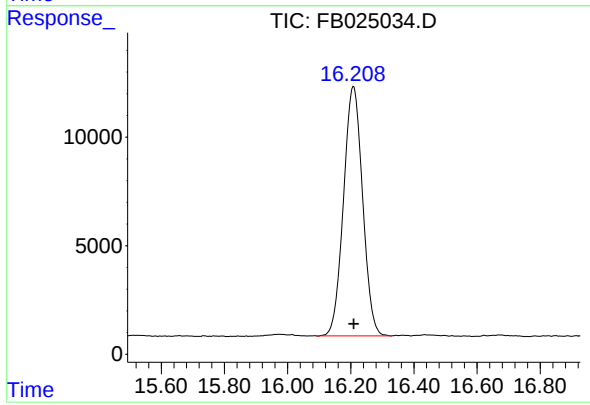

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 482443
Conc: 19.02 ng/ml