

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100821\
 Data File : FB026264.D
 Signal(s) : FID2B.CH
 Acq On : 8 Oct 2021 14:48
 Operator : AJ/MA
 Sample : FB100821GROICV
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 08 23:15:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100821.M
 Quant Title :
 QLast Update : Fri Oct 08 14:30:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.843	332779	22.082 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.847	579866	33.311 ng/ml
2) t 2,2,4-Trimethylpentane	7.500	670512	32.460 ng/ml
3) t n-Heptane	7.820	262479	11.203 ng/ml
4) t Benzene	7.957	286590	10.953 ng/ml
6) t Toluene	10.652	826546	31.904 ng/ml
7) t Ethylbenzene	13.071	239697	10.495 ng/ml
8) t m-Xylene	13.203	467563	20.844 ng/ml
9) t O-Xylene	13.927	433047	20.470 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	454323	19.524 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100821\
Data File : FB026264.D
Signal(s) : FID2B.CH
Acq On : 8 Oct 2021 14:48
Operator : AJ/MA
Sample : FB100821GROICV
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 08 23:15:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100821.M
Quant Title :
QLast Update : Fri Oct 08 14:30:36 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

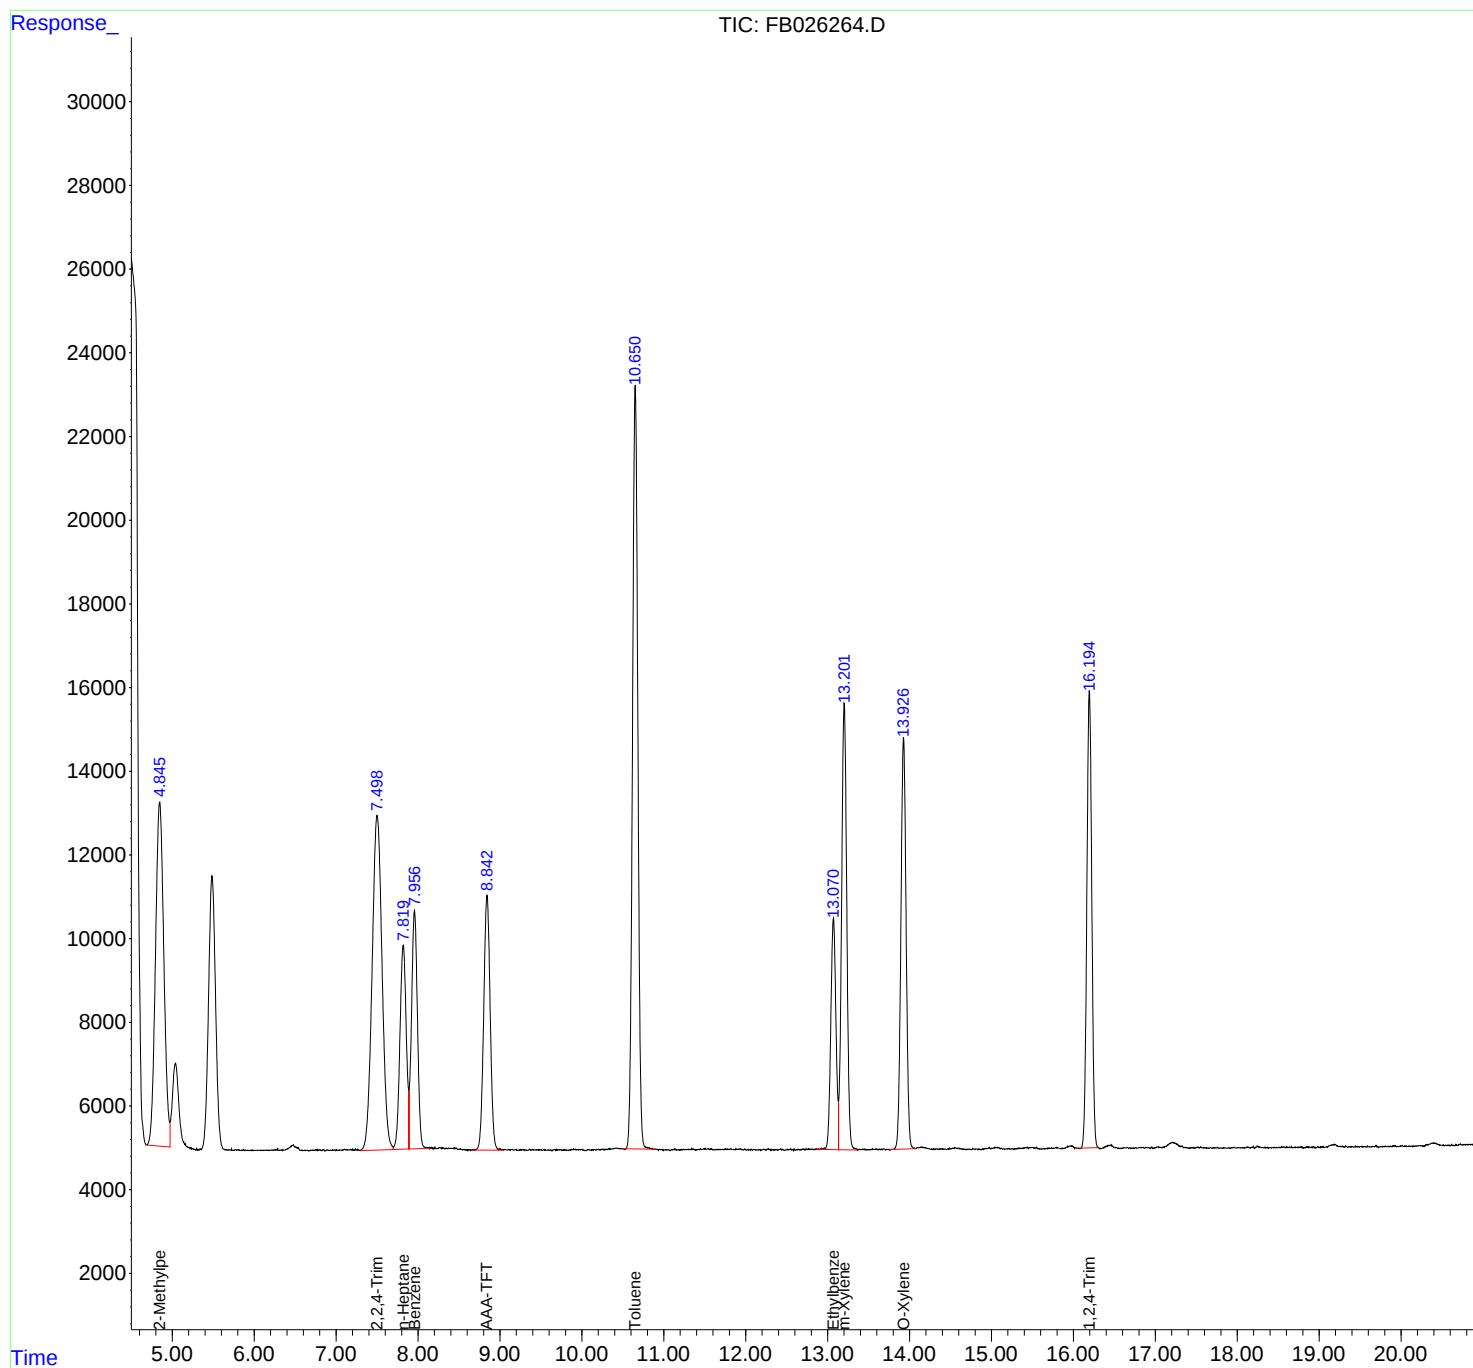


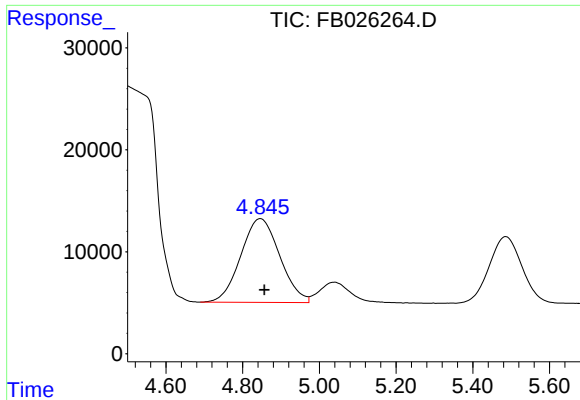

#1 2-Methylpentane


R.T.: 4.847 min
Delta R.T.: -0.010 min
Response: 579866
Conc: 33.31 ng/ml

Instrument :
FID_B
ClientSampleId :

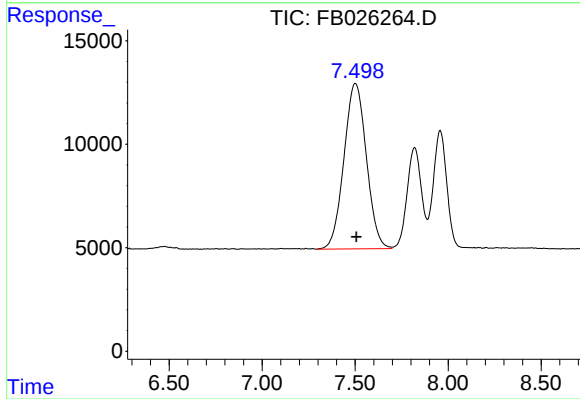


#2 2,2,4-Trimethylpentane

R.T.: 7.500 min
Delta R.T.: -0.006 min
Response: 670512
Conc: 32.46 ng/ml

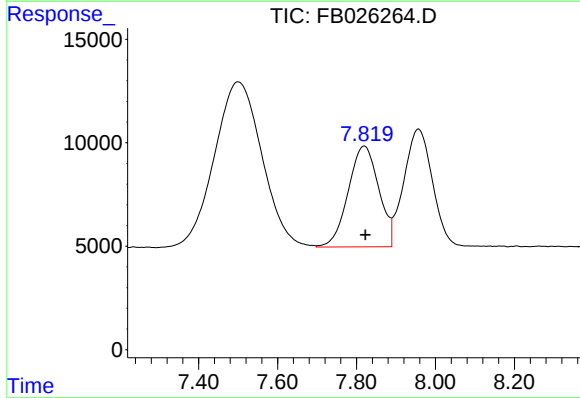


#3 n-Heptane

R.T.: 7.820 min
Delta R.T.: -0.003 min
Response: 262479
Conc: 11.20 ng/ml

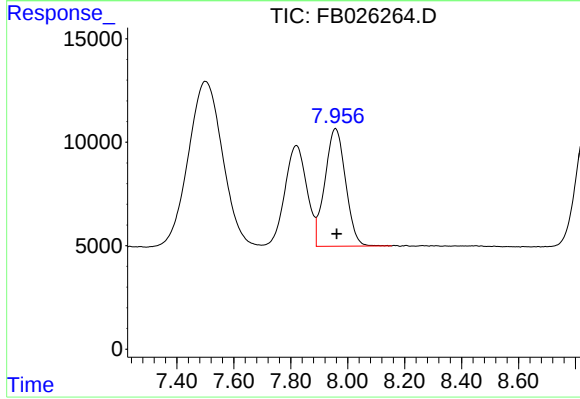

#4 Benzene


R.T.: 7.957 min
Delta R.T.: -0.004 min
Response: 286590
Conc: 10.95 ng/ml

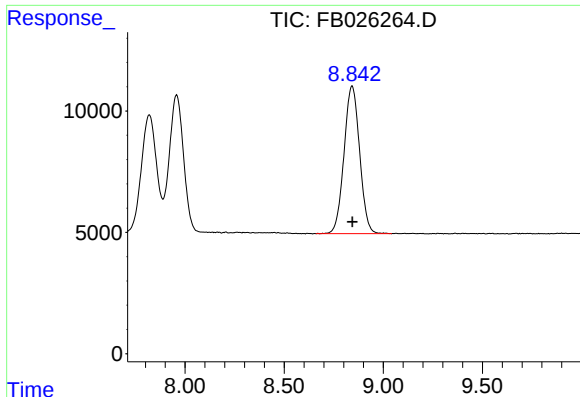

#5 AAA-TFT


R.T.: 8.843 min
Delta R.T.: -0.002 min
Response: 332779
Conc: 22.08 ng/ml

Instrument :
FID_B
ClientSampleId :

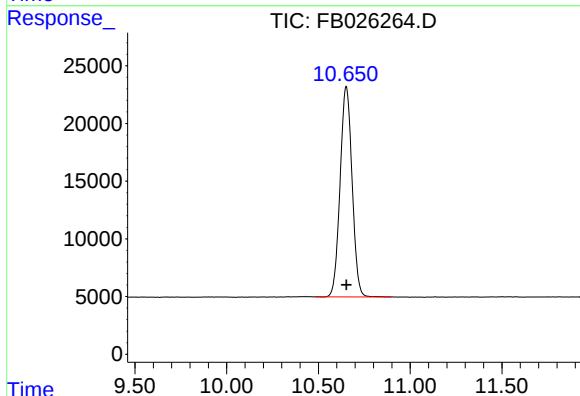


#6 Toluene

R.T.: 10.652 min
Delta R.T.: -0.001 min
Response: 826546
Conc: 31.90 ng/ml

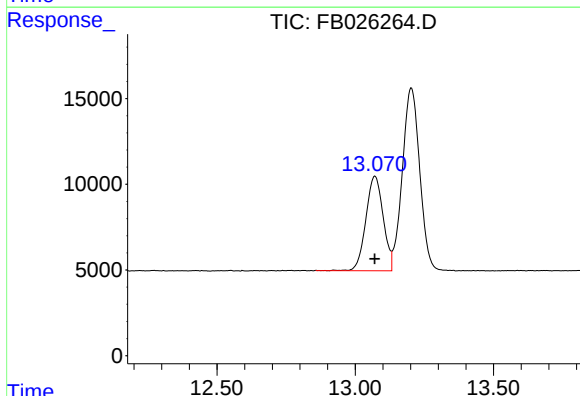


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 239697
Conc: 10.49 ng/ml

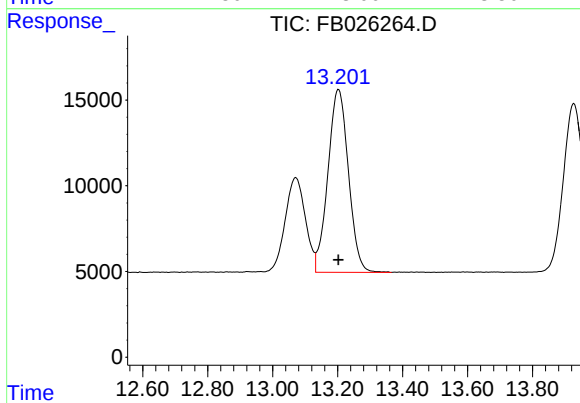

#8 m-Xylene


R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 467563
Conc: 20.84 ng/ml

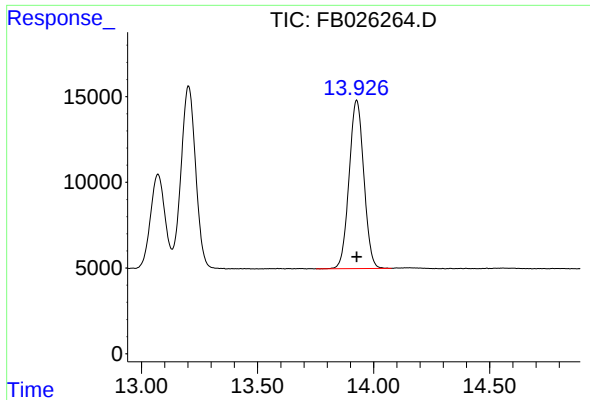

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: 0.000 min
Response: 433047
Conc: 20.47 ng/ml

Instrument :
FID_B
ClientSampleId :

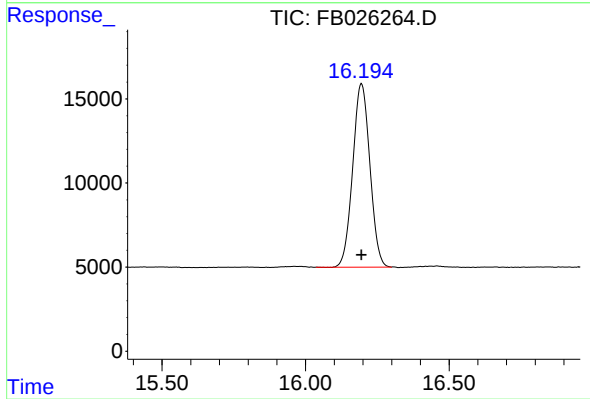

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: 0.000 min
Response: 454323
Conc: 19.52 ng/ml