

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100821\
 Data File : FB026267.D
 Signal(s) : FID2B.CH
 Acq On : 8 Oct 2021 16:43
 Operator : AJ/MA
 Sample : BSF1008S1
 Misc : 5.01G\5.00 ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 08 23:16:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100821.M
 Quant Title :
 QLast Update : Fri Oct 08 14:30:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.845	315161	20.913 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.849	598291	34.370 ng/ml
2) t 2,2,4-Trimethylpentane	7.504	687999	33.307 ng/ml
3) t n-Heptane	7.822	275410	11.755 ng/ml
4) t Benzene	7.960	304199	11.626 ng/ml
6) t Toluene	10.654	868661	33.529 ng/ml
7) t Ethylbenzene	13.073	249813	10.938 ng/ml
8) t m-Xylene	13.204	485168	21.628 ng/ml
9) t O-Xylene	13.929	445828	21.074 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	459333	19.740 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100821\
Data File : FB026267.D
Signal(s) : FID2B.CH
Acq On : 8 Oct 2021 16:43
Operator : AJ/MA
Sample : BSF1008S1
Misc : 5.01G\5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 08 23:16:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100821.M
Quant Title :
QLast Update : Fri Oct 08 14:30:36 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

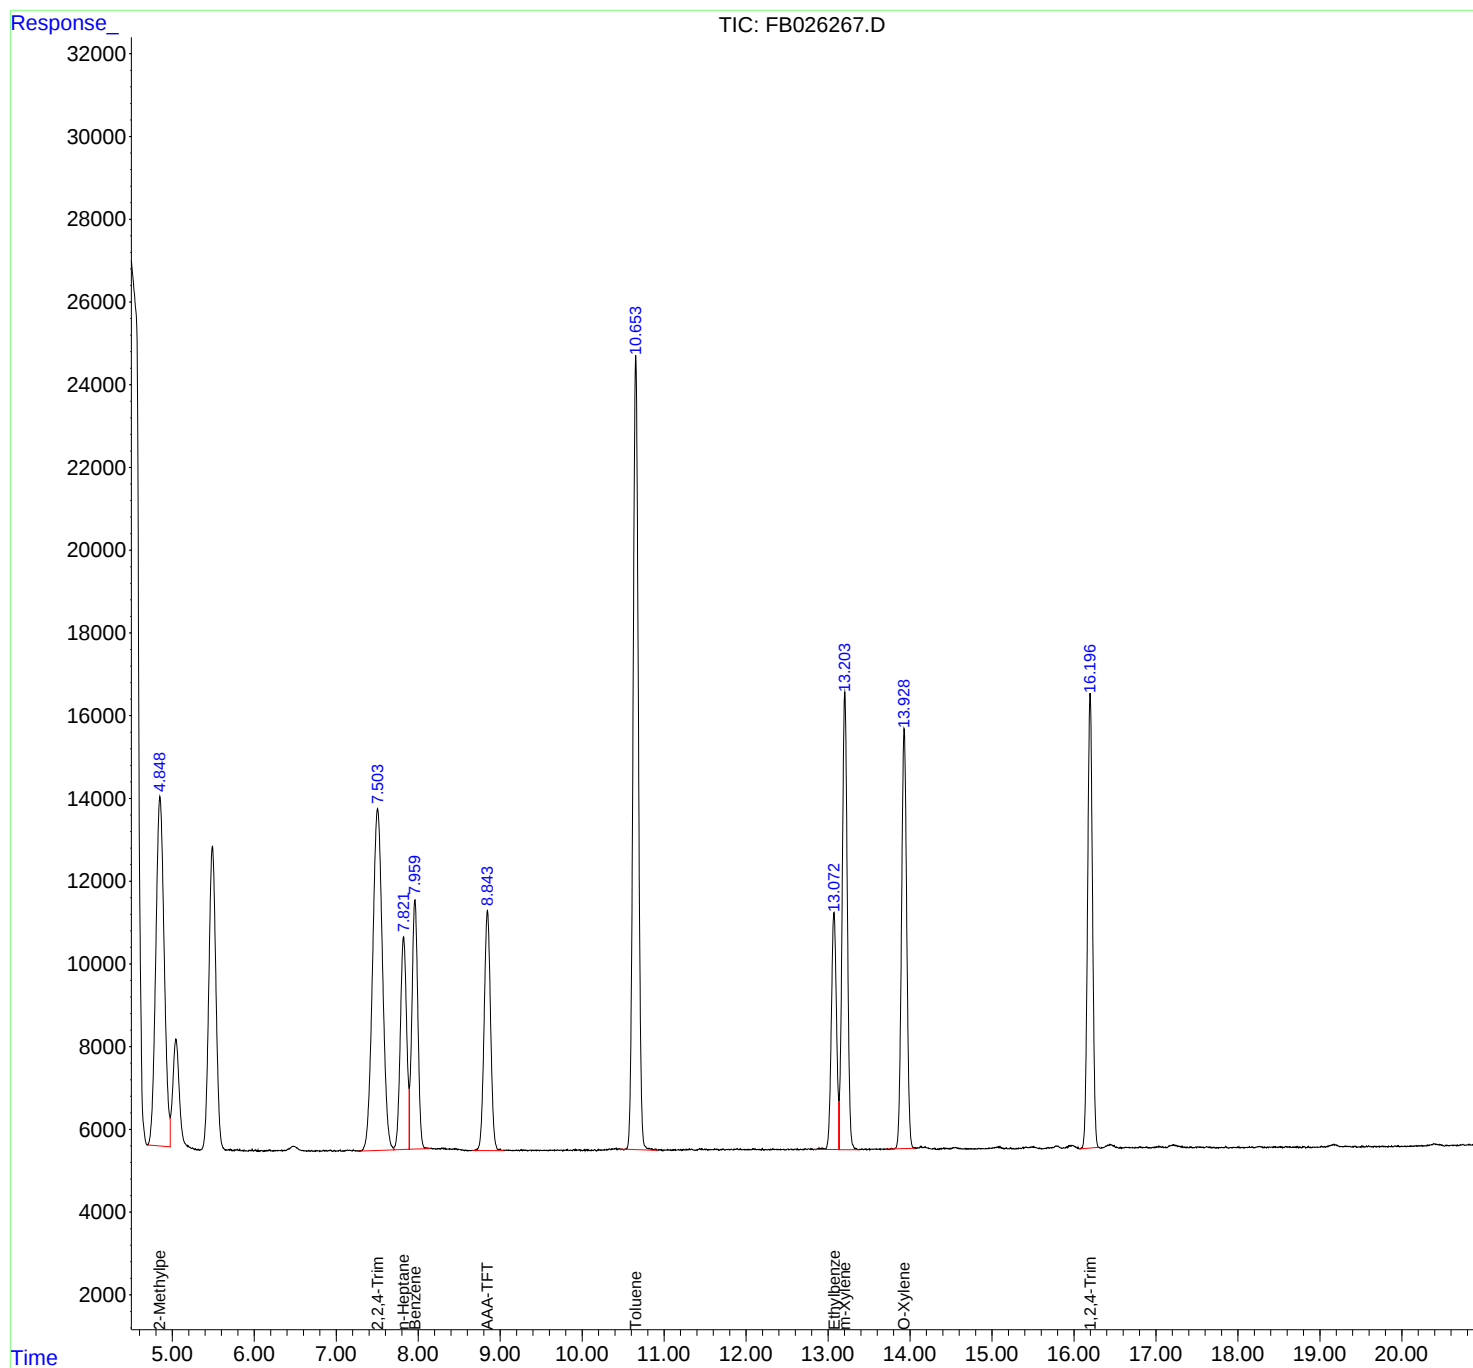


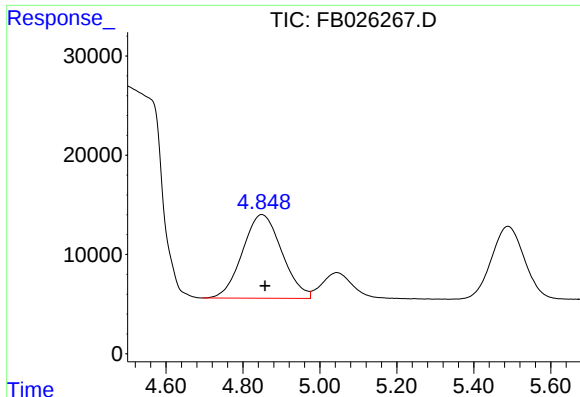

#1 2-Methylpentane


R.T.: 4.849 min
Delta R.T.: -0.008 min
Response: 598291
Conc: 34.37 ng/ml

Instrument :
FID_B
ClientSampleId :

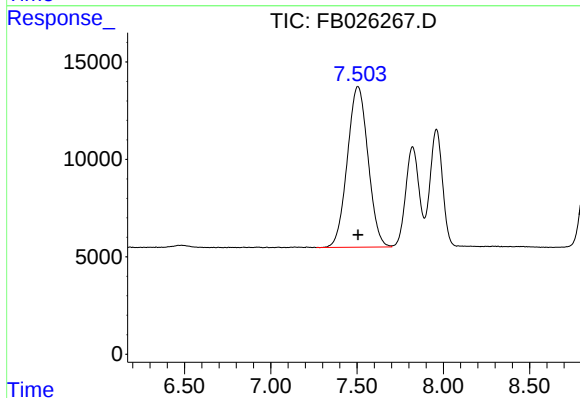


#2 2,2,4-Trimethylpentane

R.T.: 7.504 min
Delta R.T.: -0.002 min
Response: 687999
Conc: 33.31 ng/ml

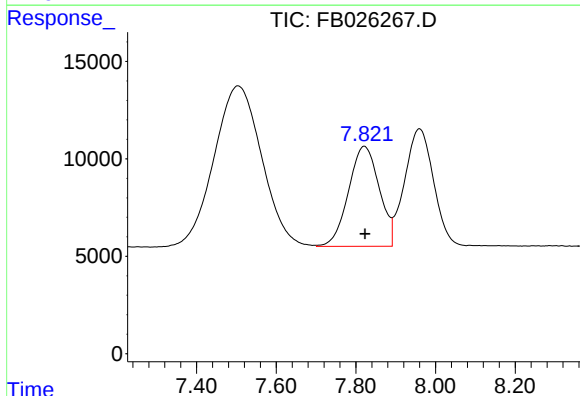


#3 n-Heptane

R.T.: 7.822 min
Delta R.T.: -0.001 min
Response: 275410
Conc: 11.76 ng/ml

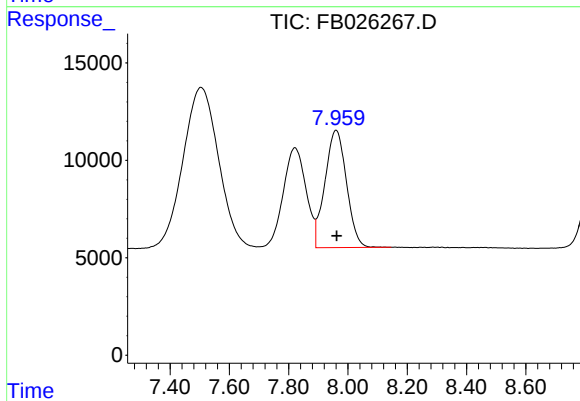

#4 Benzene


R.T.: 7.960 min
Delta R.T.: -0.001 min
Response: 304199
Conc: 11.63 ng/ml

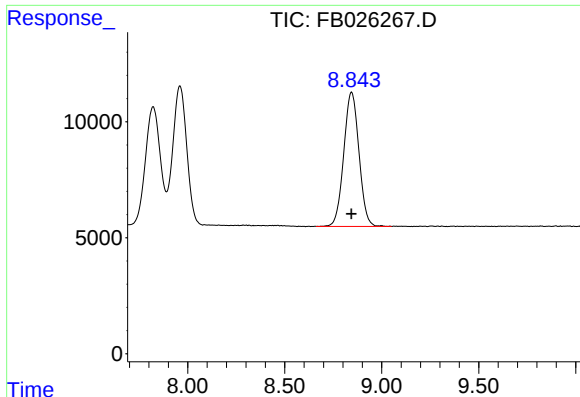

#5 AAA-TFT


R.T.: 8.845 min
Delta R.T.: 0.000 min
Response: 315161
Conc: 20.91 ng/ml

Instrument :
FID_B
ClientSampleId :

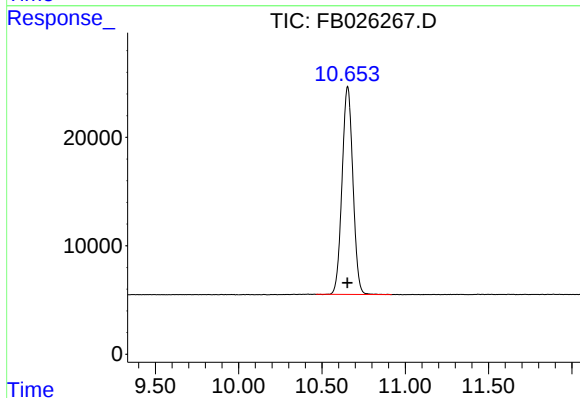


#6 Toluene

R.T.: 10.654 min
Delta R.T.: 0.001 min
Response: 868661
Conc: 33.53 ng/ml

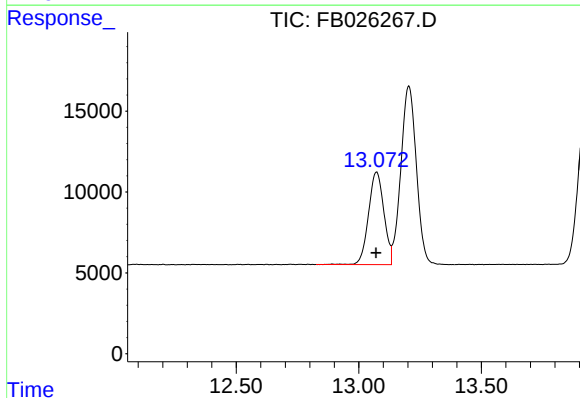


#7 Ethylbenzene

R.T.: 13.073 min
Delta R.T.: 0.002 min
Response: 249813
Conc: 10.94 ng/ml

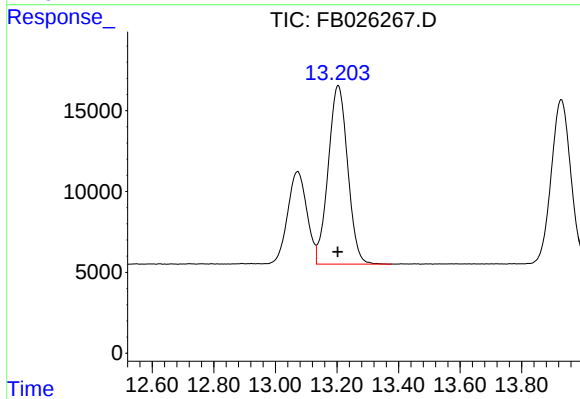

#8 m-Xylene


R.T.: 13.204 min
Delta R.T.: 0.002 min
Response: 485168
Conc: 21.63 ng/ml

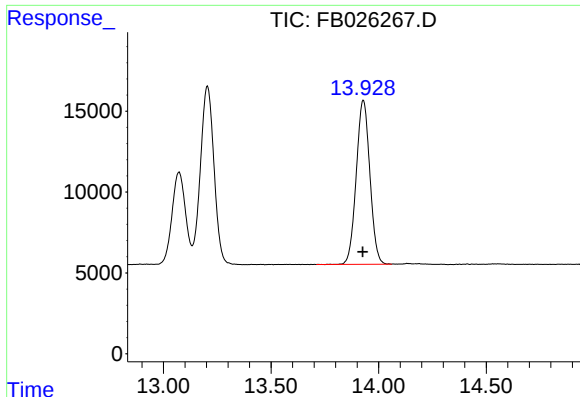

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: 0.002 min
Response: 445828
Conc: 21.07 ng/ml

Instrument :
FID_B
ClientSampleId :

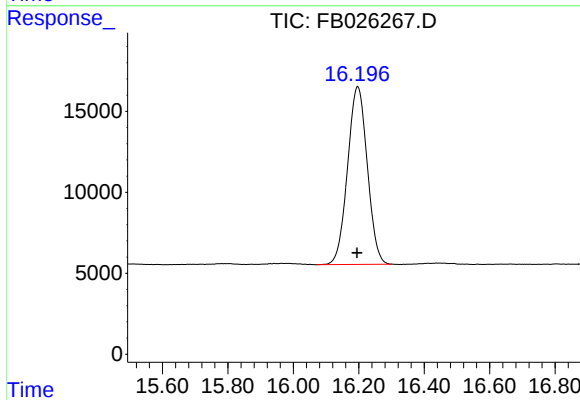

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: 0.003 min
Response: 459333
Conc: 19.74 ng/ml