

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE101121\
 Data File : FE034424.D
 Signal(s) : FID1B.CH
 Acq On : 11 Oct 2021 11:05
 Operator : AJ\MA
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 11 14:54:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100821.M
 Quant Title :
 QLast Update : Fri Oct 08 16:08:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.397	7768661	20.348 ug/ml
12) N-OCTACOSANE	16.792	7532658	19.954 ug/ml
13) N-TRIACONTANE	17.673	265066	0.711 ug/ml
14) N-DOTRIACONTANE	18.502	372664	1.041 ug/ml
15) N-TETRATRIACONTANE	19.283	282472	0.845 ug/ml
16) N-HEXATRIACONTANE	20.021	173504	0.575 ug/ml
17) N-OCTATRIACONTANE	20.744	122569	0.447 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE101121\
Data File : FE034424.D
Signal(s) : FID1B.CH
Acq On : 11 Oct 2021 11:05
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 11 14:54:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100821.M
Quant Title :
QLast Update : Fri Oct 08 16:08:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

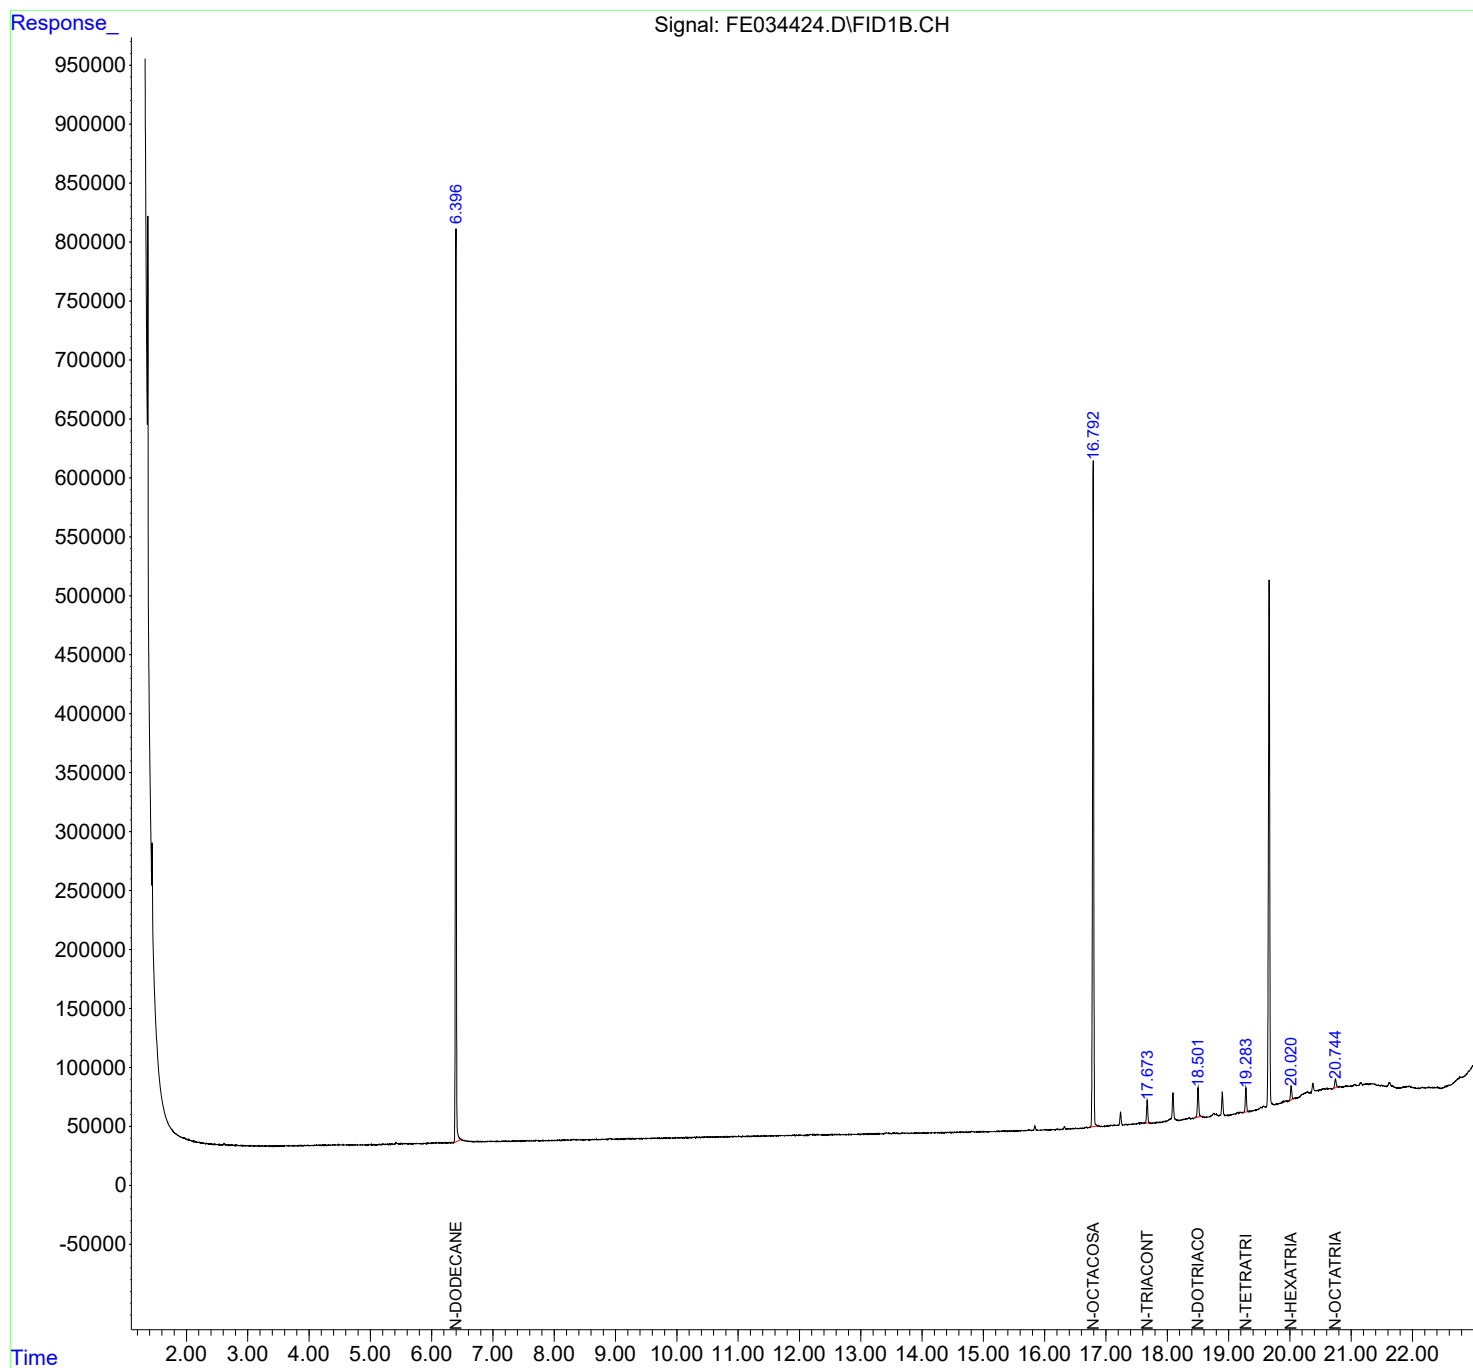


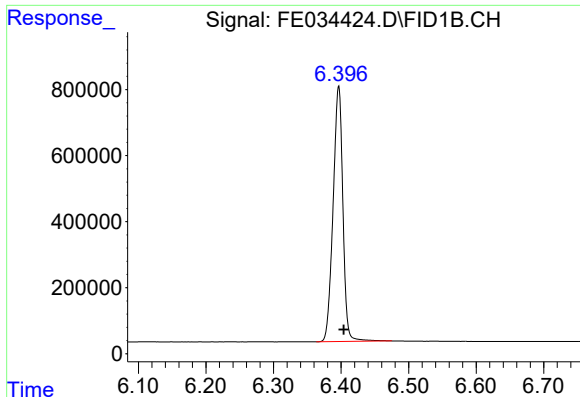

#3 N-DODECANE


R.T.: 6.397 min
Delta R.T.: -0.007 min
Response: 7768661
Conc: 20.35 ug/ml

Instrument :
FID_B
ClientSampleId :

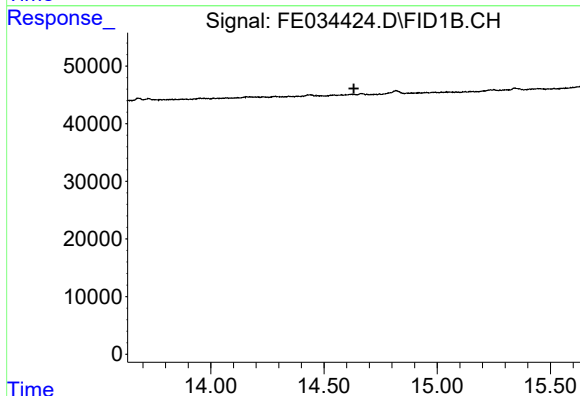


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.632 min
Response: 0
Conc: N.D.

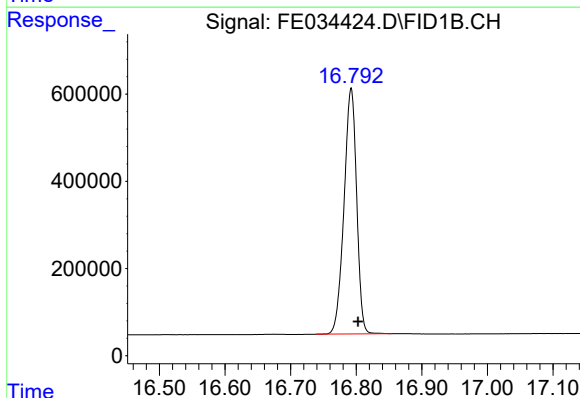


#12 N-OCTACOSANE

R.T.: 16.792 min
Delta R.T.: -0.011 min
Response: 7532658
Conc: 19.95 ug/ml

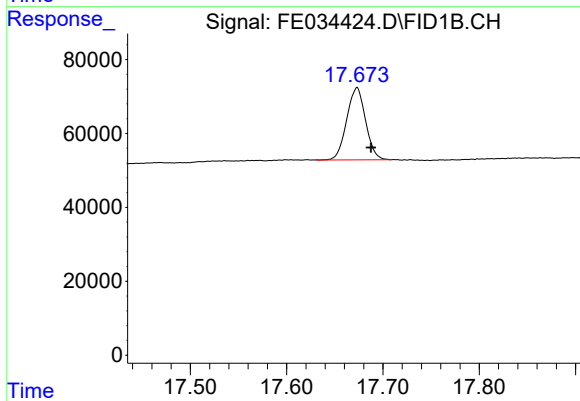

#13 N-TRIACONTANE


R.T.: 17.673 min
Delta R.T.: -0.015 min
Response: 265066
Conc: 0.71 ug/ml

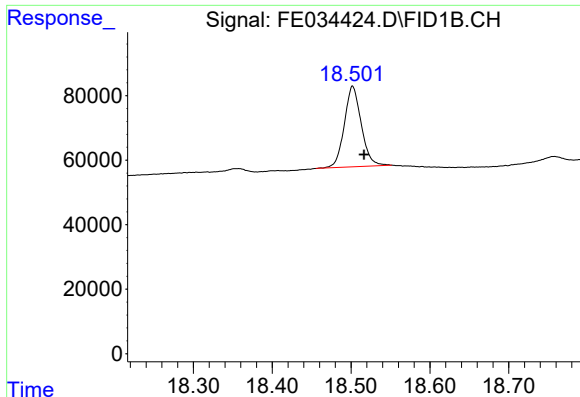

#14 N-DOTRIACONTANE


R.T.: 18.502 min
Delta R.T.: -0.015 min
Response: 372664
Conc: 1.04 ug/ml

Instrument :
FID_B
ClientSampleId :

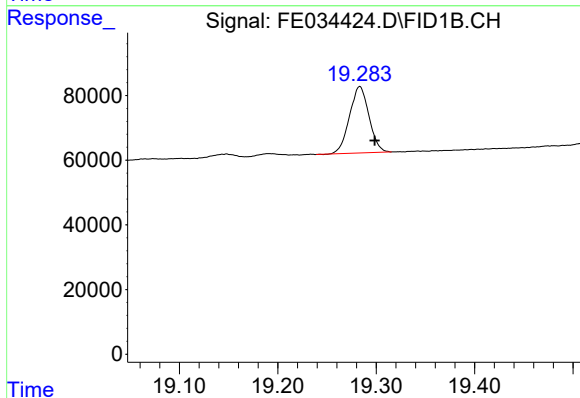


#15 N-TETRATRIACONTANE

R.T.: 19.283 min
Delta R.T.: -0.015 min
Response: 282472
Conc: 0.84 ug/ml

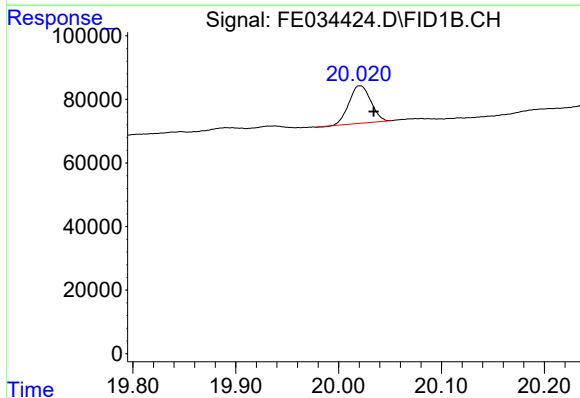

#16 N-HEXATRIACONTANE

R.T.: 20.021 min
Delta R.T.: -0.013 min
Response: 173504
Conc: 0.57 ug/ml

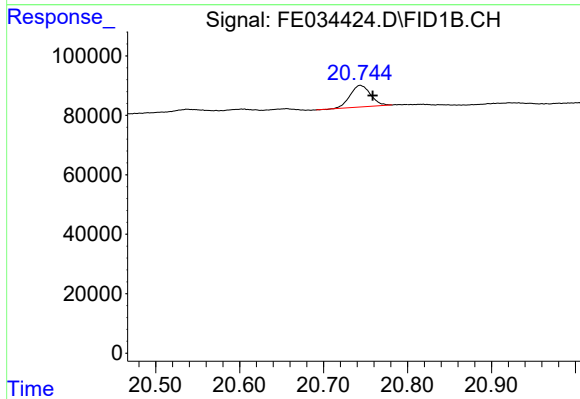

#17 N-OCTATRIACONTANE

R.T.: 20.744 min
Delta R.T.: -0.015 min
Response: 122569
Conc: 0.45 ug/ml