

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100821\
 Data File : FB026271.D
 Signal(s) : FID2B.CH
 Acq On : 8 Oct 2021 19:20
 Operator : AJ/MA
 Sample : M4145-05MS
 Misc : 4.97G\5.00 ML DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 IDW-SO-DRUM-5-100721MS

Integration File: SAMPLE.e
 Quant Time: Oct 08 23:16:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100821.M
 Quant Title :
 QLast Update : Fri Oct 08 14:30:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.844	306687	20.351 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.852	493527	28.351 ng/ml
2) t 2,2,4-Trimethylpentane	7.506	438371	21.222 ng/ml
3) t n-Heptane	7.822	171077	7.302 ng/ml
4) t Benzene	7.961	272500	10.414 ng/ml
6) t Toluene	10.655	780681	30.133 ng/ml
7) t Ethylbenzene	13.073	204226	8.942 ng/ml
8) t m-Xylene	13.205	352585	15.718 ng/ml
9) t O-Xylene	13.929	350994	16.591 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	245038	10.530 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100821\
Data File : FB026271.D
Signal(s) : FID2B.CH
Acq On : 8 Oct 2021 19:20
Operator : AJ/MA
Sample : M4145-05MS
Misc : 4.97G\5.00 ML DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
IDW-SO-DRUM-5-100721MS

Integration File: SAMPLE.e
Quant Time: Oct 08 23:16:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100821.M
Quant Title :
QLast Update : Fri Oct 08 14:30:36 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

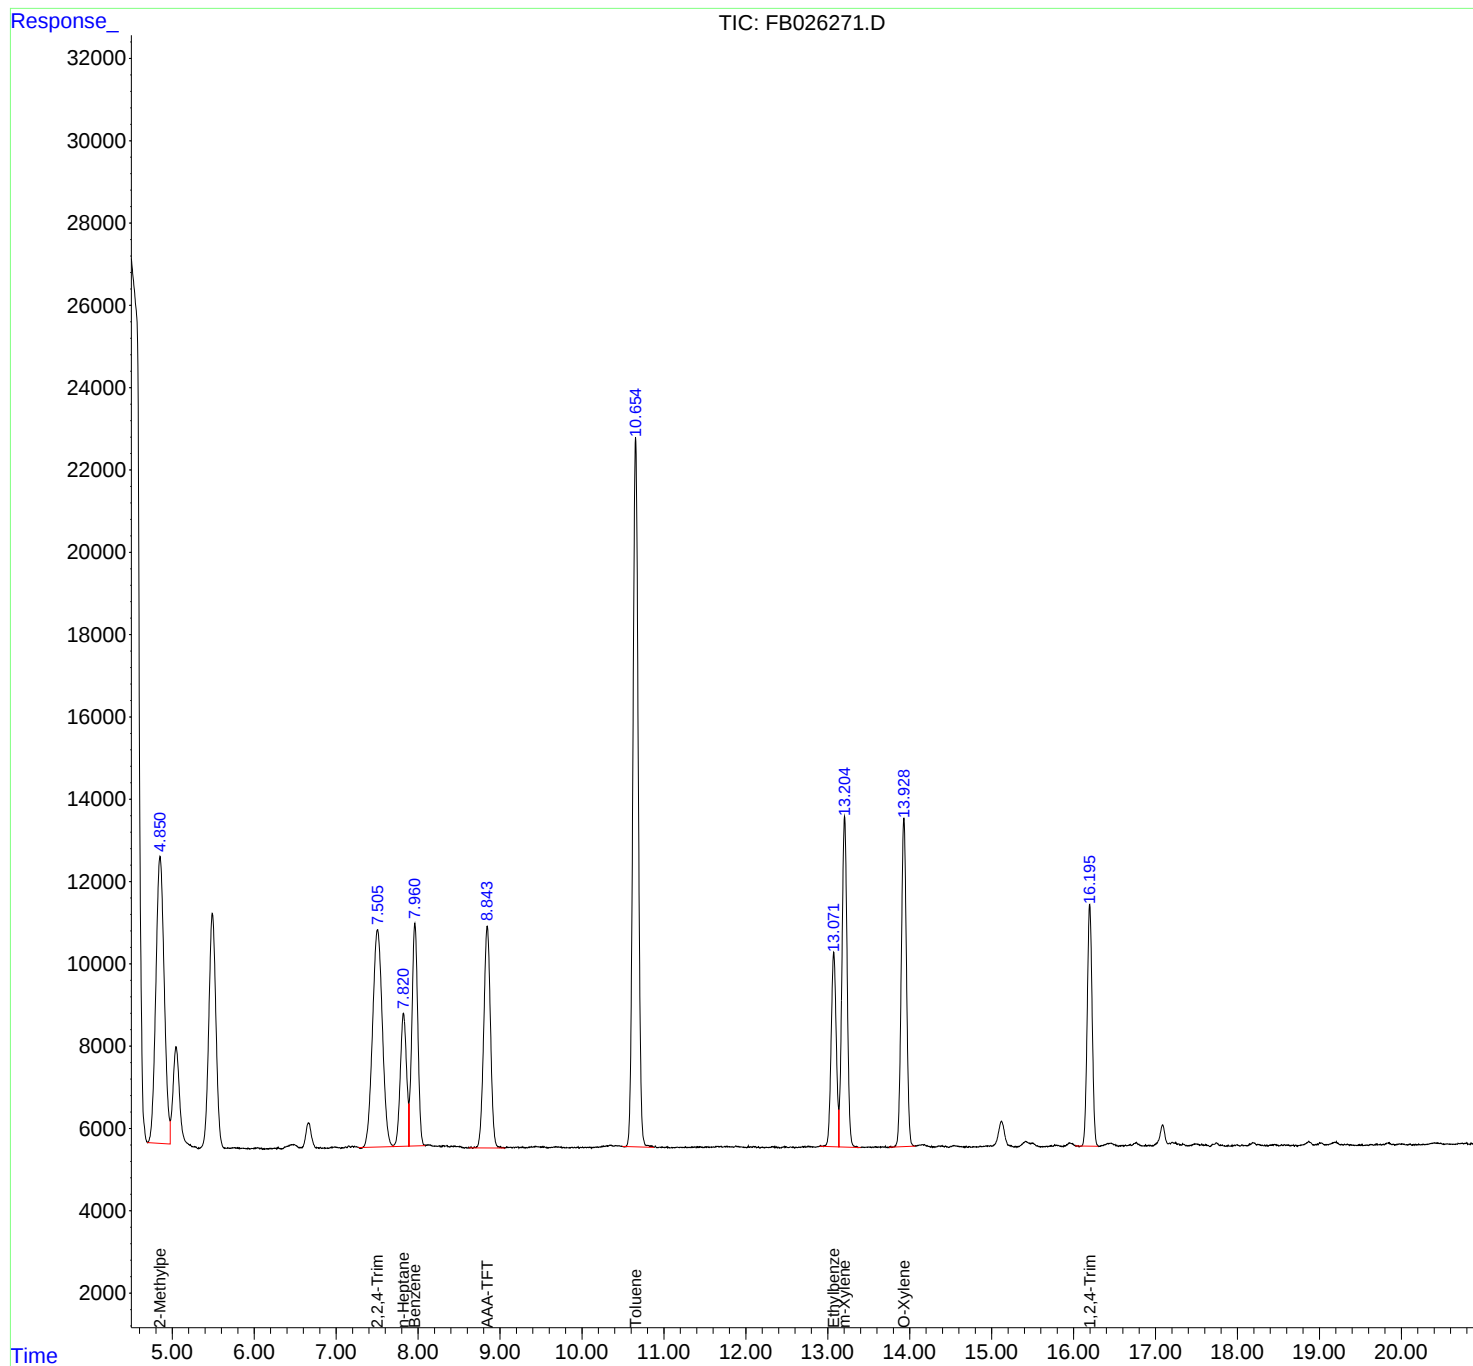


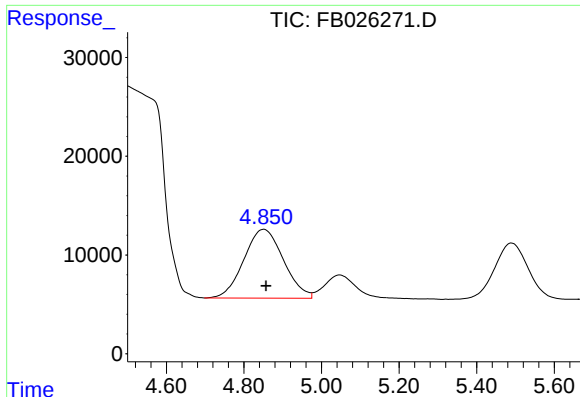

#1 2-Methylpentane


R.T.: 4.852 min
Delta R.T.: -0.005 min
Response: 493527
Conc: 28.35 ng/ml

Instrument :
FID_B
ClientSampleId :
IDW-SO-DRUM-5-100721MS

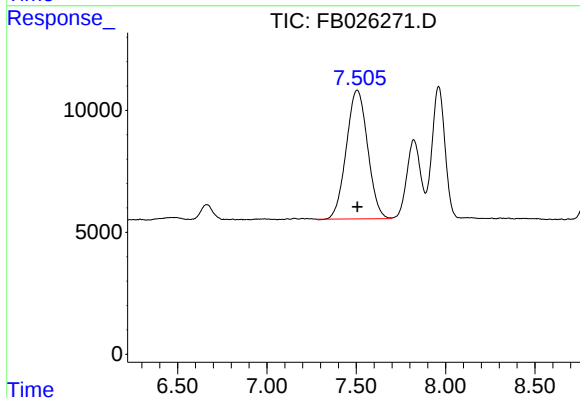


#2 2,2,4-Trimethylpentane

R.T.: 7.506 min
Delta R.T.: 0.000 min
Response: 438371
Conc: 21.22 ng/ml

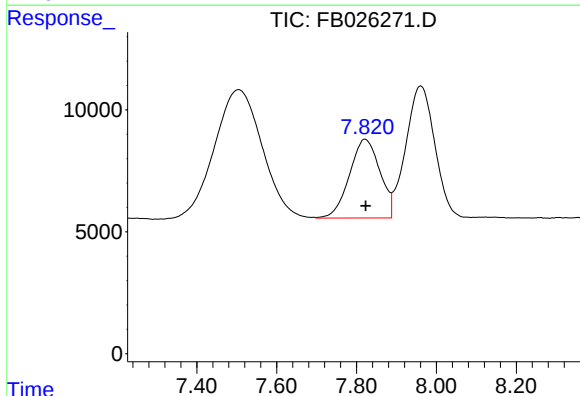


#3 n-Heptane

R.T.: 7.822 min
Delta R.T.: -0.002 min
Response: 171077
Conc: 7.30 ng/ml

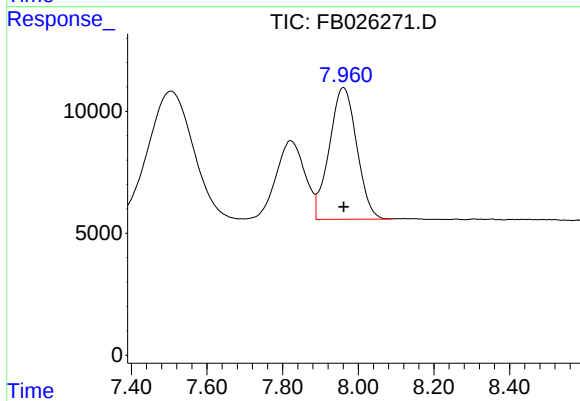

#4 Benzene


R.T.: 7.961 min
Delta R.T.: 0.000 min
Response: 272500
Conc: 10.41 ng/ml

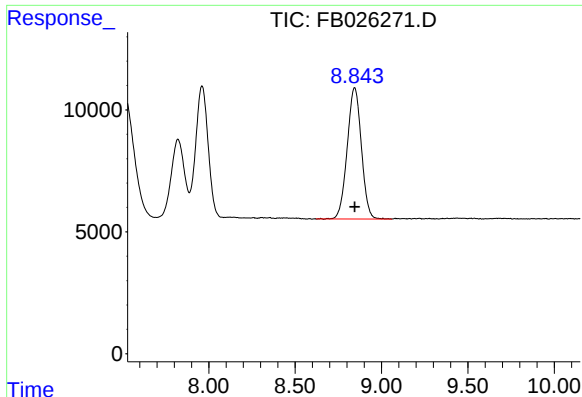

#5 AAA-TFT


R.T.: 8.844 min
Delta R.T.: 0.000 min
Response: 306687
Conc: 20.35 ng/ml

Instrument :
FID_B
ClientSampleId :
IDW-SO-DRUM-5-100721MS

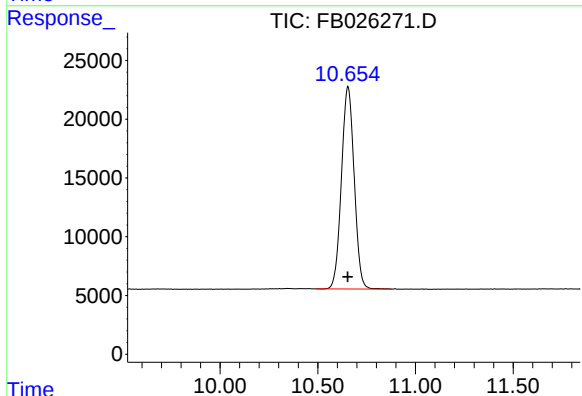


#6 Toluene

R.T.: 10.655 min
Delta R.T.: 0.002 min
Response: 780681
Conc: 30.13 ng/ml

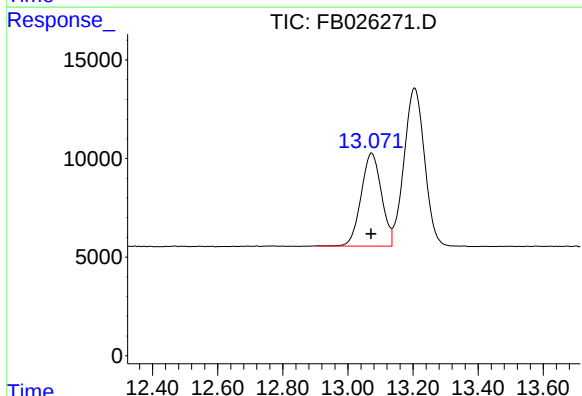


#7 Ethylbenzene

R.T.: 13.073 min
Delta R.T.: 0.002 min
Response: 204226
Conc: 8.94 ng/ml

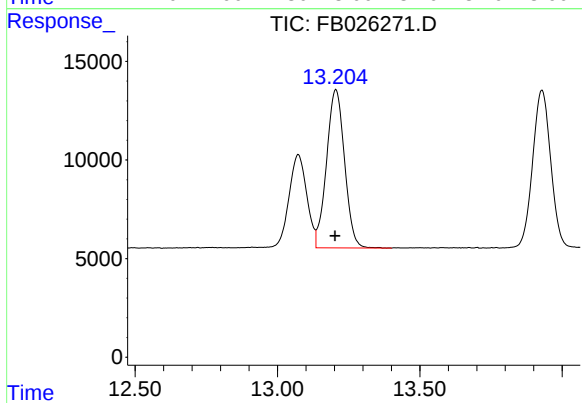

#8 m-Xylene


R.T.: 13.205 min
Delta R.T.: 0.003 min
Response: 352585
Conc: 15.72 ng/ml

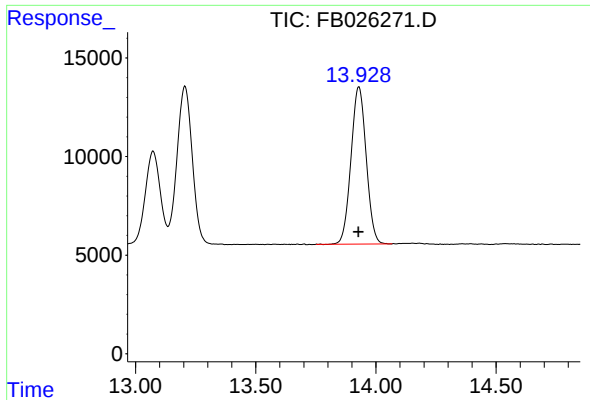

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: 0.002 min
Response: 350994
Conc: 16.59 ng/ml

Instrument :
FID_B
ClientSampleId :
IDW-SO-DRUM-5-100721MS

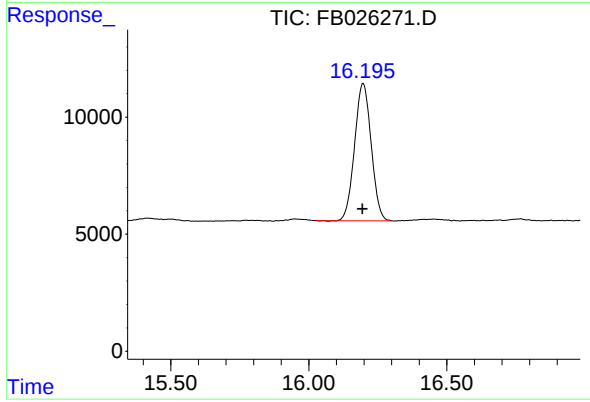

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: 0.002 min
Response: 245038
Conc: 10.53 ng/ml