

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100821\
 Data File : FB026273.D
 Signal(s) : FID2B.CH
 Acq On : 8 Oct 2021 20:36
 Operator : AJ/MA
 Sample : 20 PPB GRO STD
 Misc : 5.01G\5.00 ML DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 PPB GRO STD

Integration File: SAMPLE.e
 Quant Time: Oct 08 23:16:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100821.M
 Quant Title :
 QLast Update : Fri Oct 08 14:30:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.845	344811	22.881 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.851	570943	32.799 ng/ml
2) t 2,2,4-Trimethylpentane	7.506	665408	32.213 ng/ml
3) t n-Heptane	7.823	259895	11.093 ng/ml
4) t Benzene	7.961	293253	11.208 ng/ml
6) t Toluene	10.655	847108	32.697 ng/ml
7) t Ethylbenzene	13.073	240522	10.531 ng/ml
8) t m-Xylene	13.205	472249	21.052 ng/ml
9) t O-Xylene	13.929	438234	20.715 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	440272	18.920 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100821\
Data File : FB026273.D
Signal(s) : FID2B.CH
Acq On : 8 Oct 2021 20:36
Operator : AJ/MA
Sample : 20 PPB GRO STD
Misc : 5.01G\5.00 ML DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

Integration File: SAMPLE.e
Quant Time: Oct 08 23:16:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100821.M
Quant Title :
QLast Update : Fri Oct 08 14:30:36 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

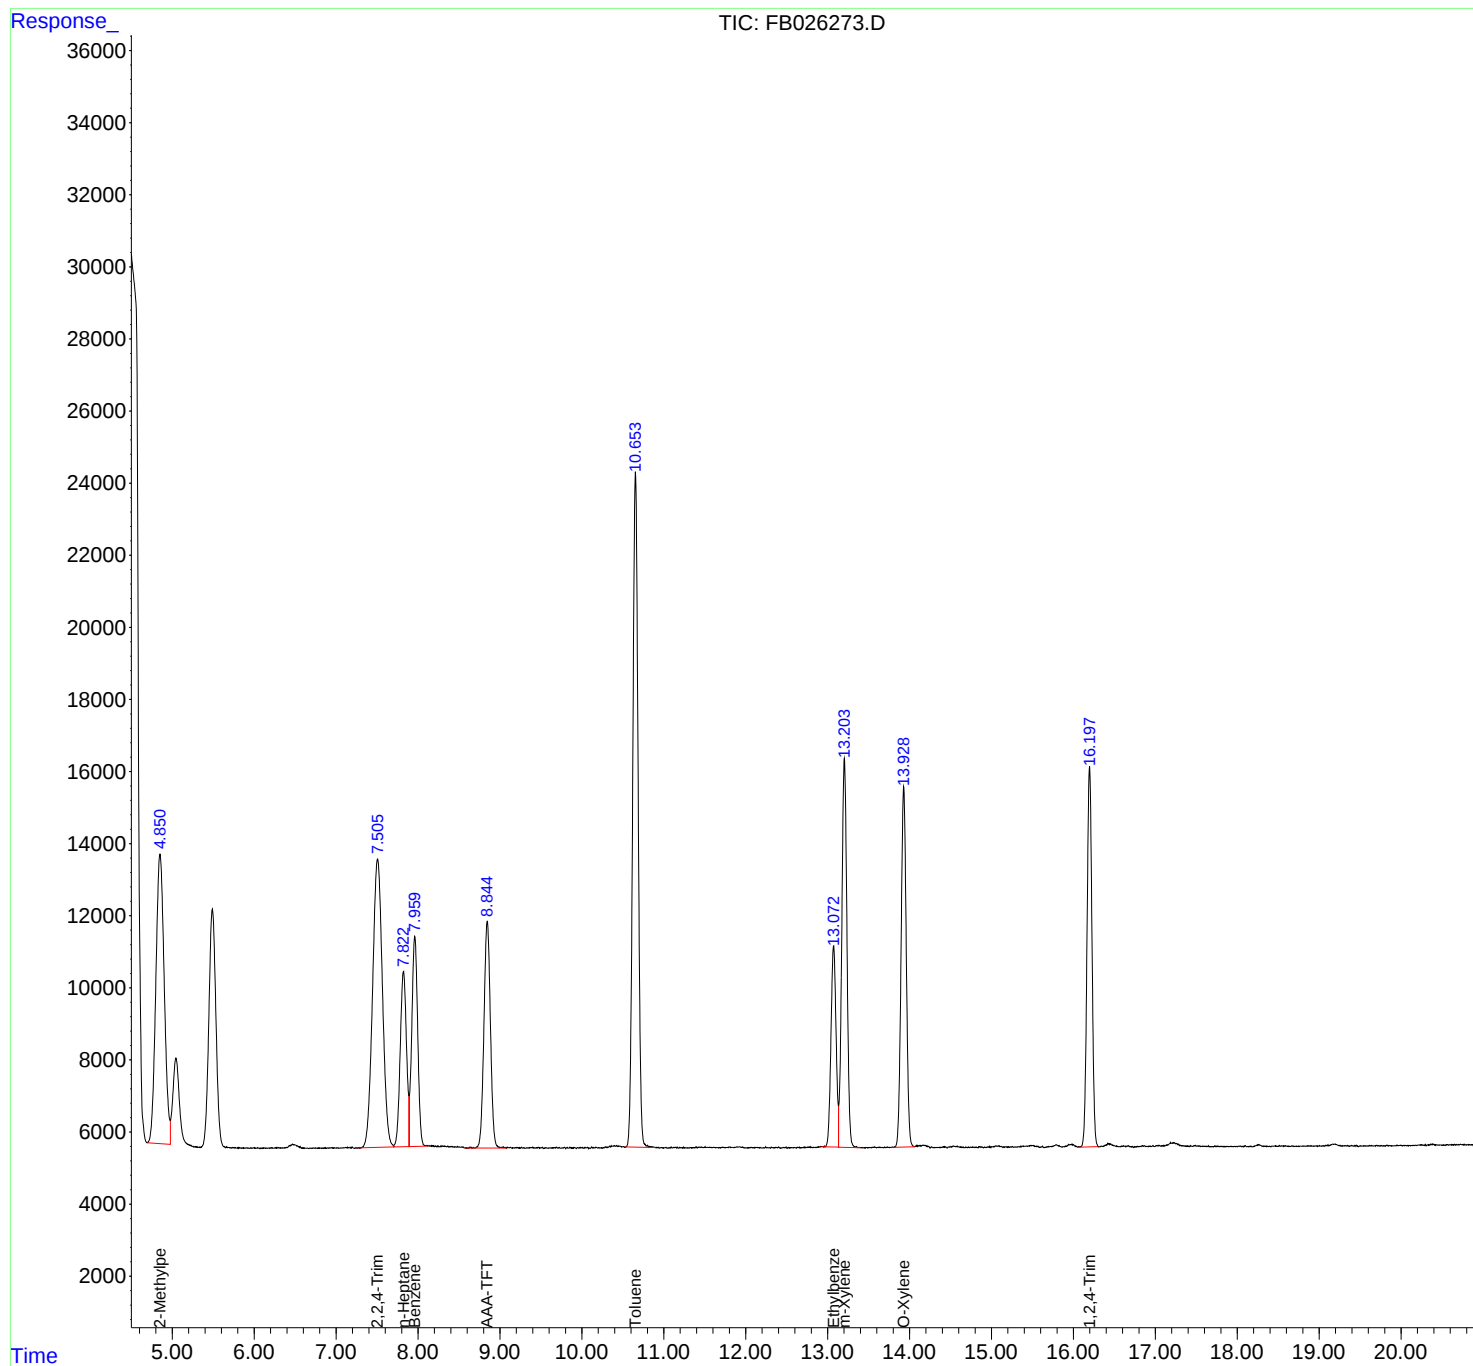


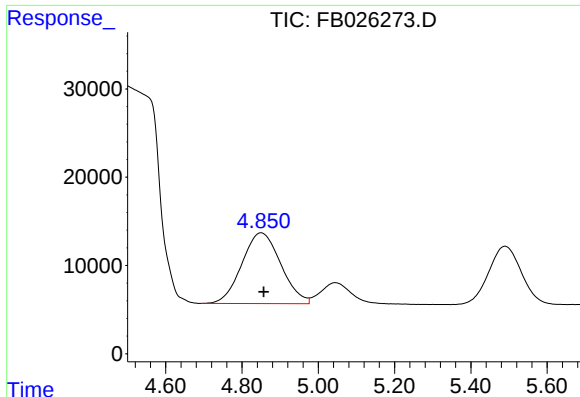

#1 2-Methylpentane


R.T.: 4.851 min
Delta R.T.: -0.006 min
Response: 570943
Conc: 32.80 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

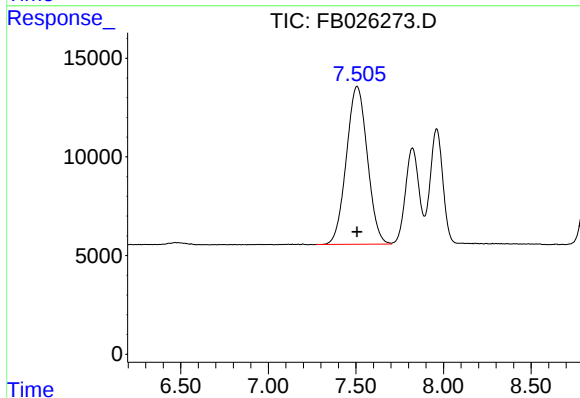


#2 2,2,4-Trimethylpentane

R.T.: 7.506 min
Delta R.T.: 0.000 min
Response: 665408
Conc: 32.21 ng/ml

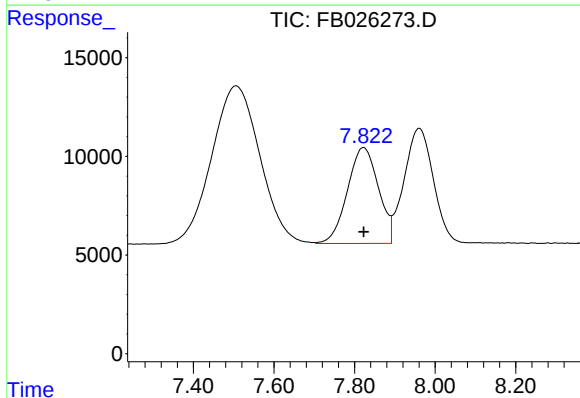


#3 n-Heptane

R.T.: 7.823 min
Delta R.T.: 0.000 min
Response: 259895
Conc: 11.09 ng/ml

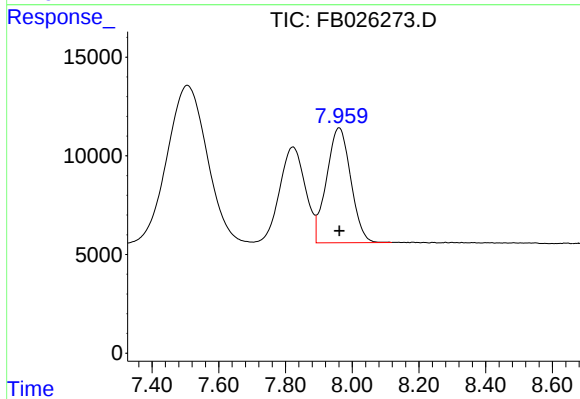

#4 Benzene


R.T.: 7.961 min
Delta R.T.: 0.000 min
Response: 293253
Conc: 11.21 ng/ml

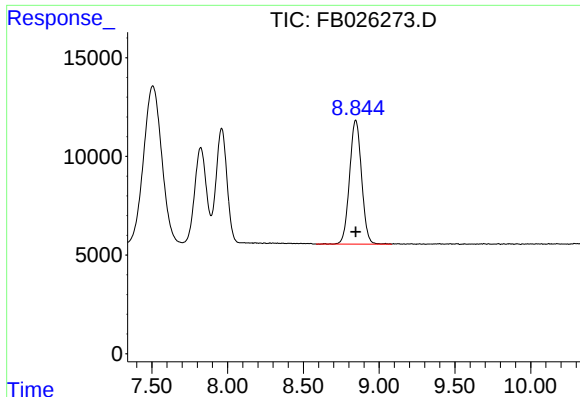

#5 AAA-TFT


R.T.: 8.845 min
Delta R.T.: 0.000 min
Response: 344811
Conc: 22.88 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

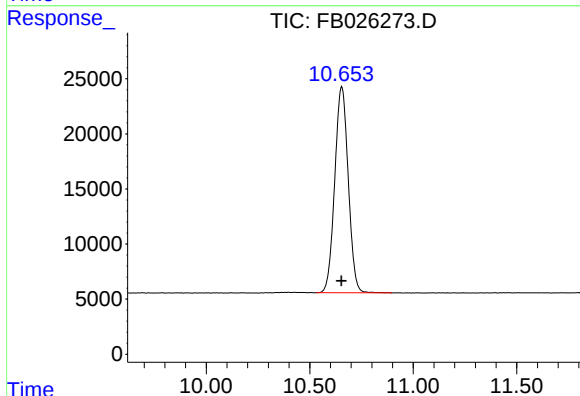


#6 Toluene

R.T.: 10.655 min
Delta R.T.: 0.002 min
Response: 847108
Conc: 32.70 ng/ml

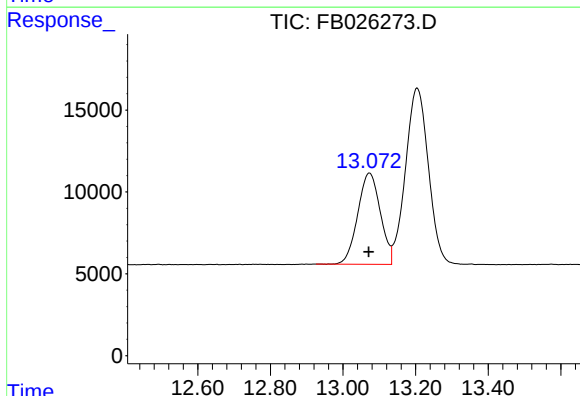


#7 Ethylbenzene

R.T.: 13.073 min
Delta R.T.: 0.002 min
Response: 240522
Conc: 10.53 ng/ml

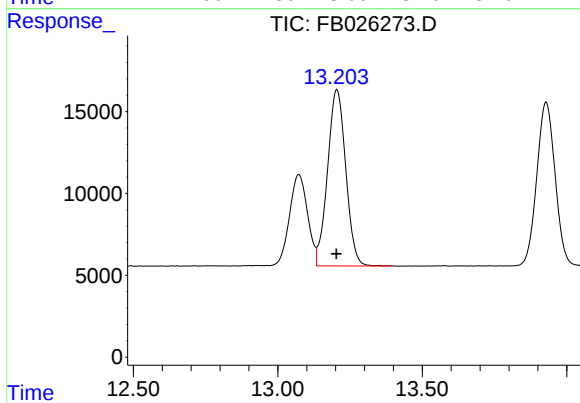

#8 m-Xylene


R.T.: 13.205 min
Delta R.T.: 0.002 min
Response: 472249
Conc: 21.05 ng/ml

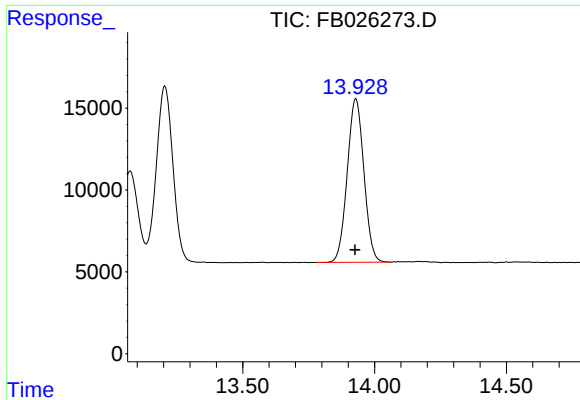

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: 0.002 min
Response: 438234
Conc: 20.72 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

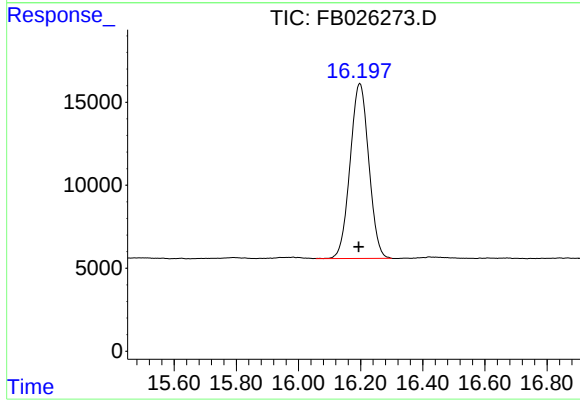

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.003 min
Response: 440272
Conc: 18.92 ng/ml