

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100918\
Data File : FB018143.D
Signal(s) : FID2B.CH
Acq On : 9 Oct 2018 11:05
Operator : MJ/SJ
Sample : J5294-01MS
Misc : 5.00g/5.00mL DI Water
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 09 11:57:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.109	173957	20.565 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.961	392105	24.621 ng/ml
2) t 2,2,4-Trimethylpentane	7.728	405725	25.495 ng/ml
3) t n-Heptane	8.064	95889	6.222 ng/ml
4) t Benzene	8.204	178887	9.397 ng/ml
6) t Toluene	10.959	418057	26.416 ng/ml
7) t Ethylbenzene	13.408	140667	8.609 ng/ml
8) t m-Xylene	13.541	300259	17.356 ng/ml
9) t O-Xylene	14.273	328974	18.103 ng/ml
10) t 1,2,4-Trimethylbenzene	16.556	371931	17.485 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100918\
Data File : FB018143.D
Signal(s) : FID2B.CH
Acq On : 9 Oct 2018 11:05
Operator : MJ/SJ
Sample : J5294-01MS
Misc : 5.00g/5.00mL DI Water
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 09 11:57:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

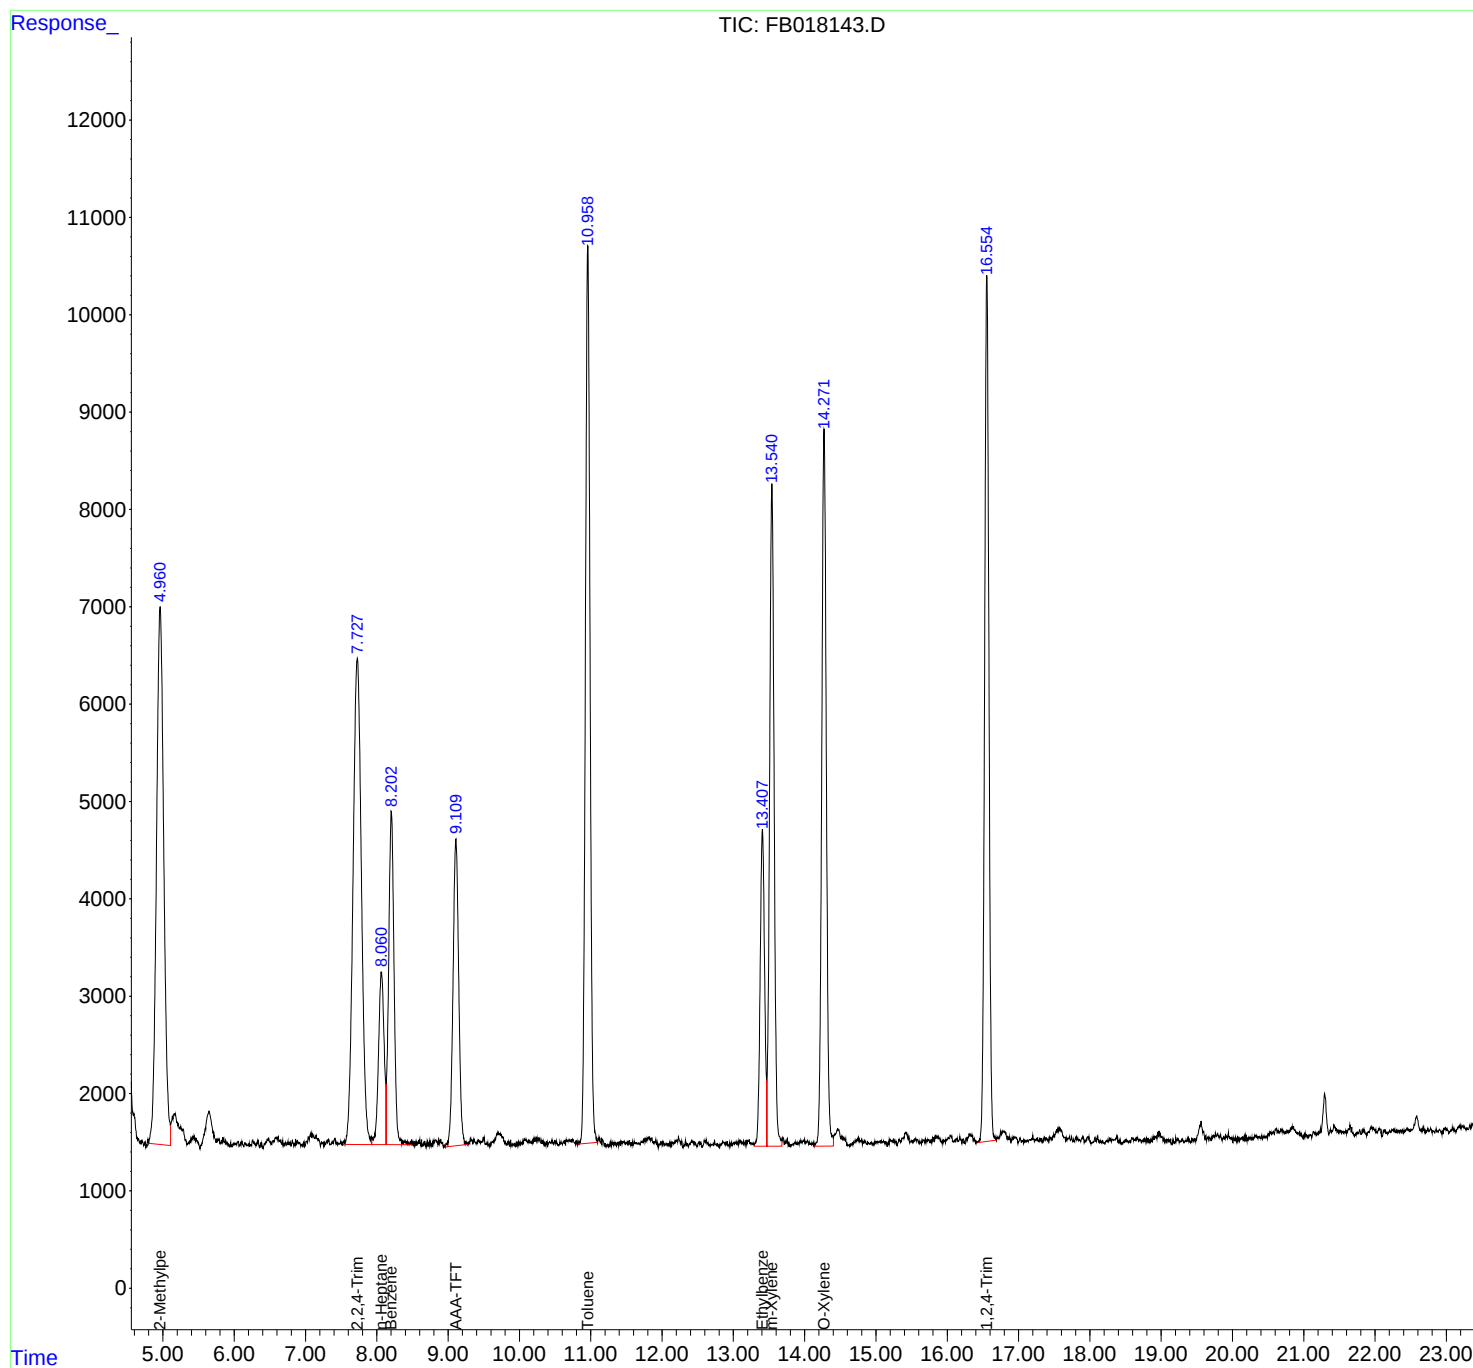

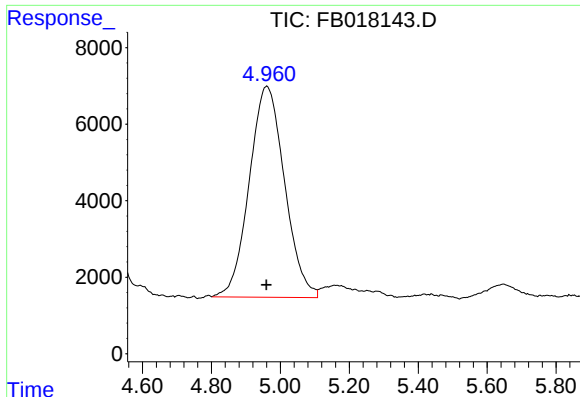


#1 2-Methylpentane

R.T.: 4.961 min
Delta R.T.: 0.001 min
Response: 392105
Conc: 24.62 ng/ml

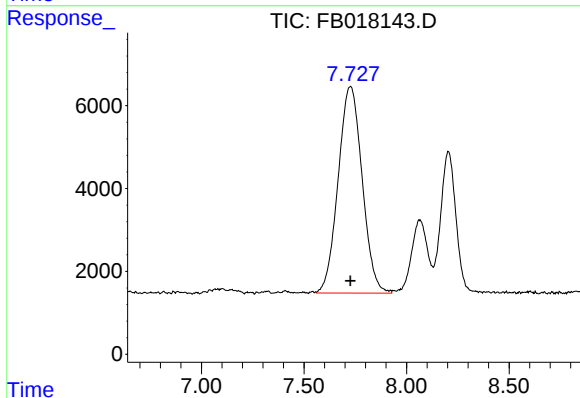


#2 2,2,4-Trimethylpentane

R.T.: 7.728 min
Delta R.T.: 0.000 min
Response: 405725
Conc: 25.50 ng/ml

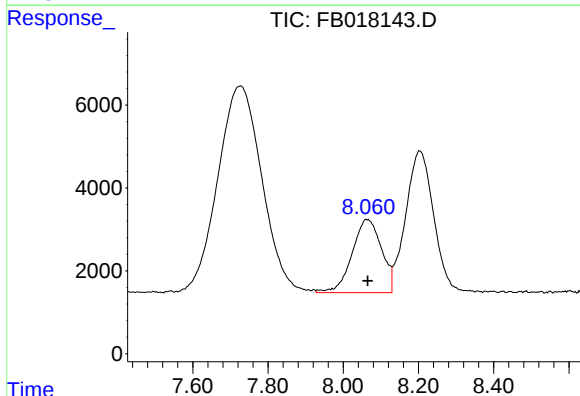


#3 n-Heptane

R.T.: 8.064 min
Delta R.T.: 0.000 min
Response: 95889
Conc: 6.22 ng/ml

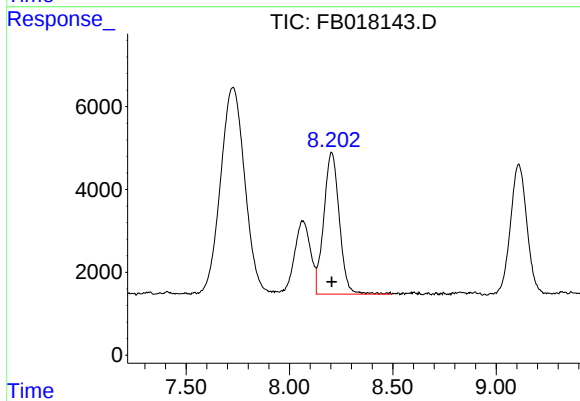


#4 Benzene

R.T.: 8.204 min
Delta R.T.: 0.000 min
Response: 178887
Conc: 9.40 ng/ml

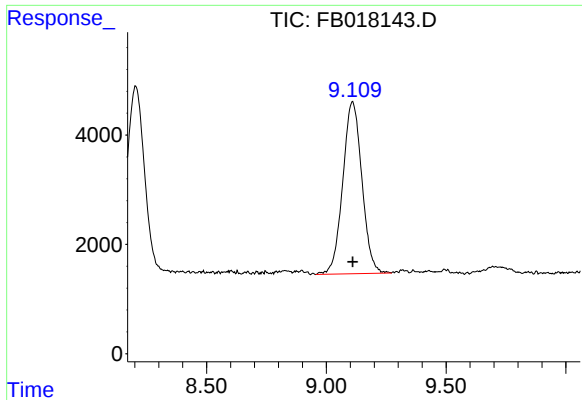


#5 AAA-TFT

R.T.: 9.109 min
Delta R.T.: 0.000 min
Response: 173957
Conc: 20.57 ng/ml

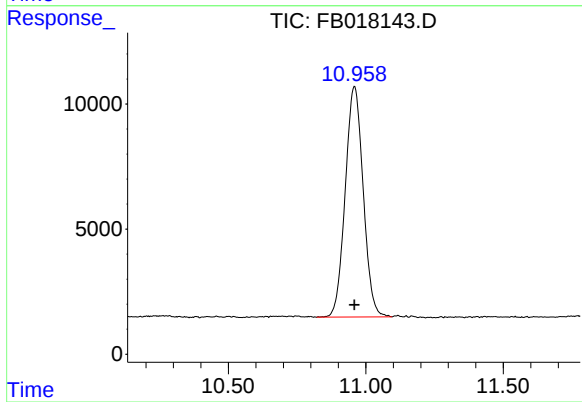


#6 Toluene

R.T.: 10.959 min
Delta R.T.: 0.000 min
Response: 418057
Conc: 26.42 ng/ml

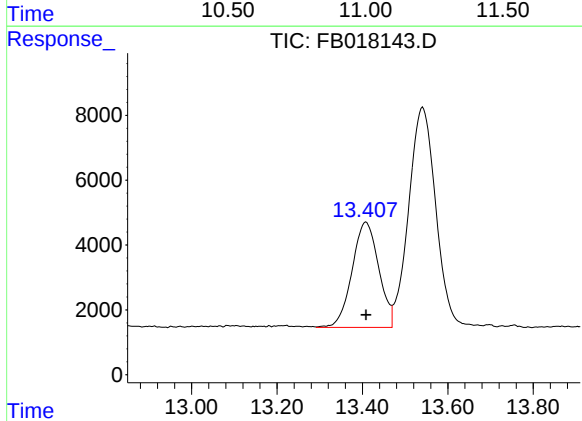


#7 Ethylbenzene

R.T.: 13.408 min
Delta R.T.: 0.000 min
Response: 140667
Conc: 8.61 ng/ml

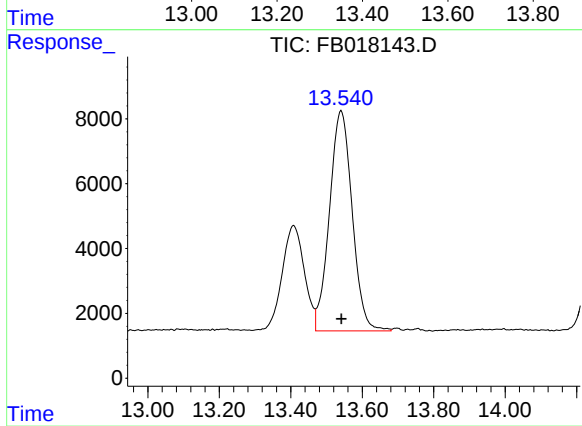


#8 m-Xylene

R.T.: 13.541 min
Delta R.T.: 0.000 min
Response: 300259
Conc: 17.36 ng/ml

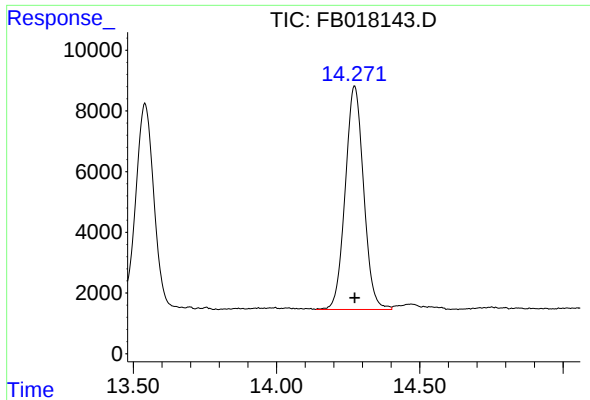

#9 O-Xylene

R.T.: 14.273 min
Delta R.T.: 0.000 min
Response: 328974
Conc: 18.10 ng/ml

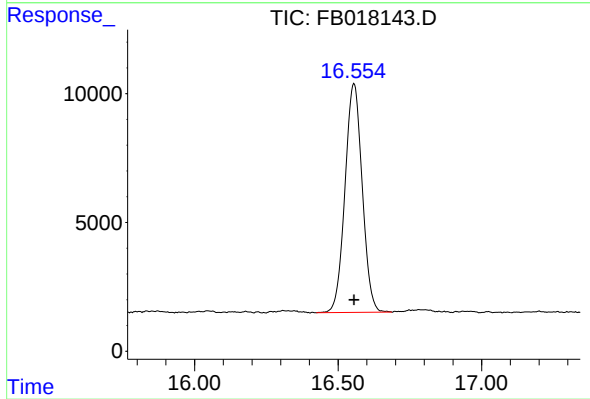

#10 1,2,4-Trimethylbenzene

R.T.: 16.556 min
Delta R.T.: 0.000 min
Response: 371931
Conc: 17.48 ng/ml