

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100918\
 Data File : FB018140.D
 Signal(s) : FID2B.CH
 Acq On : 9 Oct 2018 9:12
 Operator : MJ/SJ
 Sample : BSF1009S1
 Misc : 5.03g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 09 10:28:03 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
 Quant Title :
 QLast Update : Fri Sep 14 13:09:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.108	165935	19.617 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.959	409849	25.736 ng/ml
2) t 2,2,4-Trimethylpentane	7.725	432892	27.203 ng/ml
3) t n-Heptane	8.064	140780	9.135 ng/ml
4) t Benzene	8.203	185756	9.758 ng/ml
6) t Toluene	10.958	458719	28.985 ng/ml
7) t Ethylbenzene	13.408	155343	9.507 ng/ml
8) t m-Xylene	13.540	328453	18.986 ng/ml
9) t O-Xylene	14.272	346005	19.040 ng/ml
10) t 1,2,4-Trimethylbenzene	16.554	409739	19.262 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100918\
Data File : FB018140.D
Signal(s) : FID2B.CH
Acq On : 9 Oct 2018 9:12
Operator : MJ/SJ
Sample : BSF1009S1
Misc : 5.03g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 09 10:28:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

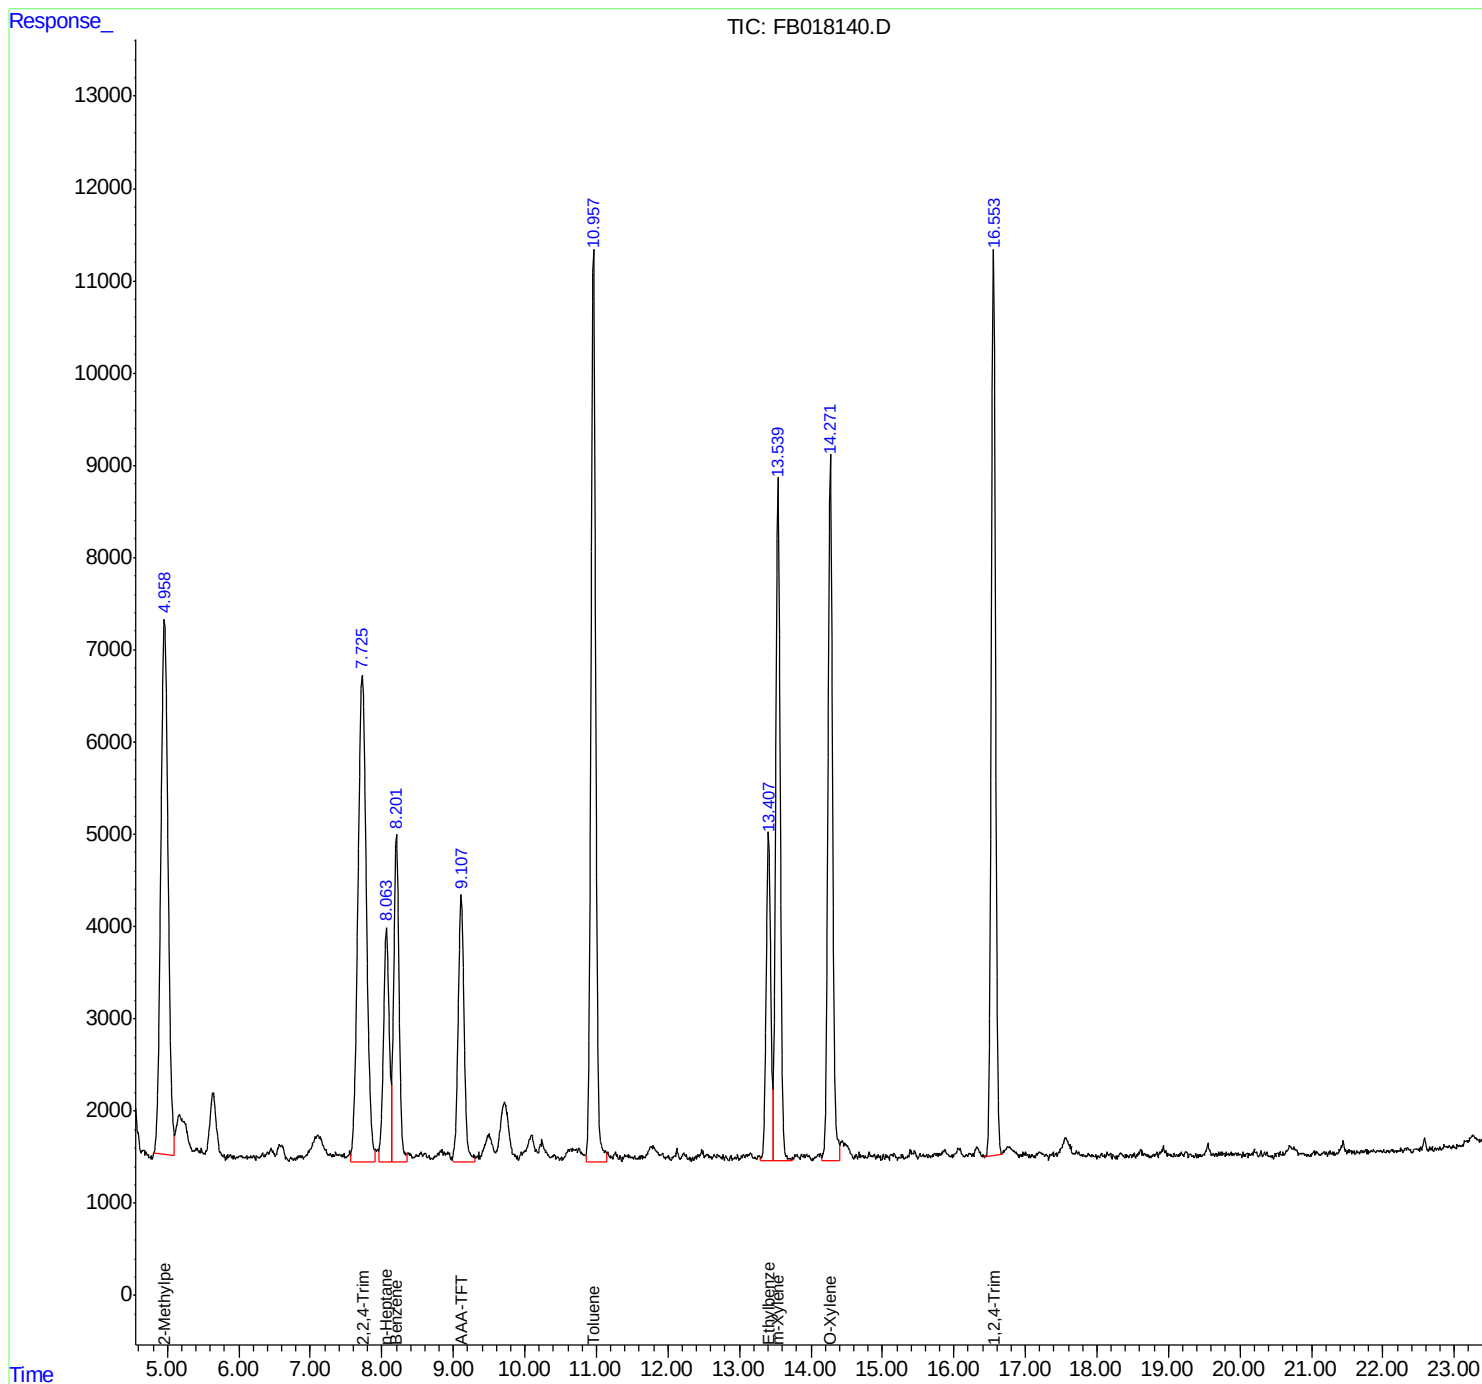

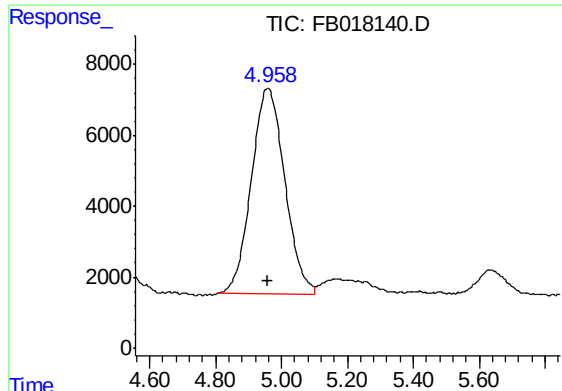


#1 2-Methylpentane

R.T.: 4.959 min
Delta R.T.: 0.000 min
Response: 409849
Conc: 25.74 ng/ml

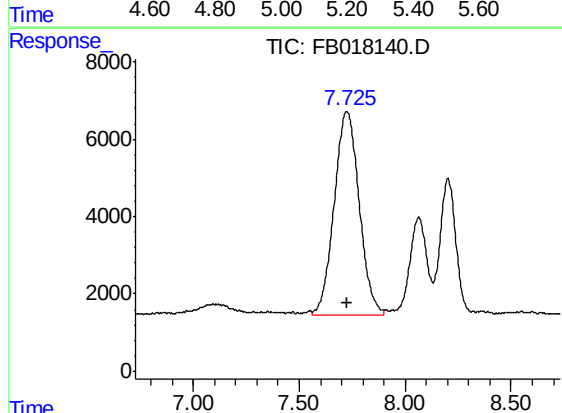


#2 2,2,4-Trimethylpentane

R.T.: 7.725 min
Delta R.T.: -0.002 min
Response: 432892
Conc: 27.20 ng/ml

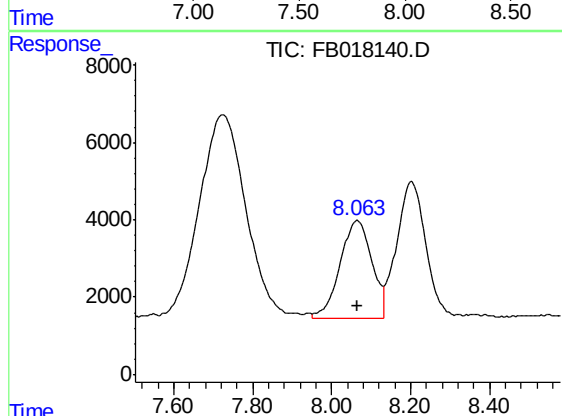


#3 n-Heptane

R.T.: 8.064 min
Delta R.T.: 0.000 min
Response: 140780
Conc: 9.14 ng/ml

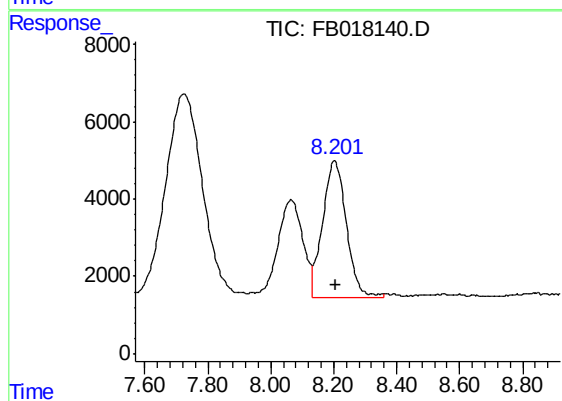


#4 Benzene

R.T.: 8.203 min
Delta R.T.: -0.002 min
Response: 185756
Conc: 9.76 ng/ml

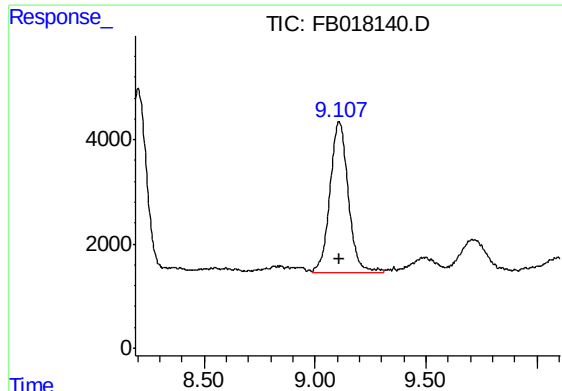


#5 AAA-TFT

R.T.: 9.108 min
Delta R.T.: -0.002 min
Response: 165935
Conc: 19.62 ng/ml

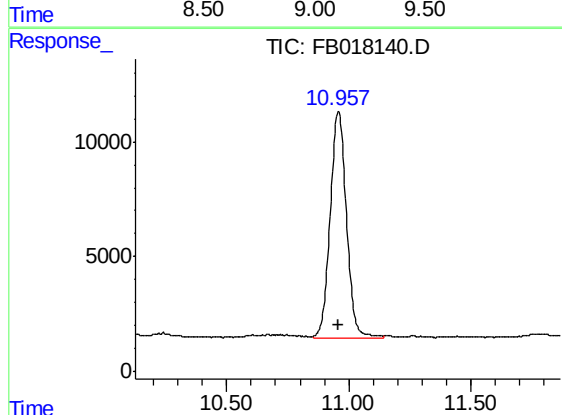


#6 Toluene

R.T.: 10.958 min
Delta R.T.: -0.001 min
Response: 458719
Conc: 28.98 ng/ml

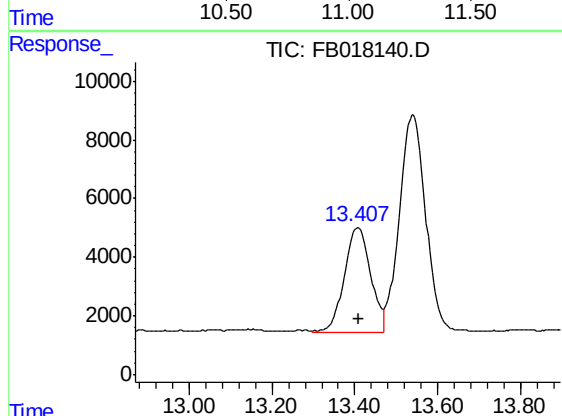


#7 Ethylbenzene

R.T.: 13.408 min
Delta R.T.: 0.000 min
Response: 155343
Conc: 9.51 ng/ml

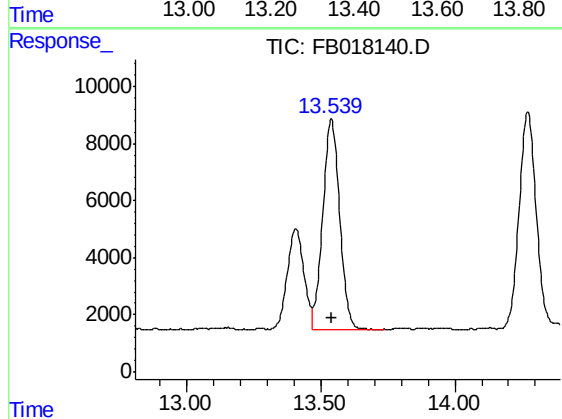


#8 m-Xylene

R.T.: 13.540 min
Delta R.T.: 0.000 min
Response: 328453
Conc: 18.99 ng/ml

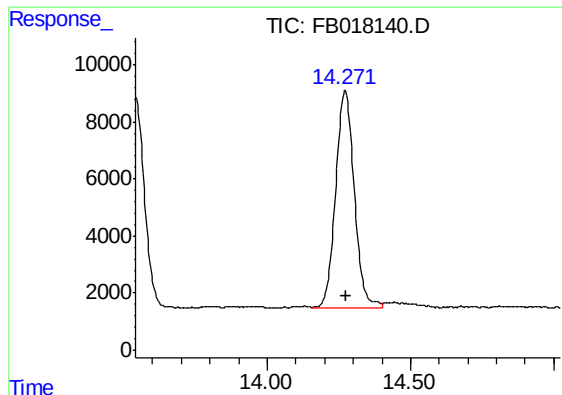

#9 O-Xylene

R.T.: 14.272 min
Delta R.T.: 0.000 min
Response: 346005
Conc: 19.04 ng/ml

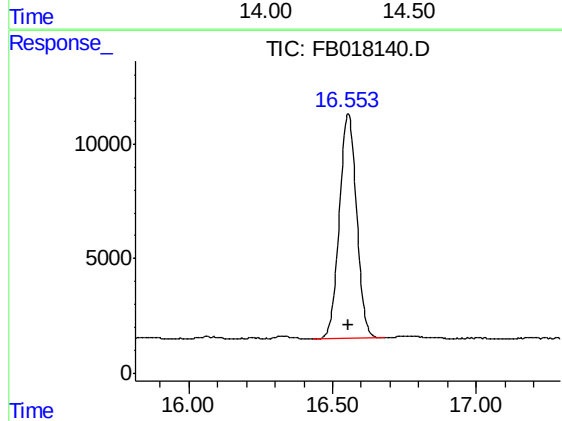

#10 1,2,4-Trimethylbenzene

R.T.: 16.554 min
Delta R.T.: -0.001 min
Response: 409739
Conc: 19.26 ng/ml