

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100919\
 Data File : FB022705.D
 Signal(s) : FID2B.CH
 Acq On : 9 Oct 2019 15:22
 Operator : DD/AJ
 Sample : K5147-02MSD
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 09 15:43:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100919.M
 Quant Title :
 QLast Update : Wed Oct 09 11:21:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	427769	16.630 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	663917	19.538 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	636635	17.599 ng/ml
3) t n-Heptane	7.756	71706	1.990 ng/ml
4) t Benzene	7.890	261125	6.075 ng/ml
6) t Toluene	10.628	736816	17.452 ng/ml
7) t Ethylbenzene	13.067	279003	7.045 ng/ml
8) t m-Xylene	13.200	422051	11.354 ng/ml
9) t O-Xylene	13.928	488411	13.922 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	248696	9.057 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100919\
Data File : FB022705.D
Signal(s) : FID2B.CH
Acq On : 9 Oct 2019 15:22
Operator : DD/AJ
Sample : K5147-02MSD
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 09 15:43:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100919.M
Quant Title :
QLast Update : Wed Oct 09 11:21:39 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

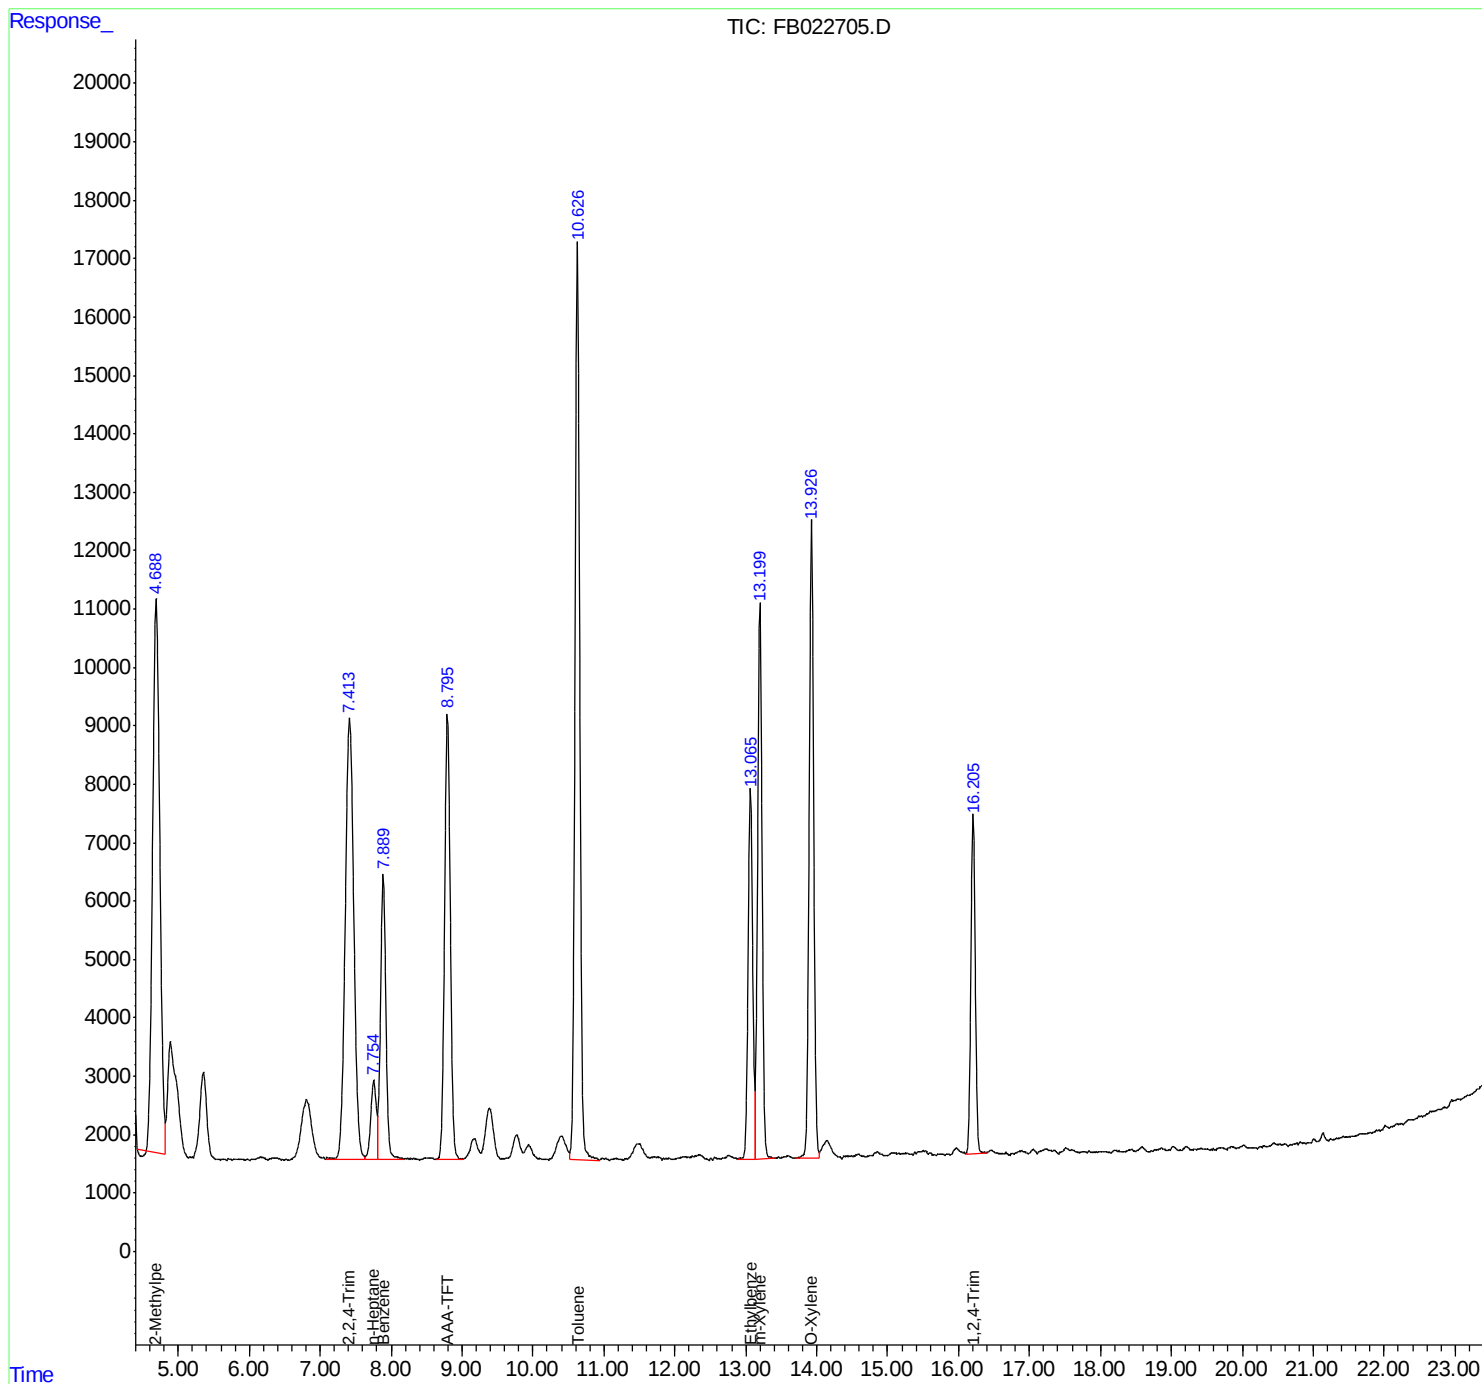

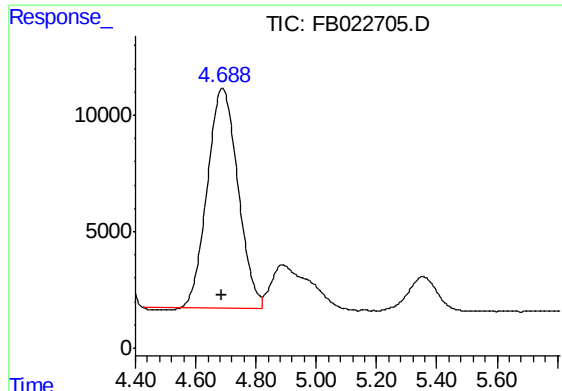


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: 0.002 min
Response: 663917
Conc: 19.54 ng/ml

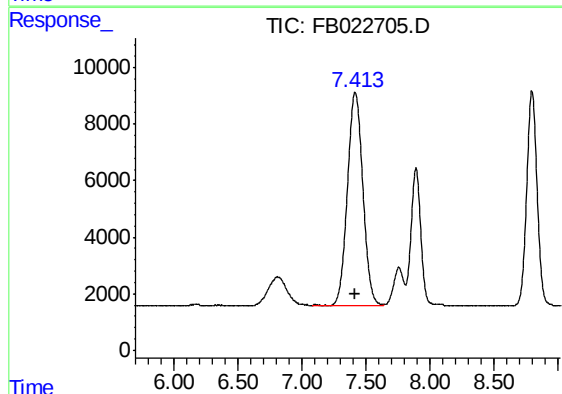


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: 0.000 min
Response: 636635
Conc: 17.60 ng/ml

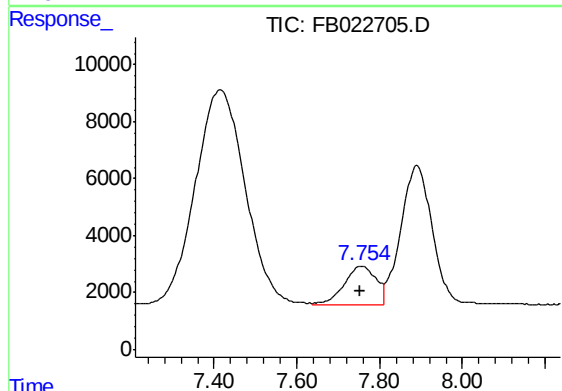


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.002 min
Response: 71706
Conc: 1.99 ng/ml

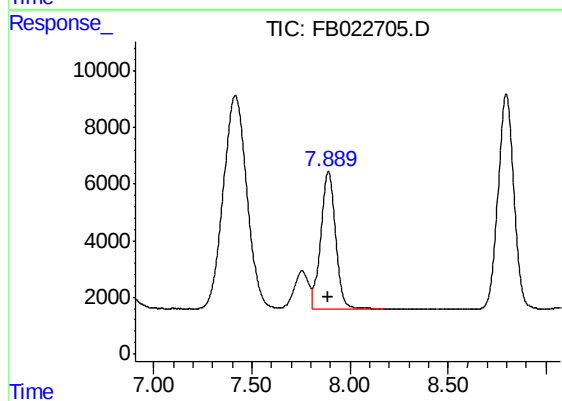


#4 Benzene

R.T.: 7.890 min
Delta R.T.: 0.002 min
Response: 261125
Conc: 6.08 ng/ml

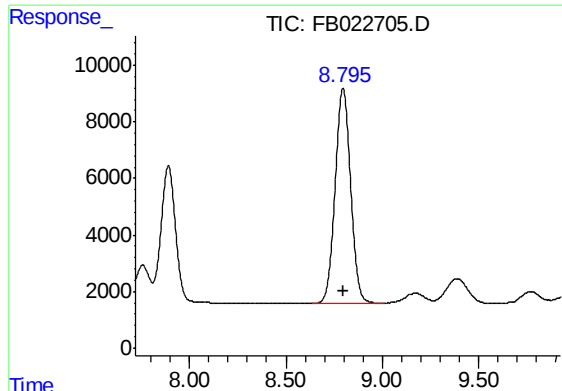


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: 0.000 min
Response: 427769
Conc: 16.63 ng/ml

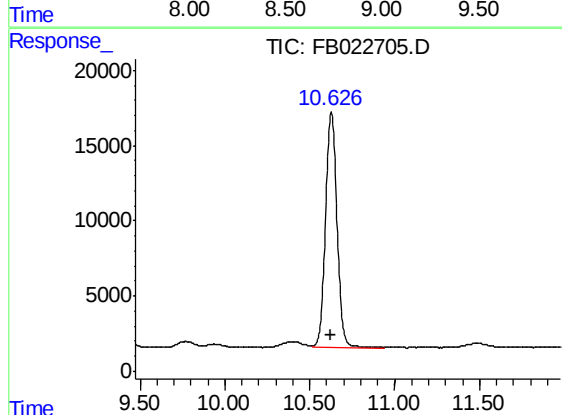


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.000 min
Response: 736816
Conc: 17.45 ng/ml

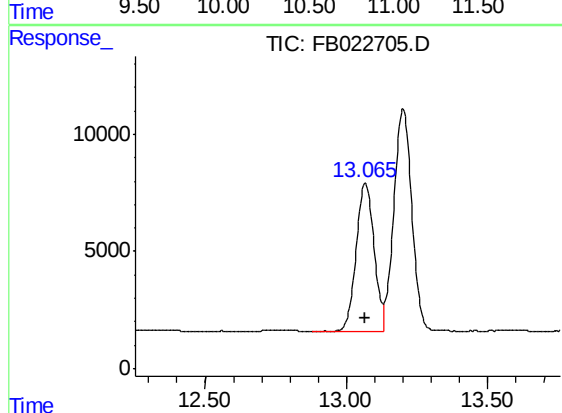


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: 0.000 min
Response: 279003
Conc: 7.04 ng/ml

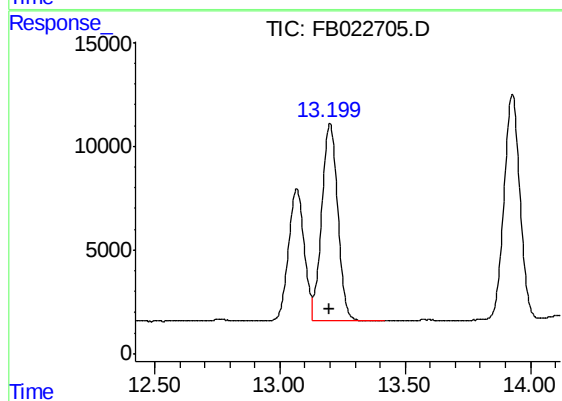


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: 0.000 min
Response: 422051
Conc: 11.35 ng/ml

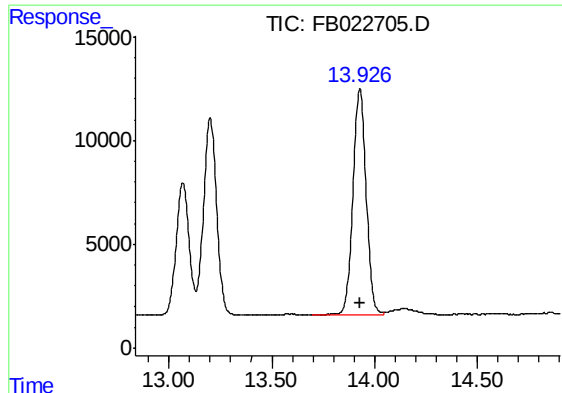

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: 0.000 min
Response: 488411
Conc: 13.92 ng/ml

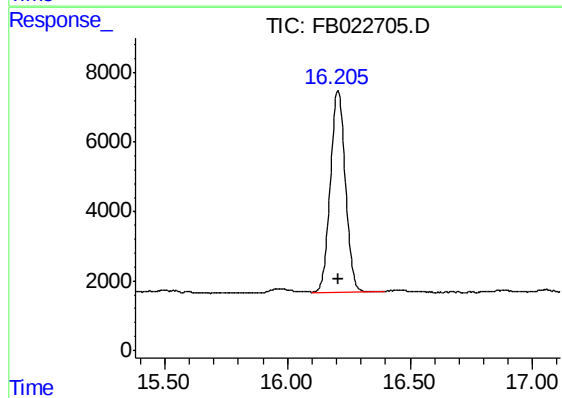

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: 0.000 min
Response: 248696
Conc: 9.06 ng/ml