

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101022\
Data File : FB028576.D
Signal(s) : FID2B.CH
Acq On : 10 Oct 2022 19:18
Operator : AJ/MA
Sample : N5066-01
Misc : 2.50G/5.00 ML DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 11 07:34:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	61358	4.743 ng/ml
Target Compounds			
4) t Benzene	7.883	7473	0.340 ng/ml
6) t Toluene	10.638	6451	0.308 ng/ml
7) t Ethylbenzene	13.068	7219	0.364 ng/ml
8) t m-Xylene	13.195	8789	0.446 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101022\
Data File : FB028576.D
Signal(s) : FID2B.CH
Acq On : 10 Oct 2022 19:18
Operator : AJ/MA
Sample : N5066-01
Misc : 2.50G/5.00 ML DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 11 07:34:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

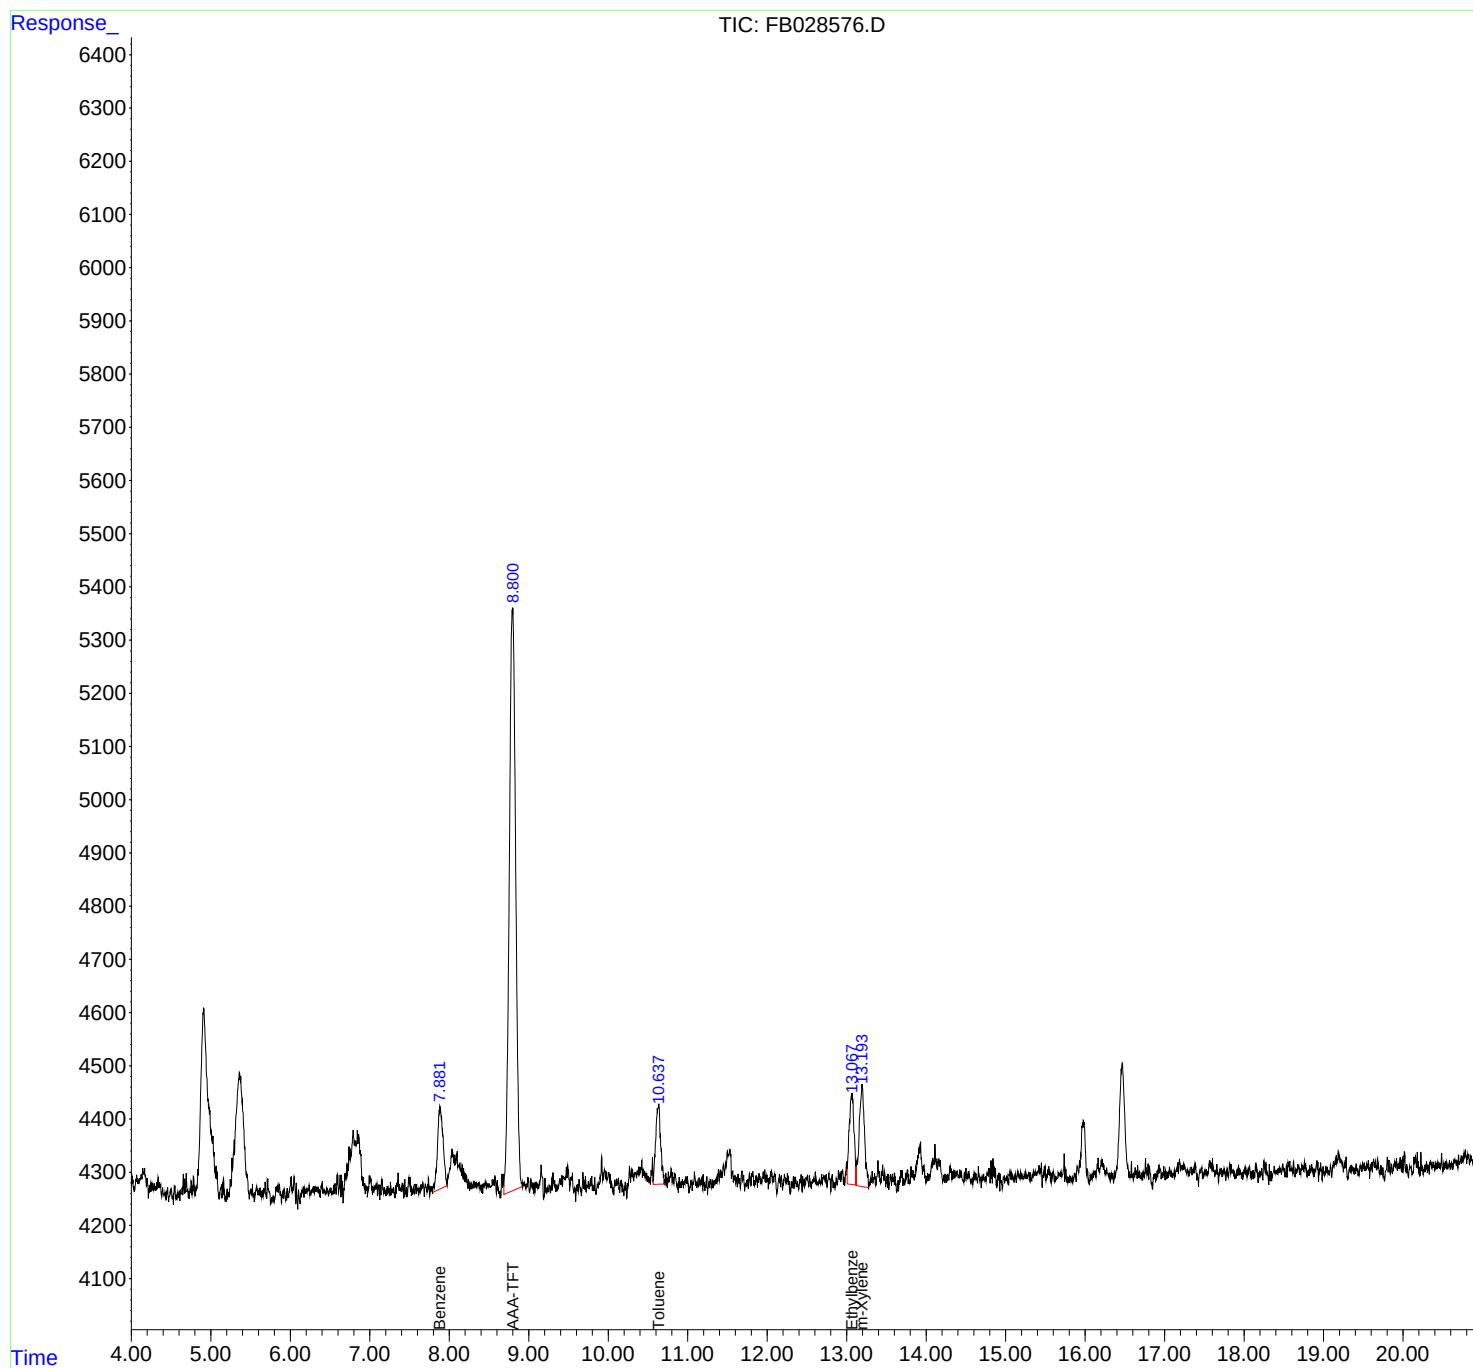


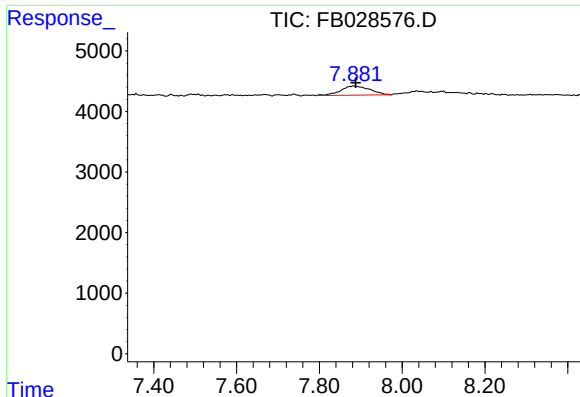

#4 Benzene


R.T.: 7.883 min
Delta R.T.: -0.005 min
Response: 7473
Conc: 0.34 ng/ml

Instrument :
FID_B
ClientSampleId :

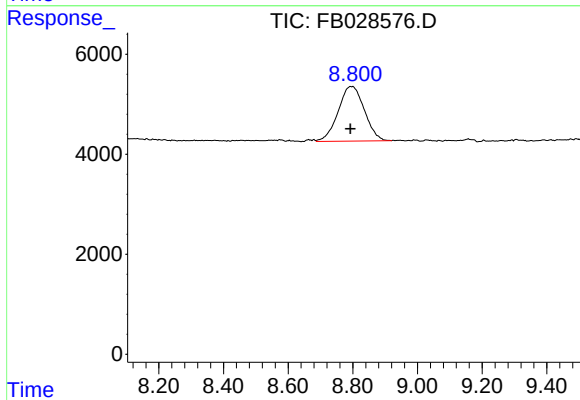


#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: 0.001 min
Response: 61358
Conc: 4.74 ng/ml

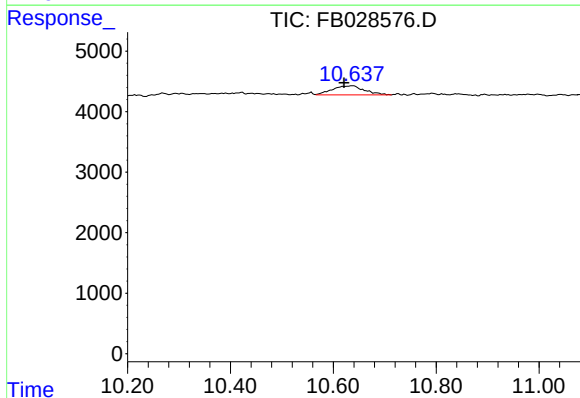


#6 Toluene

R.T.: 10.638 min
Delta R.T.: 0.017 min
Response: 6451
Conc: 0.31 ng/ml

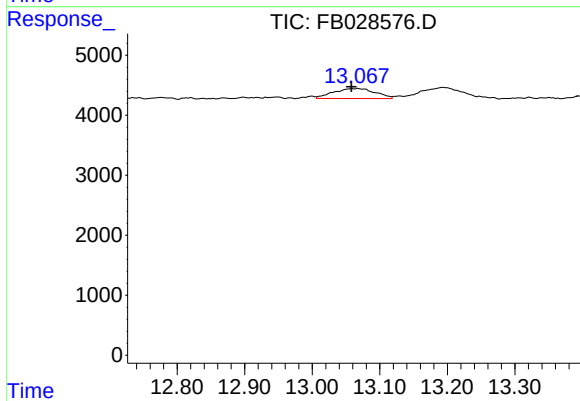

#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: 0.010 min
Response: 7219
Conc: 0.36 ng/ml

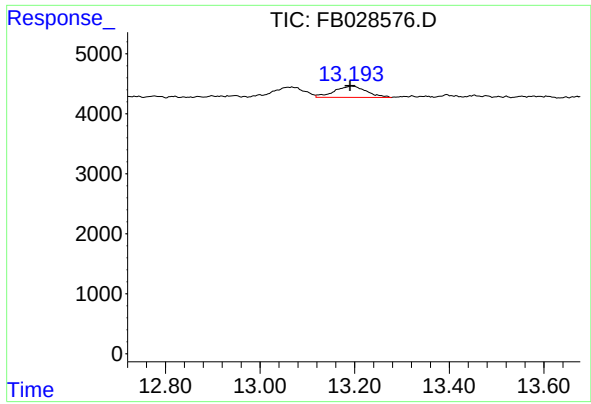

#8 m-Xylene

R.T.: 13.195 min
Delta R.T.: 0.004 min
Response: 8789
Conc: 0.45 ng/ml

Instrument :
FID_B
ClientSampleId :