

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101022\
Data File : FB028577.D
Signal(s) : FID2B.CH
Acq On : 10 Oct 2022 19:57
Operator : AJ/MA
Sample : N5066-02
Misc : 2.12G/5.00 ML DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 11 07:34:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	102508	7.924 ng/ml
Target Compounds			
8) t m-Xylene	13.209	1940	0.098 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101022\
Data File : FB028577.D
Signal(s) : FID2B.CH
Acq On : 10 Oct 2022 19:57
Operator : AJ/MA
Sample : N5066-02
Misc : 2.12G/5.00 ML DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 11 07:34:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

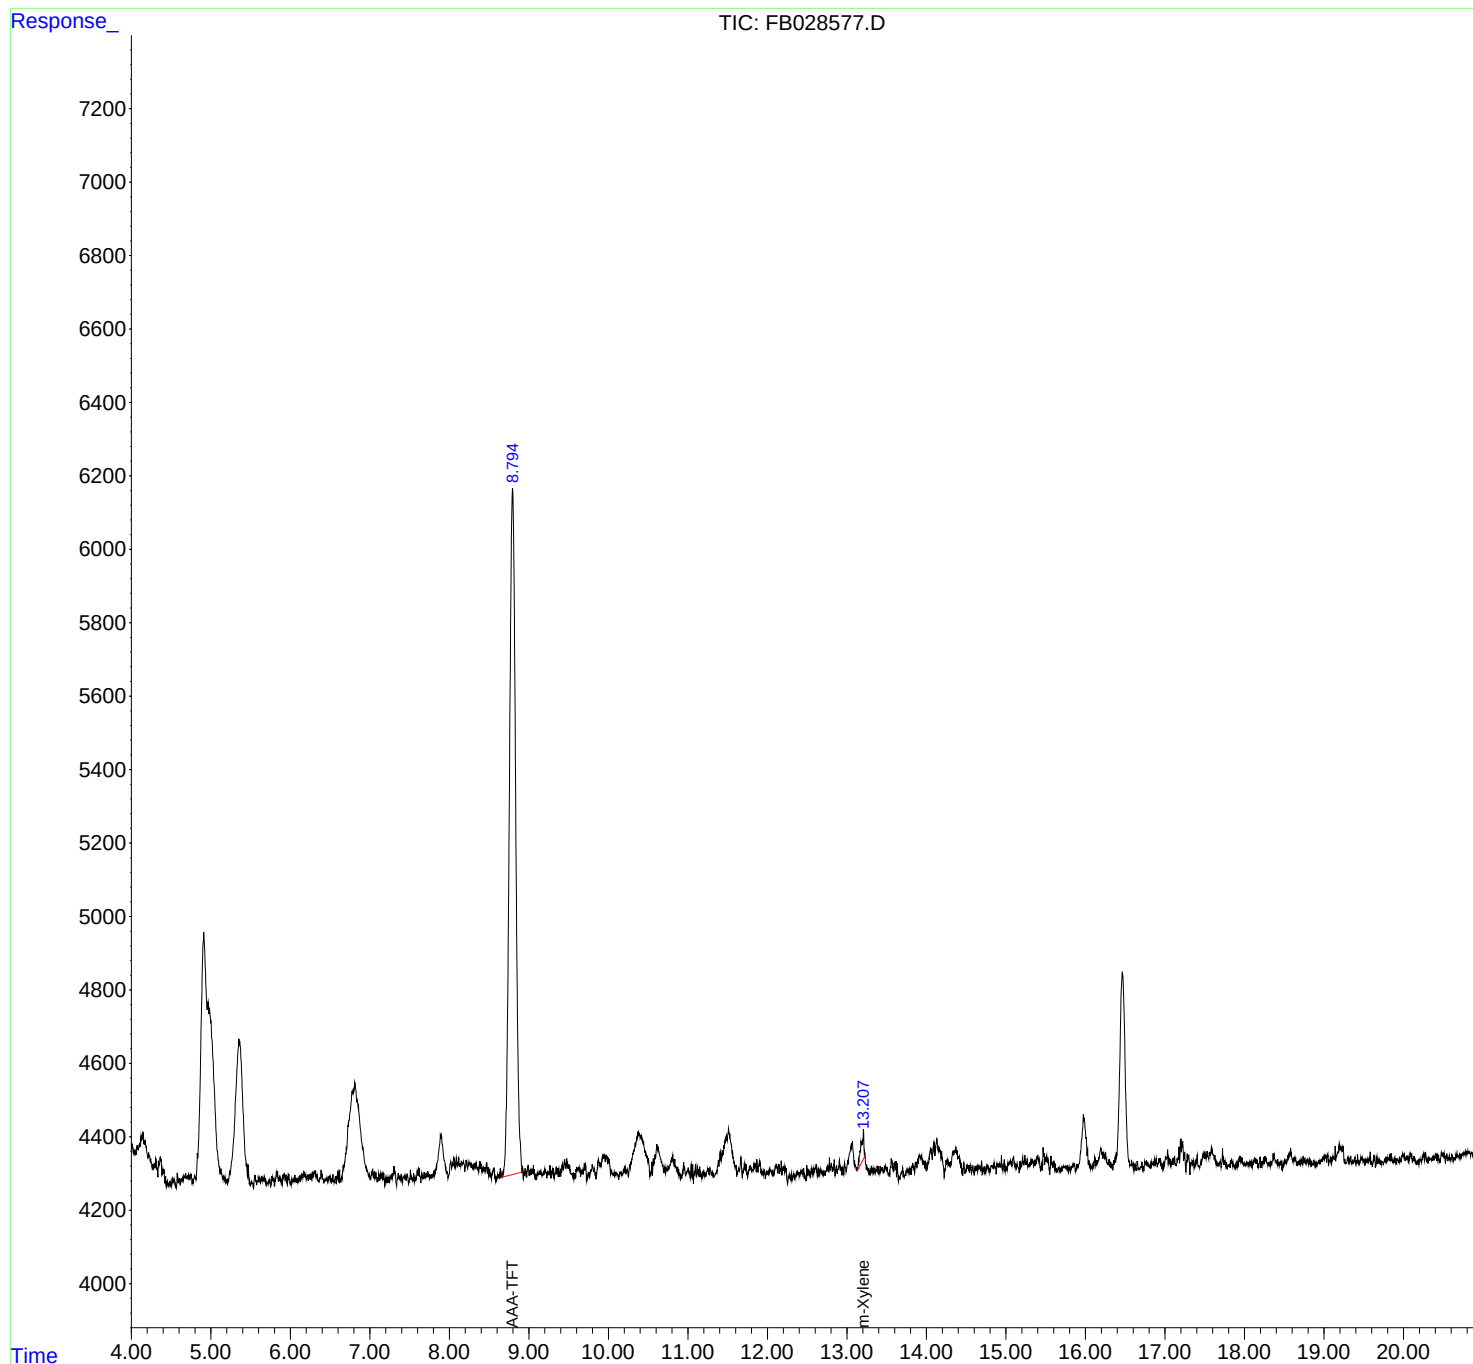


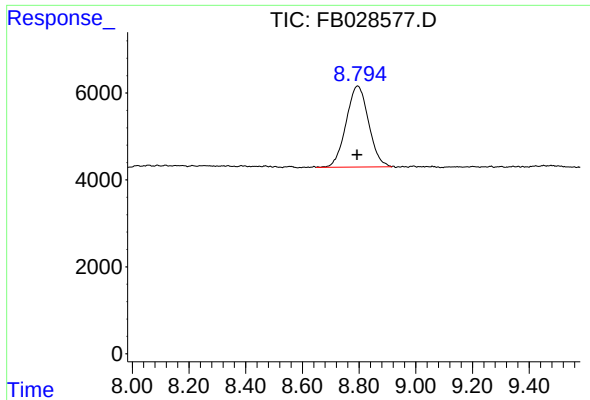

#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: 0.003 min
Response: 102508
Conc: 7.92 ng/ml

Instrument :
FID_B
ClientSampleId :

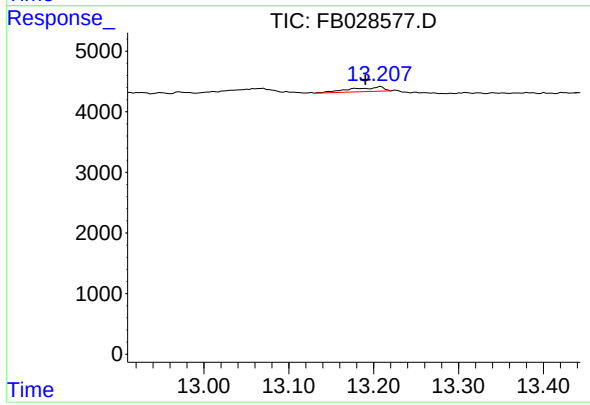

#8 m-Xylene

R.T.: 13.209 min
Delta R.T.: 0.018 min
Response: 1940
Conc: 0.10 ng/ml