

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101022\
Data File : FB028580.D
Signal(s) : FID2B.CH
Acq On : 10 Oct 2022 21:55
Operator : AJ/MA
Sample : N5067-18
Misc : 2.56G/5.00 ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 11 07:34:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

4) t	Benzene	7.891	32494	1.479 ng/ml
7) t	Ethylbenzene	13.061	67191	3.386 ng/ml
8) t	m-Xylene	13.185	21905	1.112 ng/ml
9) t	O-Xylene	13.921	810	0.042 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101022\
Data File : FB028580.D
Signal(s) : FID2B.CH
Acq On : 10 Oct 2022 21:55
Operator : AJ/MA
Sample : N5067-18
Misc : 2.56G/5.00 ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 11 07:34:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

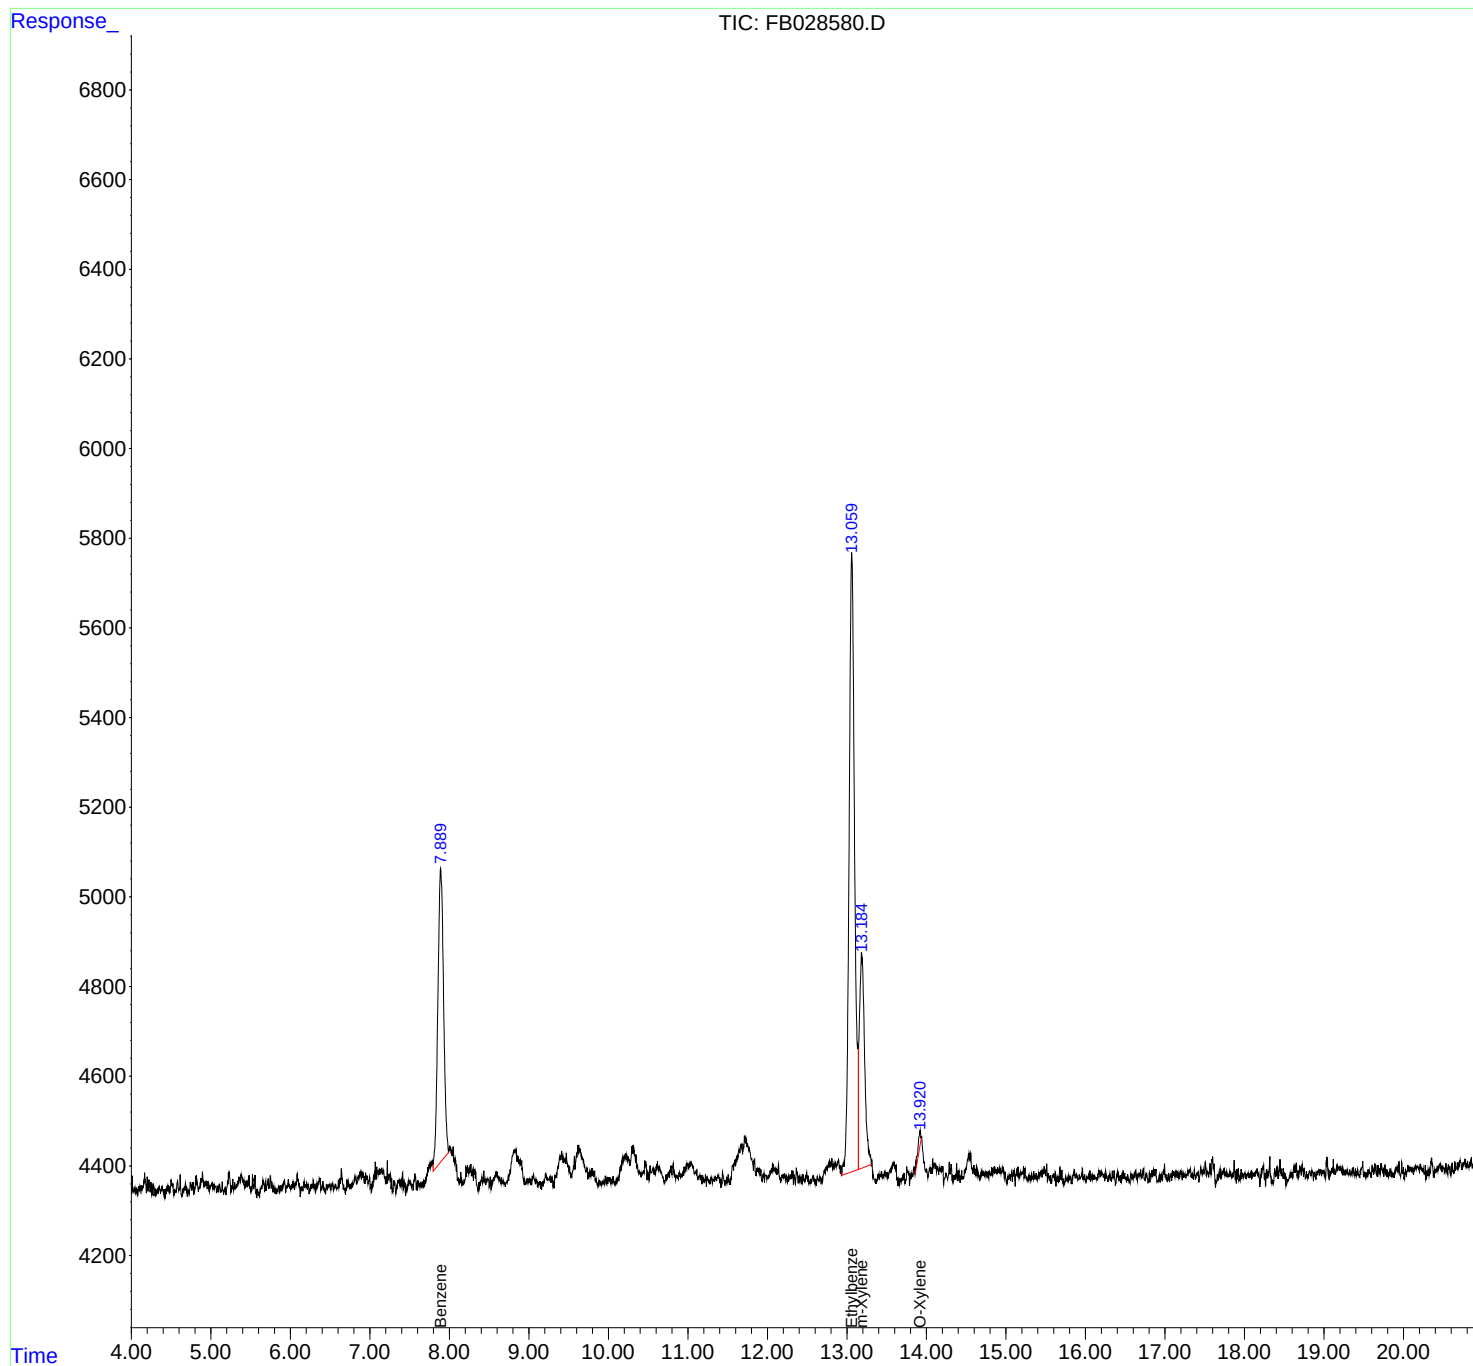


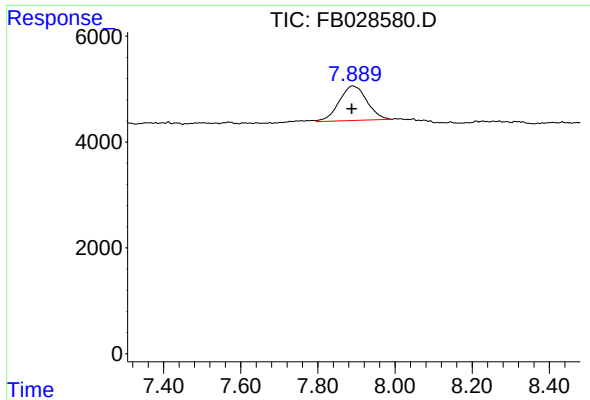

#4 Benzene


R.T.: 7.891 min
Delta R.T.: 0.003 min
Response: 32494
Conc: 1.48 ng/ml

Instrument :
FID_B
ClientSampleId :

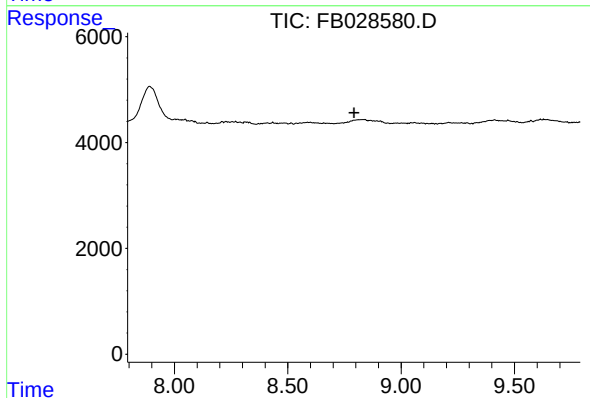


#5 AAA-TFT

R.T.: 0.000 min
Exp R.T. : 8.793 min
Response: 0
Conc: N.D.

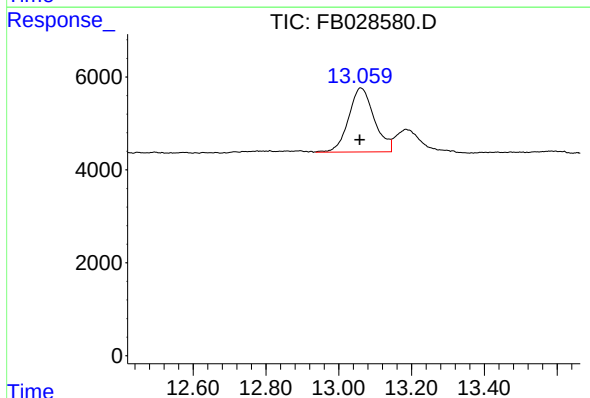


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: 0.003 min
Response: 67191
Conc: 3.39 ng/ml

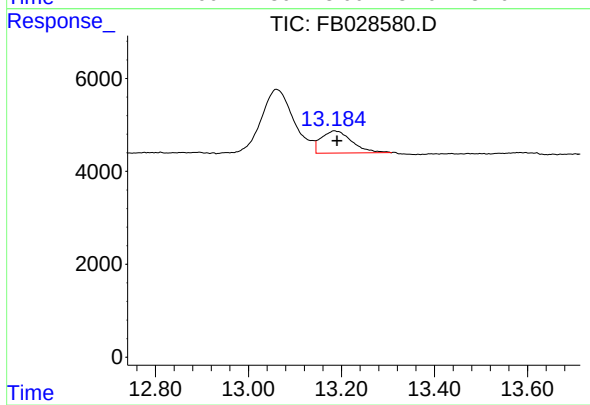

#8 m-Xylene

R.T.: 13.185 min
Delta R.T.: -0.005 min
Response: 21905
Conc: 1.11 ng/ml

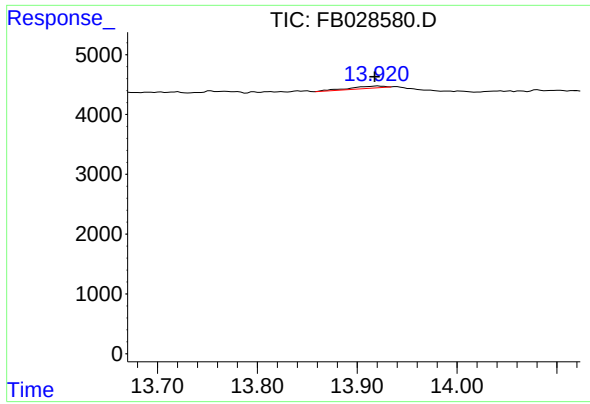

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: 0.004 min
Response: 810
Conc: 0.04 ng/ml

Instrument :
FID_B
ClientSampleId :