

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101022\
 Data File : FB028599.D
 Signal(s) : FID2B.CH
 Acq On : 11 Oct 2022 12:48
 Operator : AJ/MA
 Sample : N5067-20 50X
 Misc : 2.63G/5.00 ML DI MEOH
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 12 04:49:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	347753	26.880 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.734	23853	1.458 ng/ml
3) t n-Heptane	7.746	270951	15.996 ng/ml
4) t Benzene	7.886	159333	7.254 ng/ml
6) t Toluene	10.621	976605	46.594 ng/ml
7) t Ethylbenzene	13.059	2477816	124.850 ng/ml
8) t m-Xylene	13.189	4506234	228.732 ng/ml
9) t O-Xylene	13.918	1578484	81.136 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	1962648	101.381 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101022\
Data File : FB028599.D
Signal(s) : FID2B.CH
Acq On : 11 Oct 2022 12:48
Operator : AJ/MA
Sample : N5067-20 50X
Misc : 2.63G/5.00 ML DI MEOH
ALS Vial : 40 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 12 04:49:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

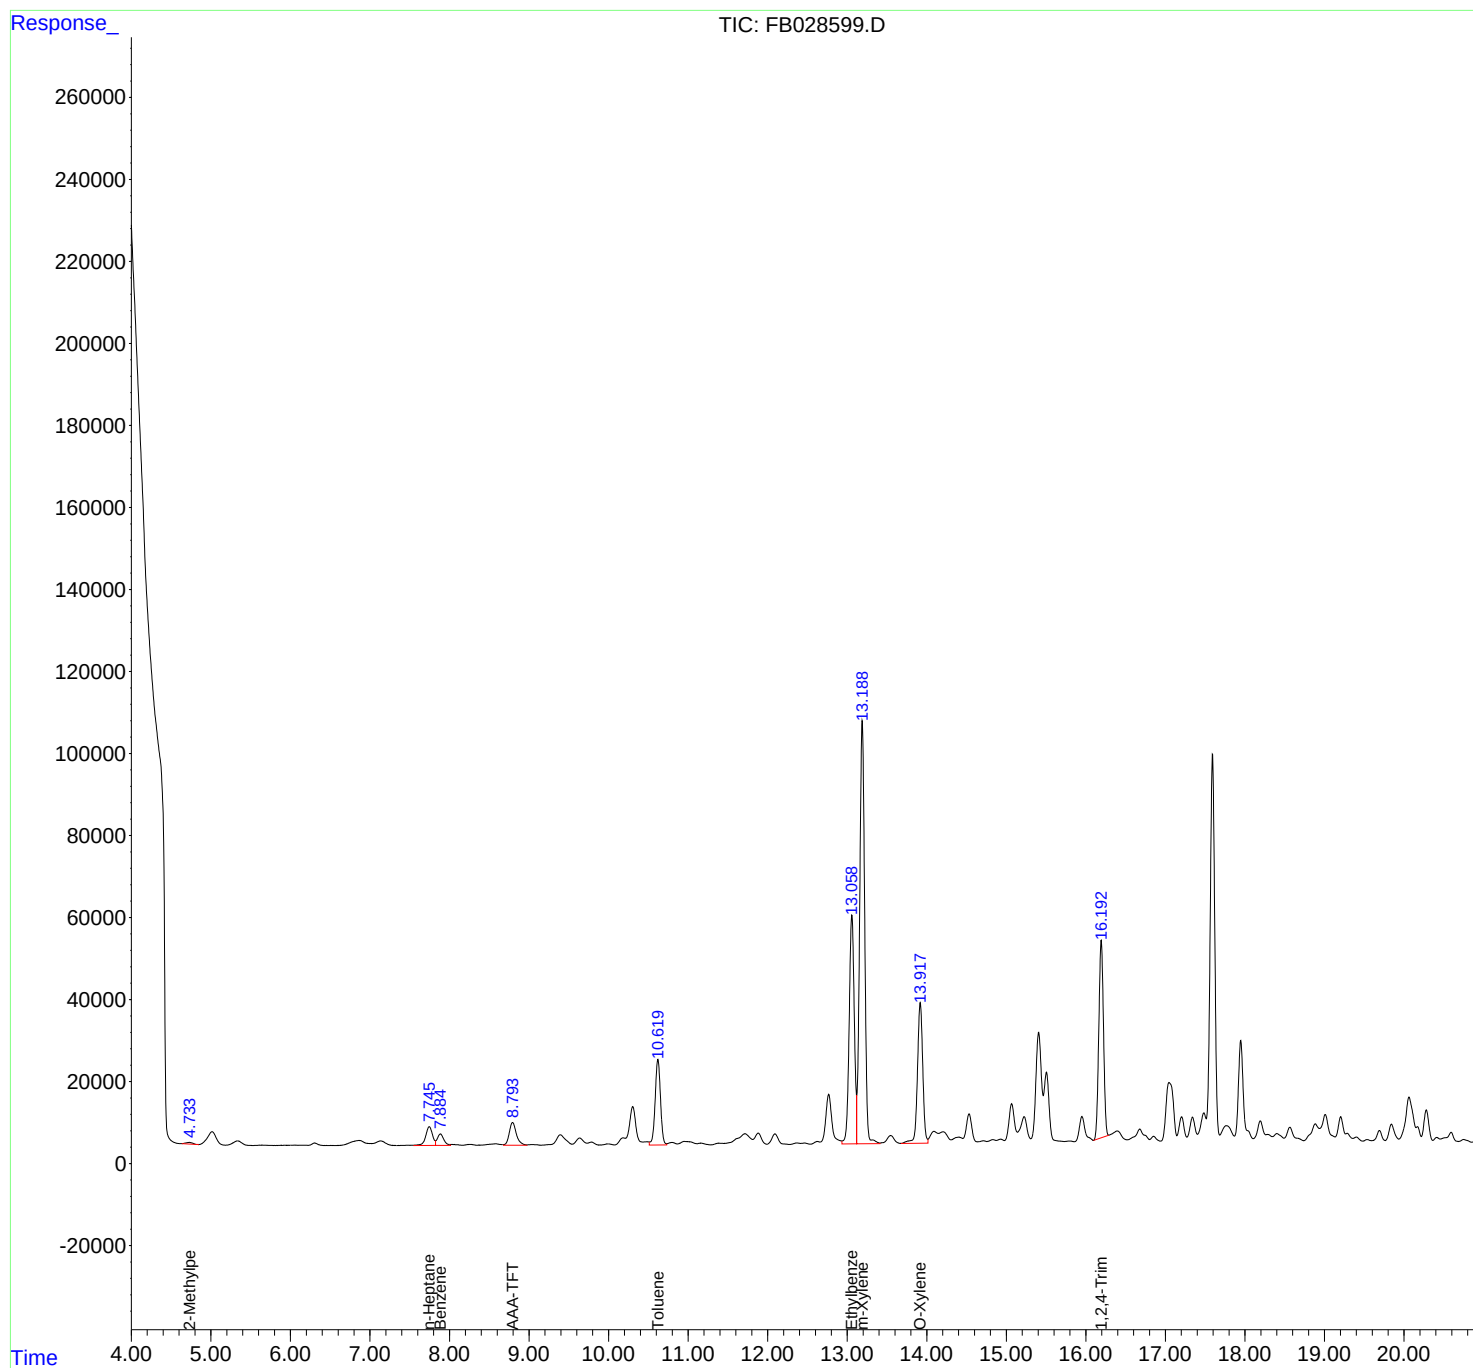


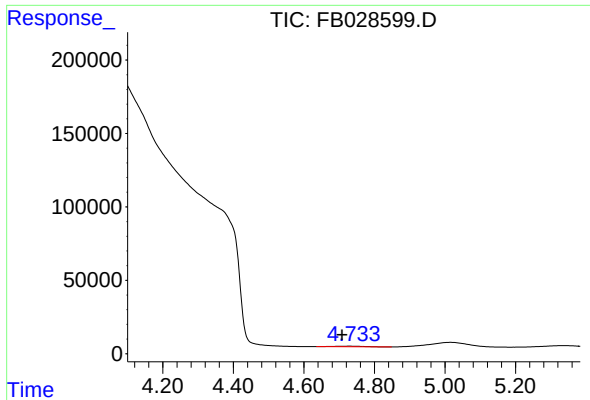

#1 2-Methylpentane


R.T.: 4.734 min
Delta R.T.: 0.026 min
Response: 23853
Conc: 1.46 ng/ml

Instrument :
FID_B
ClientSampleId :

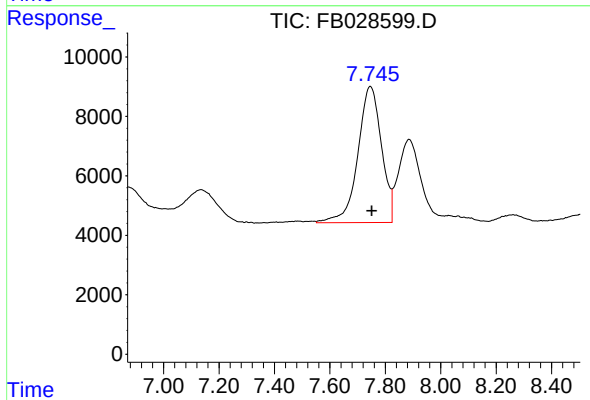


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: -0.005 min
Response: 270951
Conc: 16.00 ng/ml

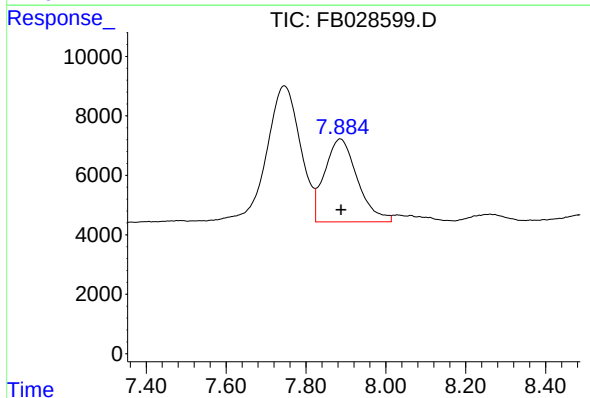


#4 Benzene

R.T.: 7.886 min
Delta R.T.: -0.002 min
Response: 159333
Conc: 7.25 ng/ml

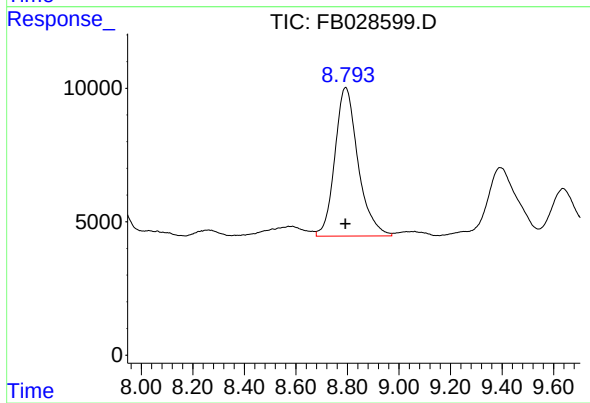

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.000 min
Response: 347753
Conc: 26.88 ng/ml

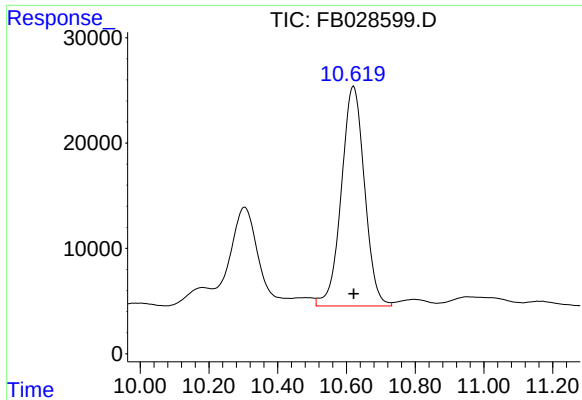

#6 Toluene


R.T.: 10.621 min
Delta R.T.: 0.000 min
Response: 976605
Conc: 46.59 ng/ml

Instrument :
FID_B
ClientSampleId :

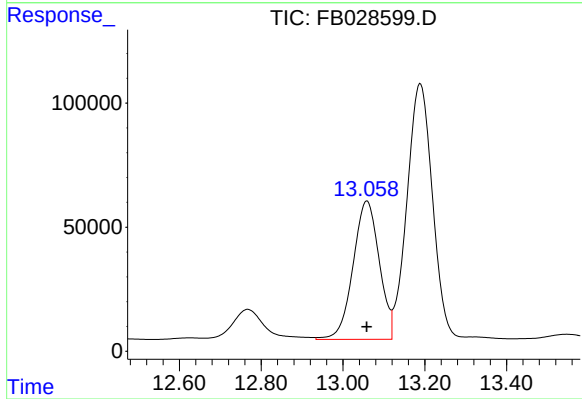


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.000 min
Response: 2477816
Conc: 124.85 ng/ml

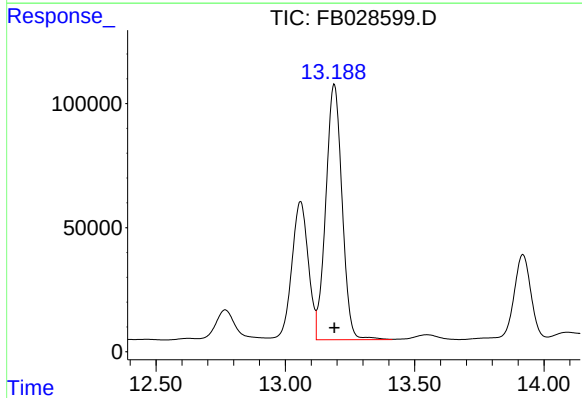


#8 m-Xylene

R.T.: 13.189 min
Delta R.T.: -0.001 min
Response: 4506234
Conc: 228.73 ng/ml

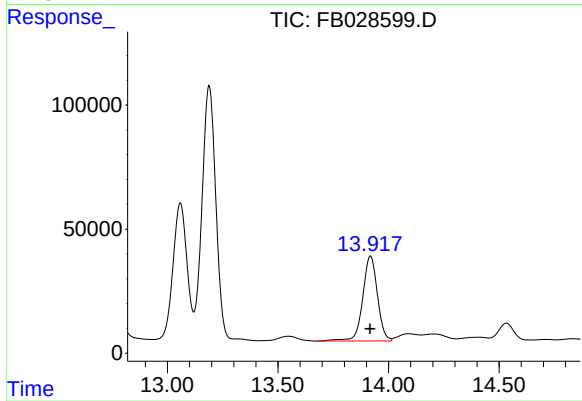

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.000 min
Response: 1578484
Conc: 81.14 ng/ml

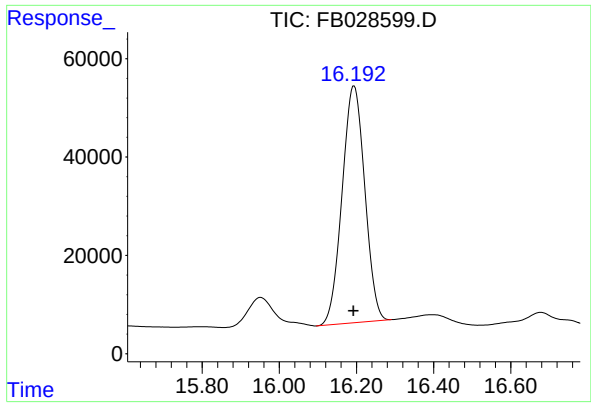

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min

Delta R.T.: 0.001 min

Response: 1962648

Conc: 101.38 ng/ml

Instrument :

FID_B

ClientSampleId :