

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101022\
 Data File : FB028582.D
 Signal(s) : FID2B.CH
 Acq On : 10 Oct 2022 23:14
 Operator : AJ/MA
 Sample : BSF1010S3
 Misc : 2.50G/5.00 ML DI WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1010S3

Integration File: SAMPLE.e
 Quant Time: Oct 11 07:35:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	243595	18.829 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	578393	35.356 ng/ml
2) t 2,2,4-Trimethylpentane	7.426	596756	33.021 ng/ml
3) t n-Heptane	7.751	196397	11.595 ng/ml
4) t Benzene	7.888	237214	10.800 ng/ml
6) t Toluene	10.620	673540	32.134 ng/ml
7) t Ethylbenzene	13.057	217033	10.936 ng/ml
8) t m-Xylene	13.190	414845	21.057 ng/ml
9) t O-Xylene	13.917	404126	20.773 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	395582	20.434 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101022\
Data File : FB028582.D
Signal(s) : FID2B.CH
Acq On : 10 Oct 2022 23:14
Operator : AJ/MA
Sample : BSF1010S3
Misc : 2.50G/5.00 ML DI WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1010S3

Integration File: SAMPLE.e
Quant Time: Oct 11 07:35:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

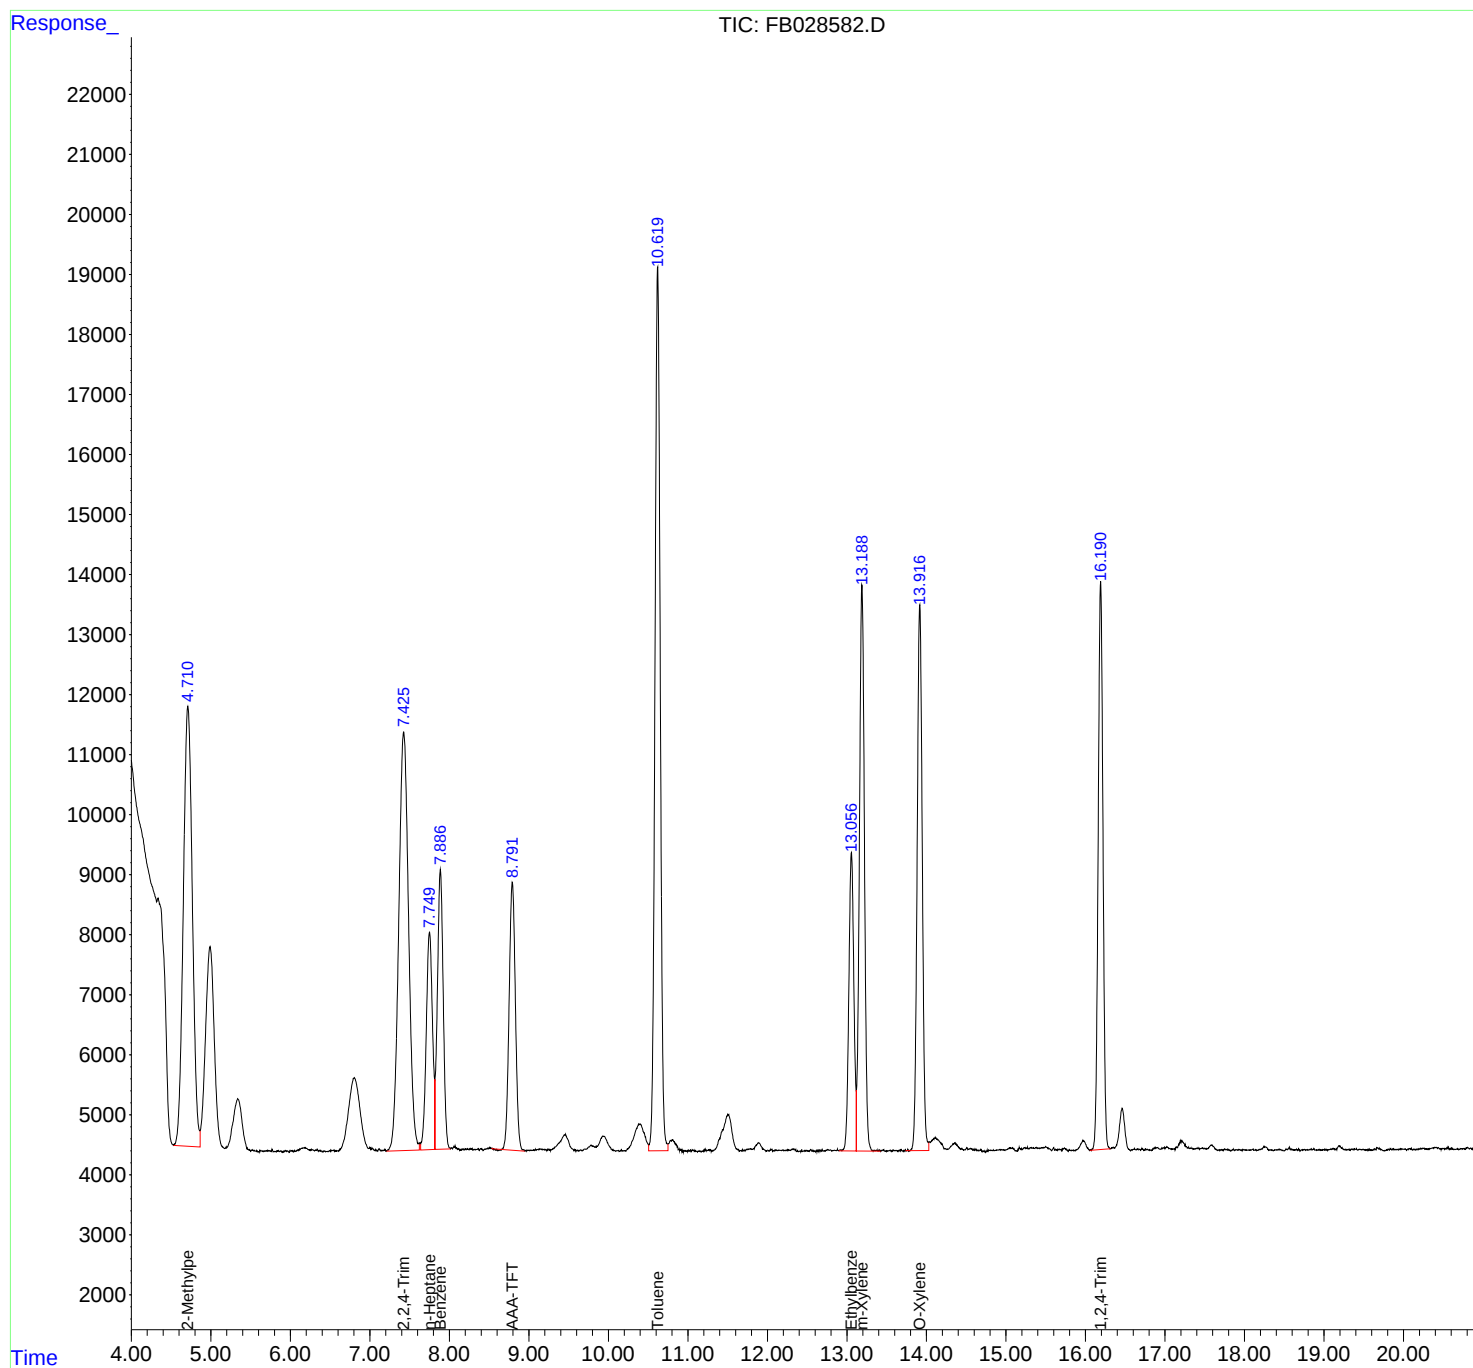


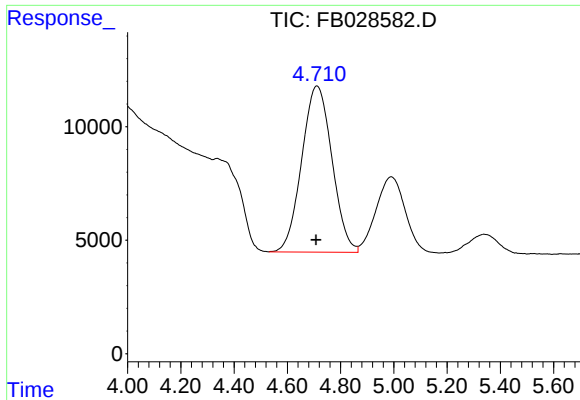

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: 0.004 min
Response: 578393
Conc: 35.36 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1010S3

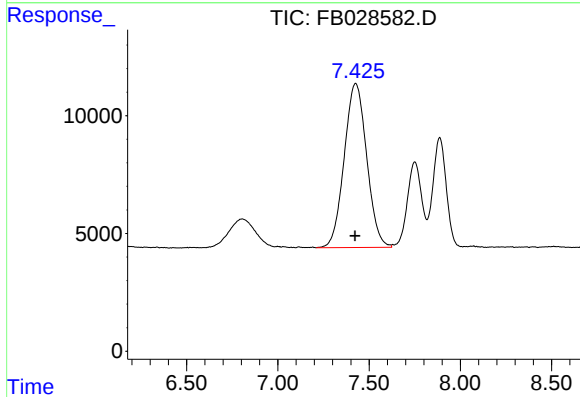


#2 2,2,4-Trimethylpentane

R.T.: 7.426 min
Delta R.T.: 0.003 min
Response: 596756
Conc: 33.02 ng/ml

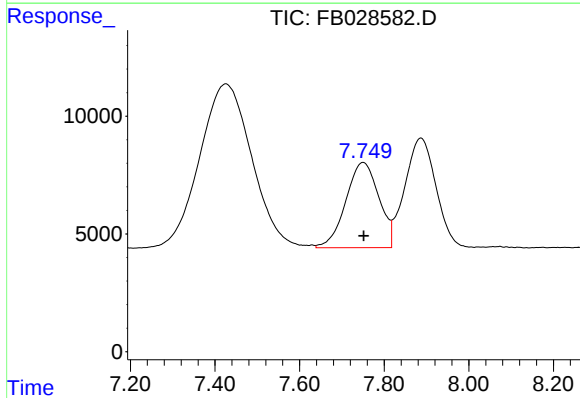


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.000 min
Response: 196397
Conc: 11.59 ng/ml

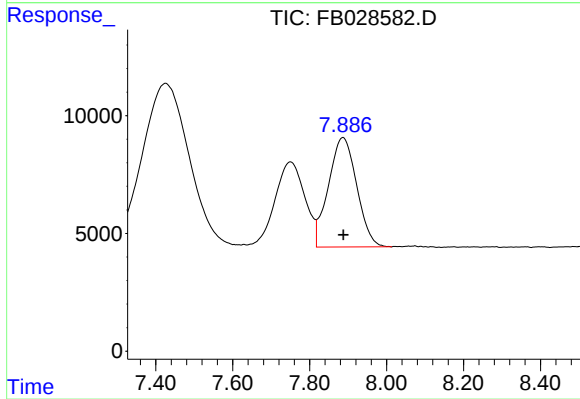

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.000 min
Response: 237214
Conc: 10.80 ng/ml

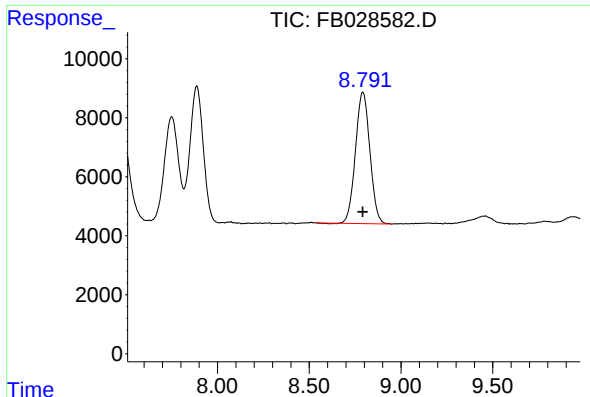

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 243595
Conc: 18.83 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1010S3

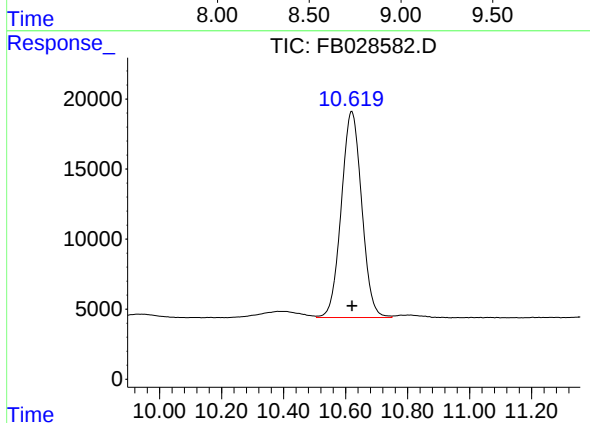


#6 Toluene

R.T.: 10.620 min
Delta R.T.: -0.001 min
Response: 673540
Conc: 32.13 ng/ml

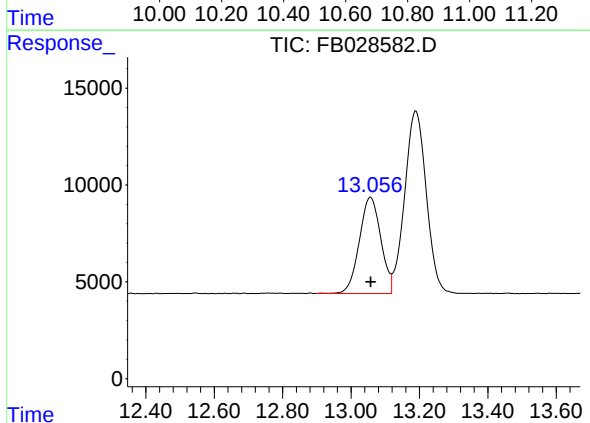


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.000 min
Response: 217033
Conc: 10.94 ng/ml

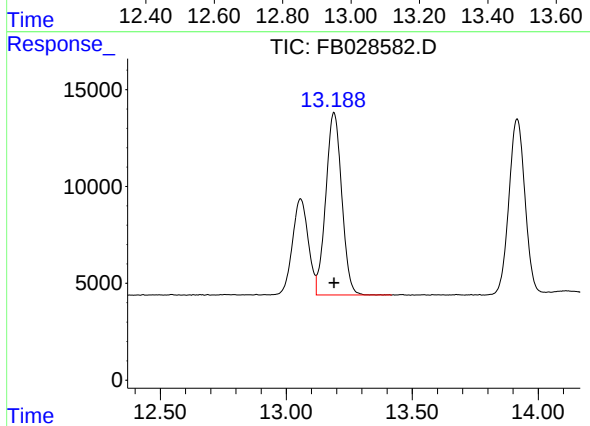

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.000 min
Response: 414845
Conc: 21.06 ng/ml

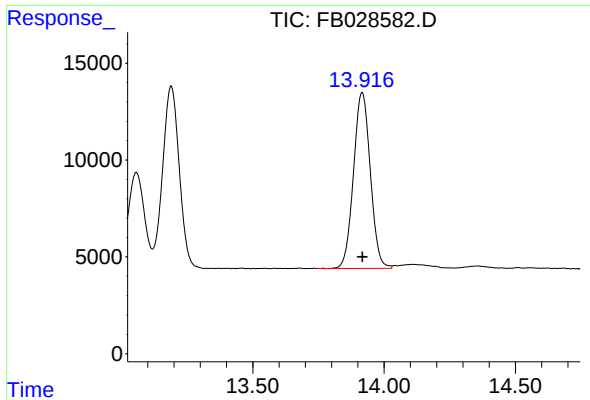

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.000 min
Response: 404126
Conc: 20.77 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1010S3

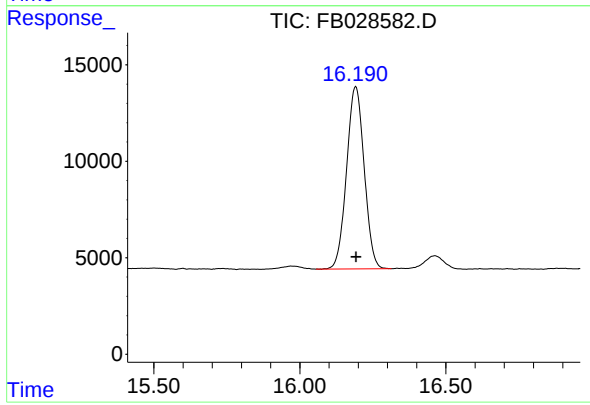

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: -0.001 min
Response: 395582
Conc: 20.43 ng/ml