

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101023\
 Data File : FB030405.D
 Signal(s) : FID2B.CH
 Acq On : 10 Oct 2023 12:12
 Operator : YP/AJ
 Sample : FB101023GROICV
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 FB101023GROICV

Integration File: Calibration.e
 Quant Time: Oct 10 12:16:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
 Quant Title :
 QLast Update : Tue Oct 10 11:38:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.787	236941	20.752 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	393934	28.156 ng/ml
2) t 2,2,4-Trimethylpentane	7.411	435360	26.369 ng/ml
3) t n-Heptane	7.748	146918	9.802 ng/ml
4) t Benzene	7.883	190774	9.298 ng/ml
6) t Toluene	10.615	559645	27.720 ng/ml
7) t Ethylbenzene	13.051	183024	9.169 ng/ml
8) t m-Xylene	13.184	356901	18.108 ng/ml
9) t O-Xylene	13.910	344807	17.519 ng/ml
10) t 1,2,4-Trimethylbenzene	16.185	343944	16.649 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101023\
Data File : FB030405.D
Signal(s) : FID2B.CH
Acq On : 10 Oct 2023 12:12
Operator : YP/AJ
Sample : FB101023GROICV
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
FB101023GROICV

Integration File: Calibration.e
Quant Time: Oct 10 12:16:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
Quant Title :
QLast Update : Tue Oct 10 11:38:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

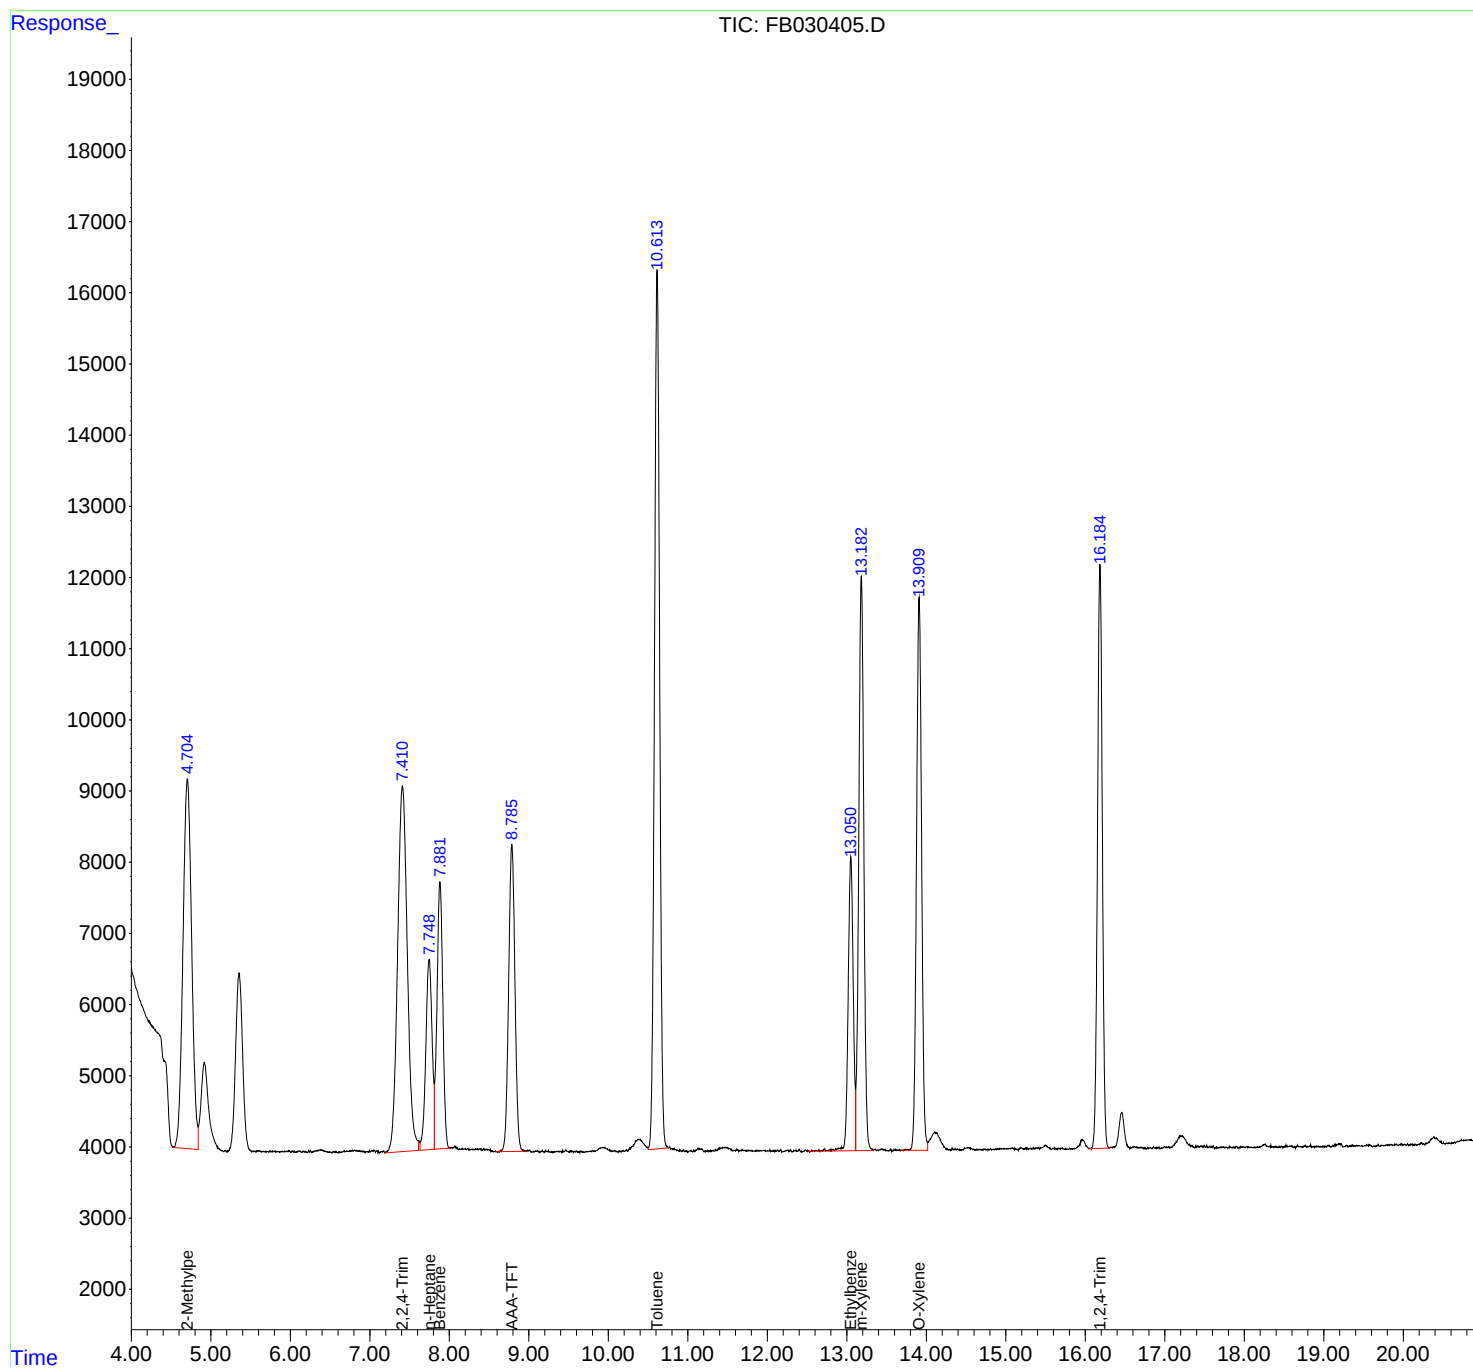


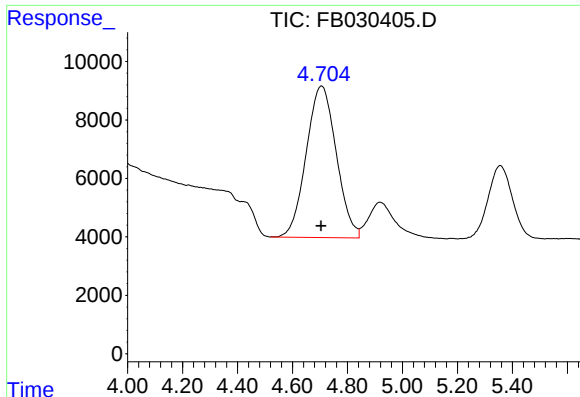

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: 0.002 min
Response: 393934
Conc: 28.16 ng/ml

Instrument :
FID_B
ClientSampleId :
FB101023GROICV

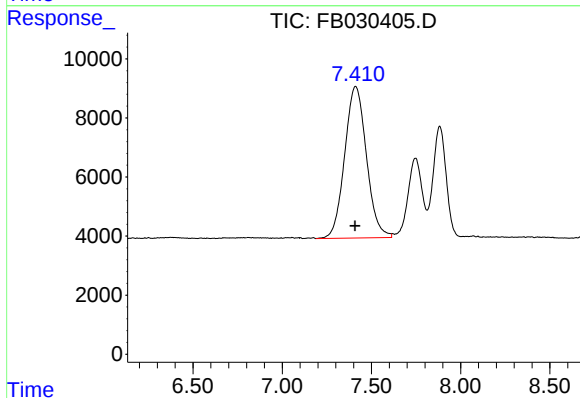


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min
Delta R.T.: 0.002 min
Response: 435360
Conc: 26.37 ng/ml

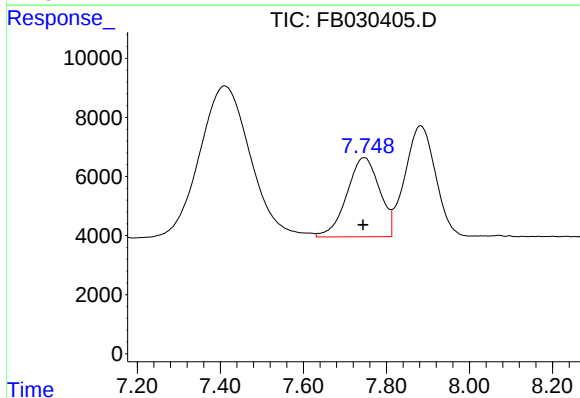


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: 0.004 min
Response: 146918
Conc: 9.80 ng/ml

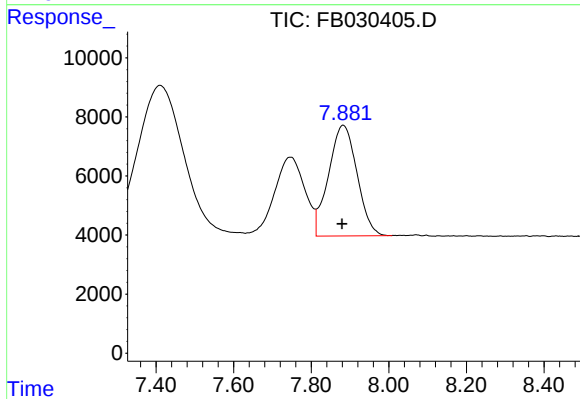

#4 Benzene


R.T.: 7.883 min
Delta R.T.: 0.003 min
Response: 190774
Conc: 9.30 ng/ml

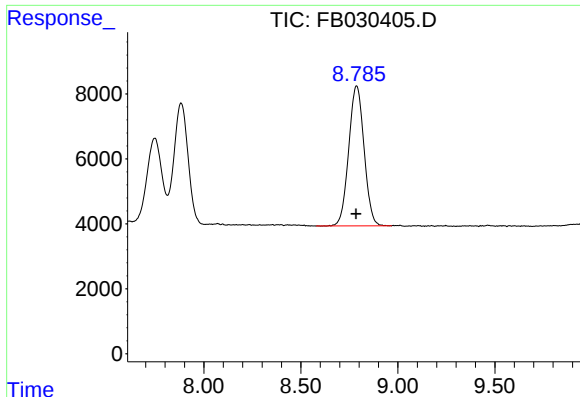

#5 AAA-TFT


R.T.: 8.787 min
Delta R.T.: 0.003 min
Response: 236941
Conc: 20.75 ng/ml

Instrument :
FID_B
ClientSampleId :
FB101023GROICV

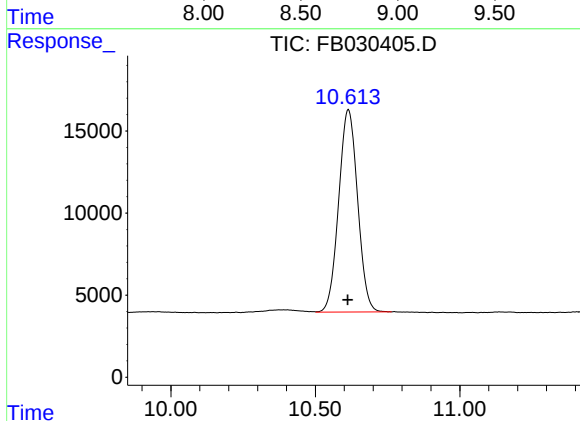


#6 Toluene

R.T.: 10.615 min
Delta R.T.: 0.002 min
Response: 559645
Conc: 27.72 ng/ml

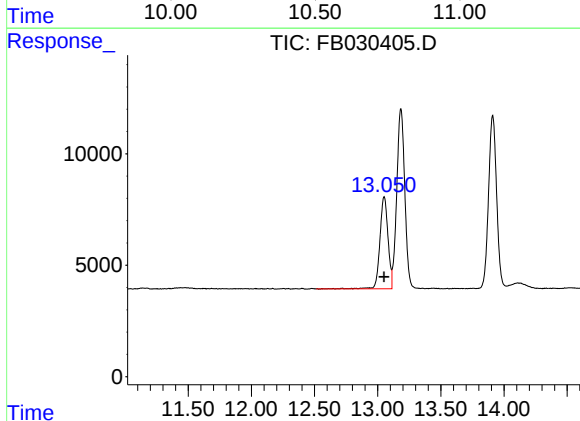


#7 Ethylbenzene

R.T.: 13.051 min
Delta R.T.: 0.002 min
Response: 183024
Conc: 9.17 ng/ml

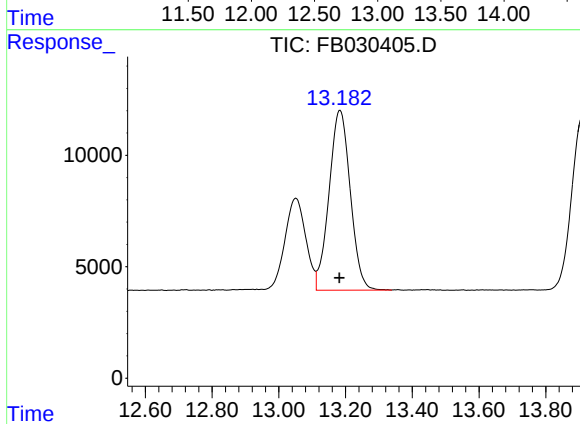

#8 m-Xylene


R.T.: 13.184 min
Delta R.T.: 0.002 min
Response: 356901
Conc: 18.11 ng/ml

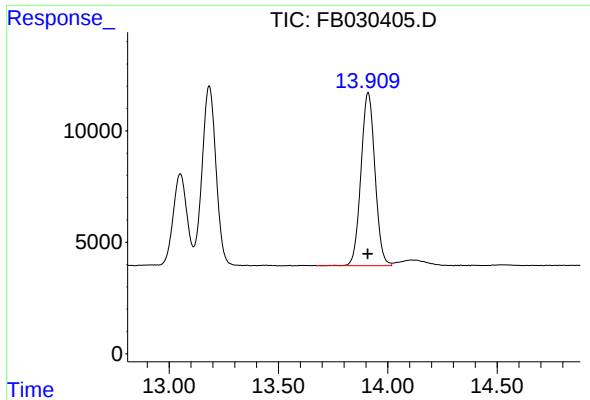

#9 O-Xylene

R.T.: 13.910 min
Delta R.T.: 0.002 min
Response: 344807
Conc: 17.52 ng/ml

Instrument :
FID_B
ClientSampleId :
FB101023GROICV

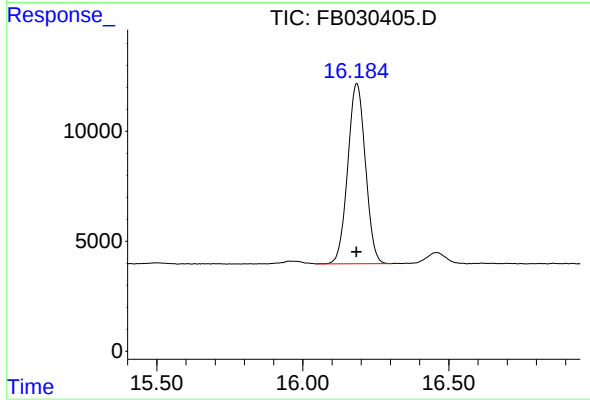

#10 1,2,4-Trimethylbenzene

R.T.: 16.185 min
Delta R.T.: 0.002 min
Response: 343944
Conc: 16.65 ng/ml