

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101024\
 Data File : FB030983.D
 Signal(s) : FID2B.CH
 Acq On : 10 Oct 2024 9:46
 Operator : YP/AJ
 Sample : VBF1010S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 11 04:31:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
 Quant Title :
 QLast Update : Fri Oct 04 11:53:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	490106	16.349 ng/ml
Target Compounds			
6) t Toluene	10.624	10151	0.188 ng/ml
7) t Ethylbenzene	13.048	5716	0.121 ng/ml
8) t m-Xylene	13.192	10183	0.195 ng/ml
9) t O-Xylene	13.927	13679	0.281 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	19922	0.608 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101024\
Data File : FB030983.D
Signal(s) : FID2B.CH
Acq On : 10 Oct 2024 9:46
Operator : YP/AJ
Sample : VBF1010S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 11 04:31:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
Quant Title :
QLast Update : Fri Oct 04 11:53:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

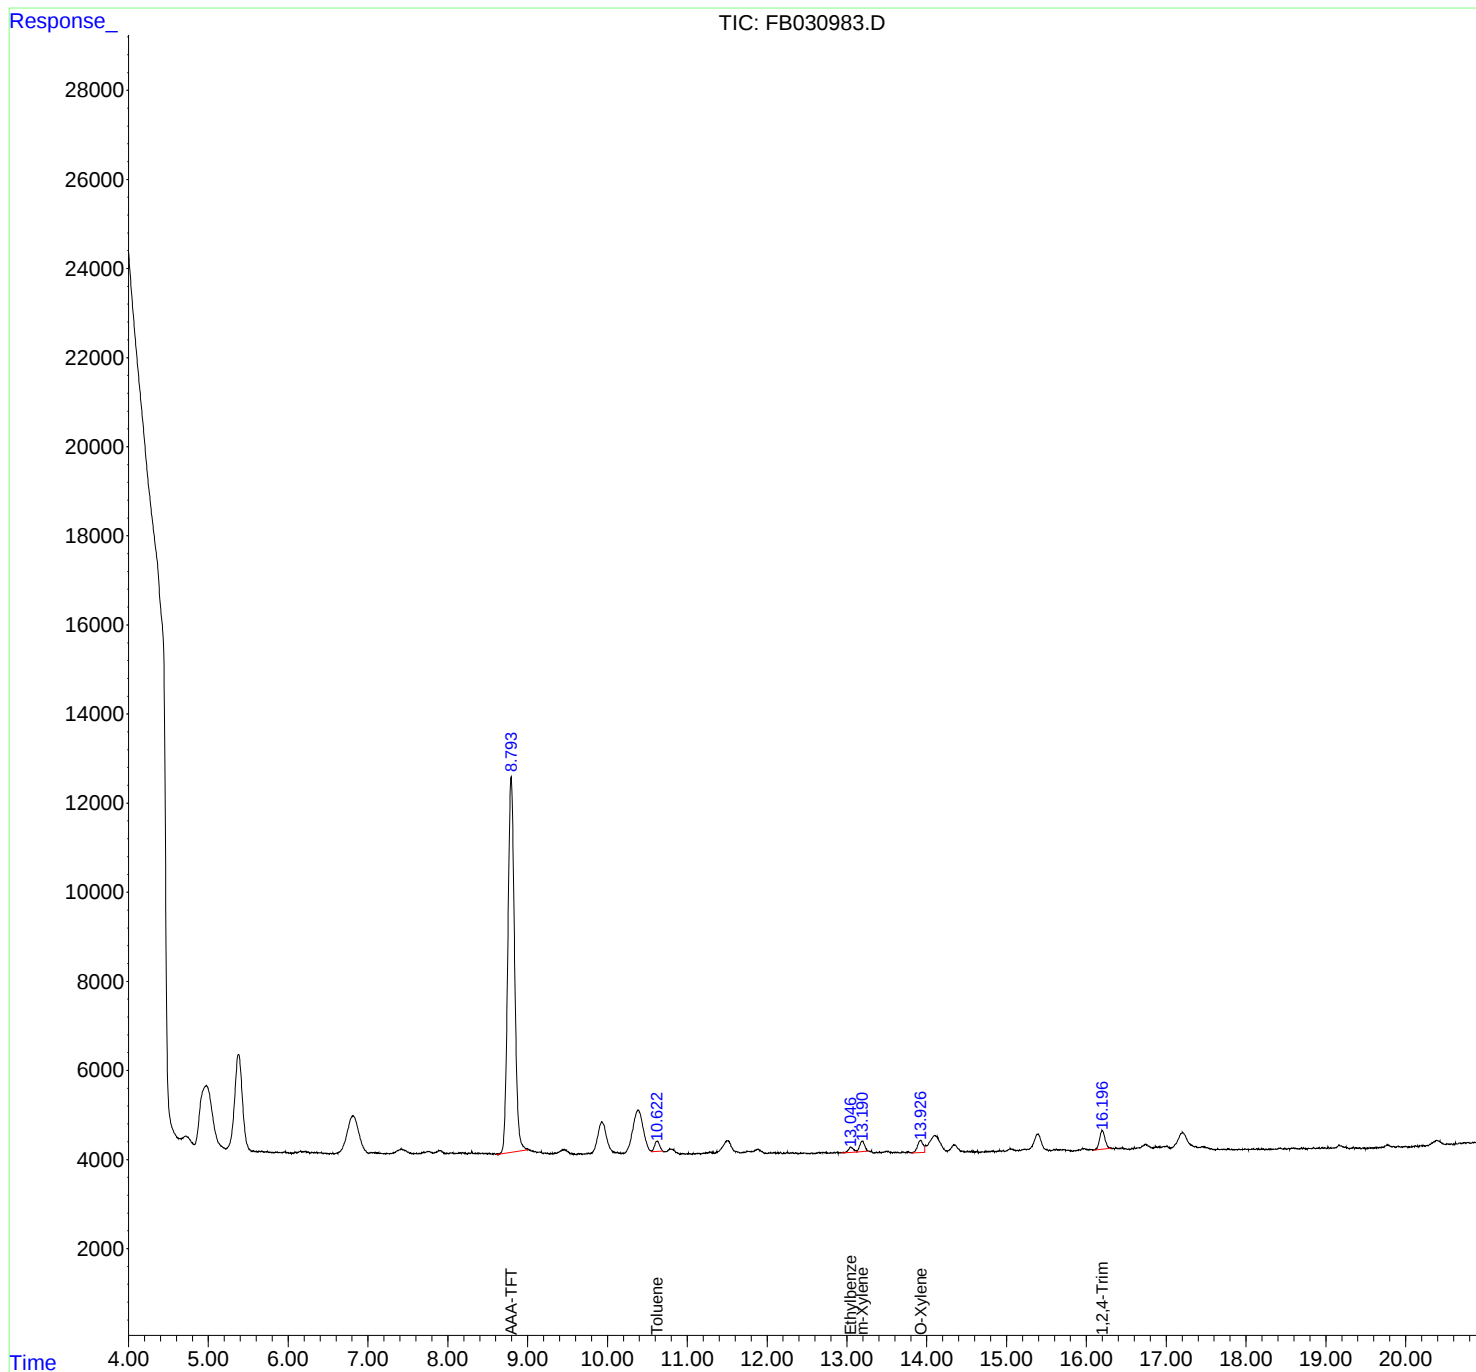


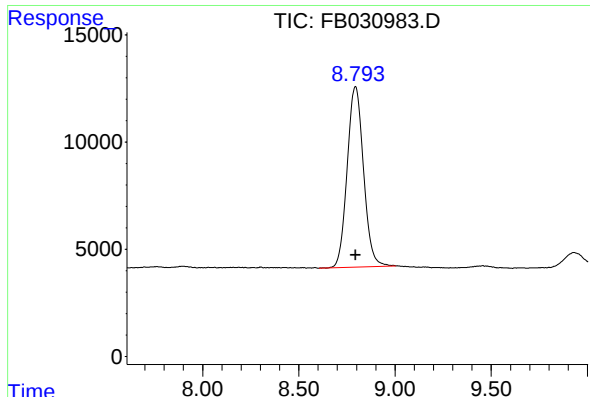

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: -0.001 min
Response: 490106
Conc: 16.35 ng/ml

Instrument :
FID_B
ClientSampleId :

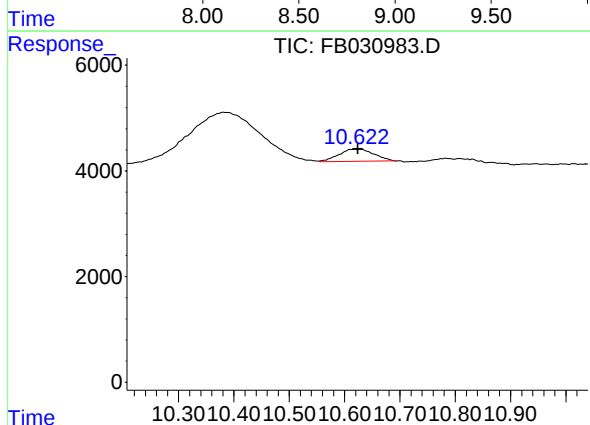


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.001 min
Response: 10151
Conc: 0.19 ng/ml

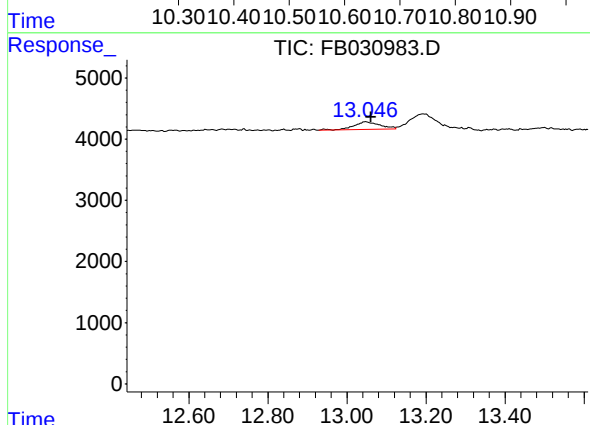


#7 Ethylbenzene

R.T.: 13.048 min
Delta R.T.: -0.012 min
Response: 5716
Conc: 0.12 ng/ml

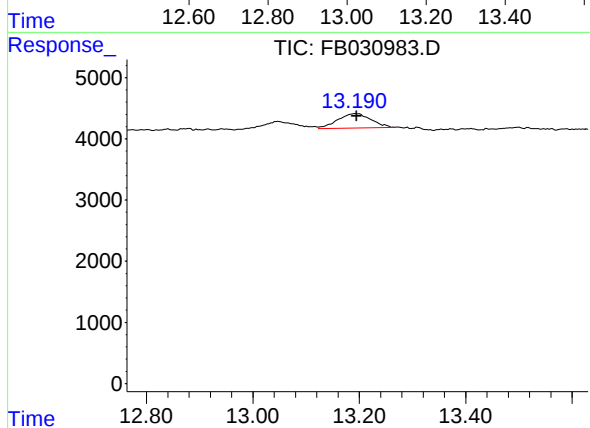

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: -0.003 min
Response: 10183
Conc: 0.20 ng/ml

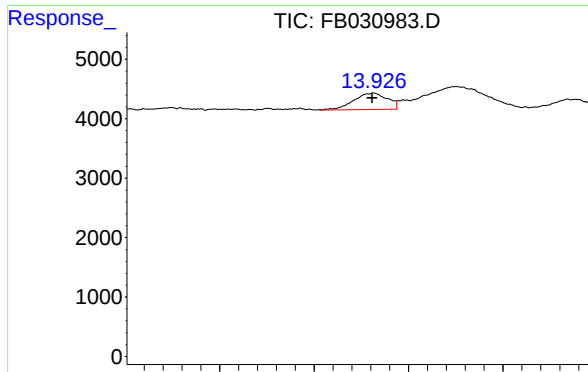

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: 0.005 min
Response: 13679
Conc: 0.28 ng/ml

Instrument :
FID_B
ClientSampleId :

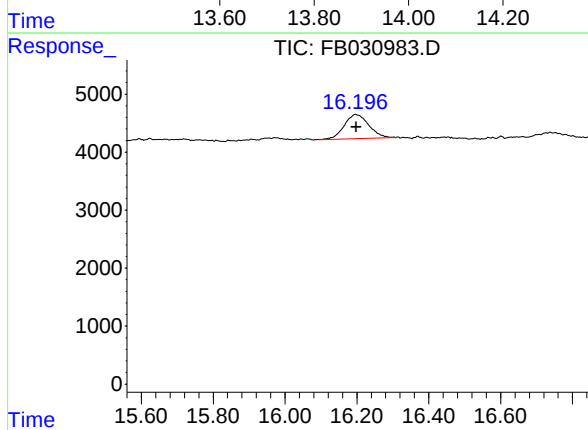

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: -0.001 min
Response: 19922
Conc: 0.61 ng/ml