

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101024\
 Data File : FB030985.D
 Signal(s) : FID2B.CH
 Acq On : 10 Oct 2024 10:40
 Operator : YP/AJ
 Sample : BSF1010S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1010S1

Integration File: Calibration.e
 Quant Time: Oct 11 04:31:51 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
 Quant Title :
 QLast Update : Fri Oct 04 11:53:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	431430	14.392 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.728	1082367	29.995 ng/ml
2) t 2,2,4-Trimethylpentane	7.431	1382392	29.009 ng/ml
3) t n-Heptane	7.757	446468	9.898 ng/ml
4) t Benzene	7.897	540199	9.828 ng/ml
6) t Toluene	10.625	1549594	28.686 ng/ml
7) t Ethylbenzene	13.061	459109	9.686 ng/ml
8) t m-Xylene	13.194	997233	19.116 ng/ml
9) t O-Xylene	13.922	933577	19.192 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	695324	21.220 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101024\
Data File : FB030985.D
Signal(s) : FID2B.CH
Acq On : 10 Oct 2024 10:40
Operator : YP/AJ
Sample : BSF1010S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1010S1

Integration File: Calibration.e
Quant Time: Oct 11 04:31:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
Quant Title :
QLast Update : Fri Oct 04 11:53:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

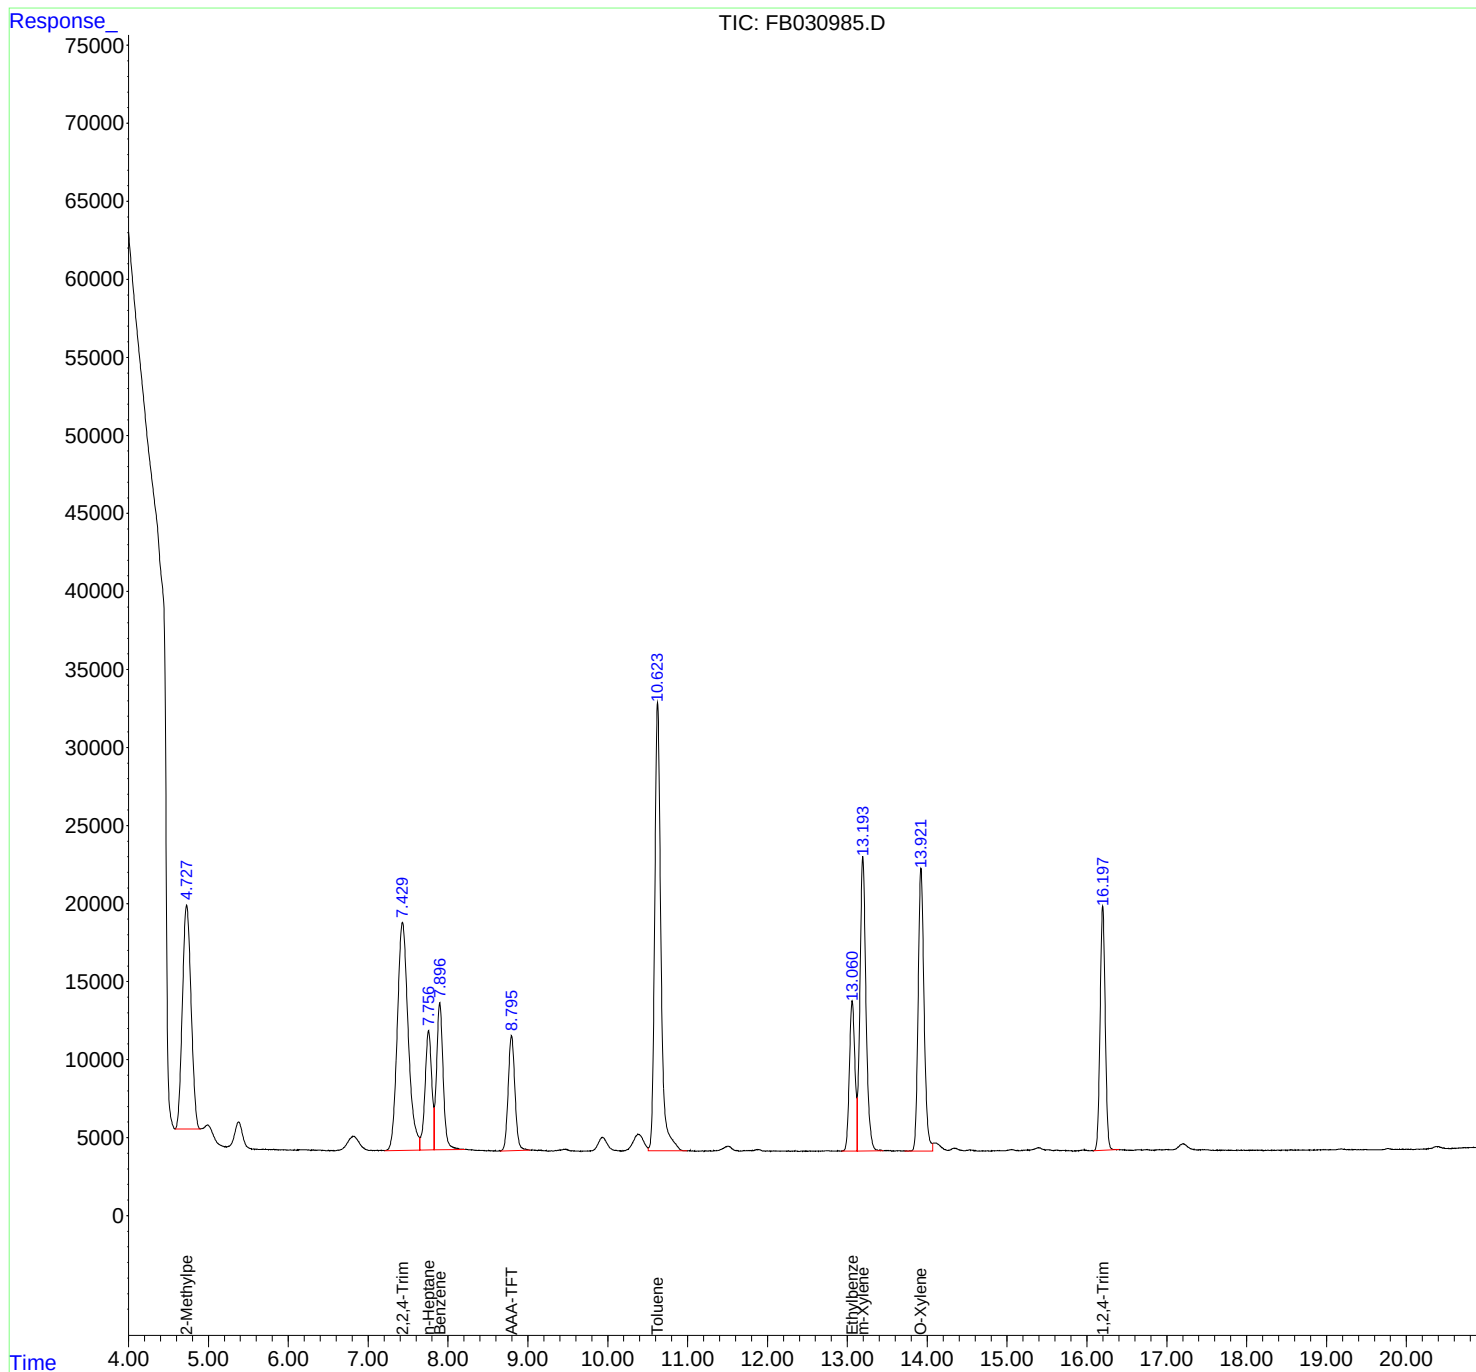


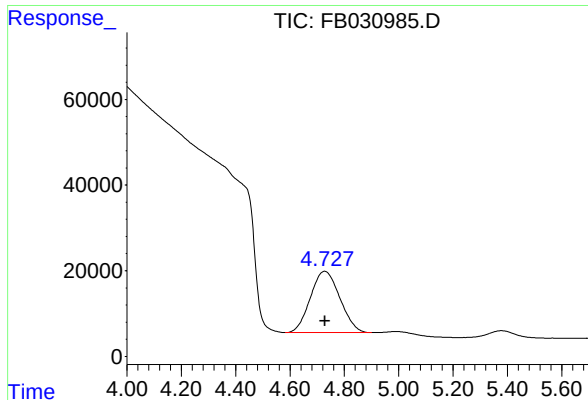

#1 2-Methylpentane


R.T.: 4.728 min
Delta R.T.: 0.000 min
Response: 1082367
Conc: 30.00 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1010S1

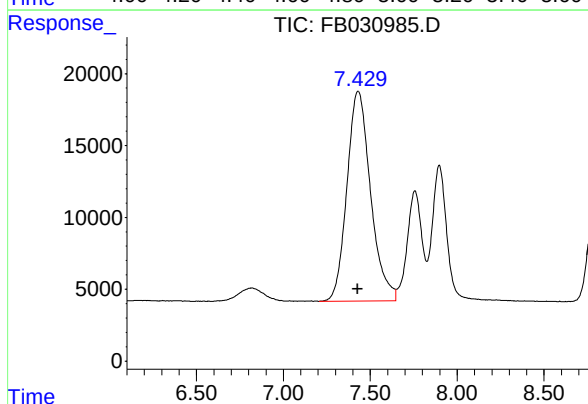


#2 2,2,4-Trimethylpentane

R.T.: 7.431 min
Delta R.T.: 0.003 min
Response: 1382392
Conc: 29.01 ng/ml

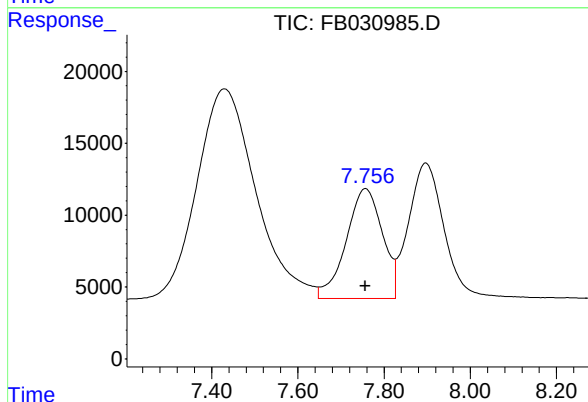


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 446468
Conc: 9.90 ng/ml

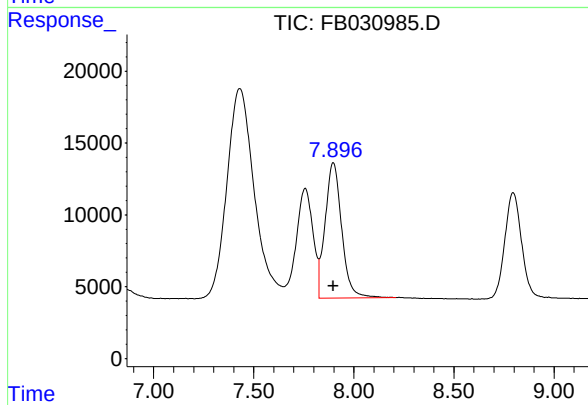

#4 Benzene


R.T.: 7.897 min
Delta R.T.: 0.000 min
Response: 540199
Conc: 9.83 ng/ml

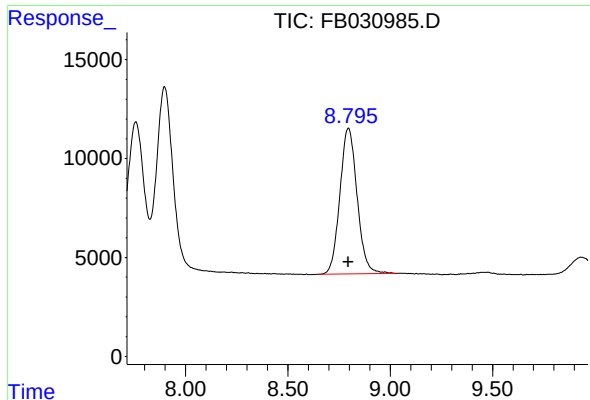

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: 0.000 min
Response: 431430
Conc: 14.39 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1010S1

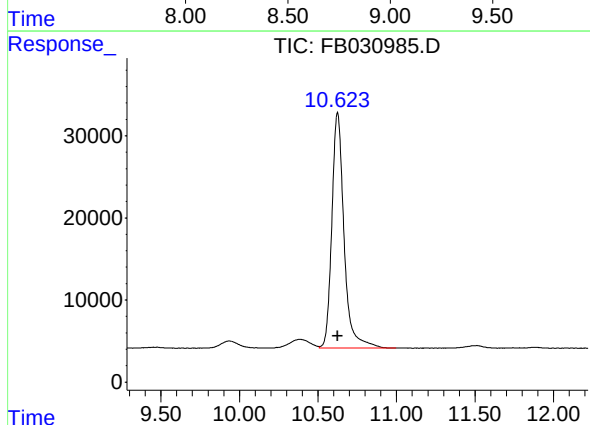


#6 Toluene

R.T.: 10.625 min
Delta R.T.: 0.000 min
Response: 1549594
Conc: 28.69 ng/ml

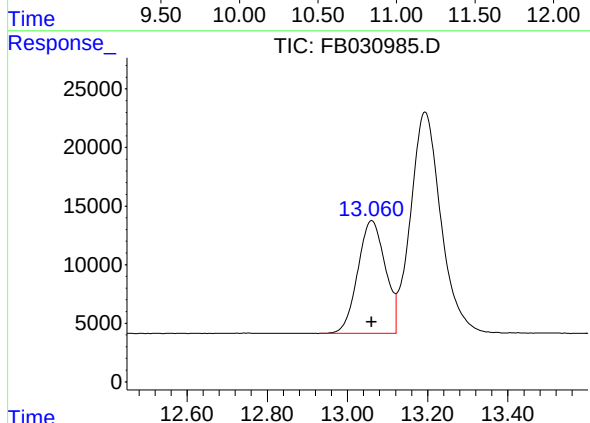


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: 0.000 min
Response: 459109
Conc: 9.69 ng/ml

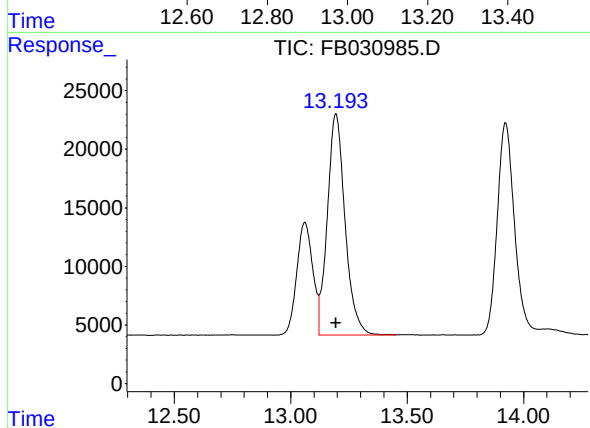

#8 m-Xylene


R.T.: 13.194 min
Delta R.T.: 0.000 min
Response: 997233
Conc: 19.12 ng/ml

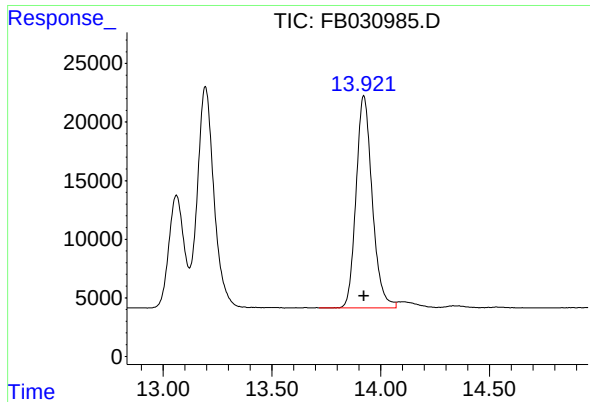

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.000 min
Response: 933577
Conc: 19.19 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1010S1

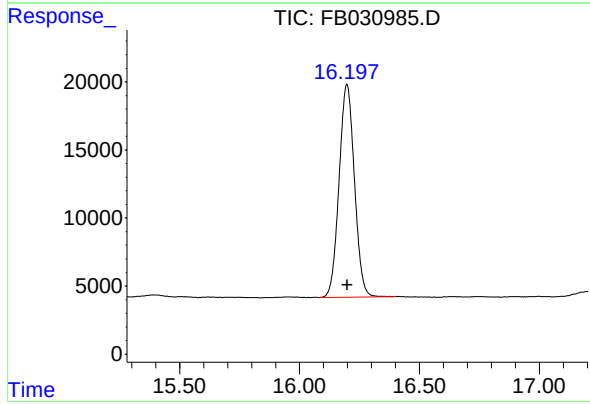

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.000 min
Response: 695324
Conc: 21.22 ng/ml