

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB101124\  
 Data File : FB031001.D  
 Signal(s) : FID2B.CH  
 Acq On : 11 Oct 2024 9:44  
 Operator : YP/AJ  
 Sample : VBF1011S2 50X  
 Misc : 5.00G/5.00 ML DI WATER  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
 FID\_B  
**ClientSampleId :**  
 VBF1011S2

Integration File: Calibration.e  
 Quant Time: Oct 14 01:40:11 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB100424.M  
 Quant Title :  
 QLast Update : Fri Oct 04 11:53:51 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
5) s AAA-TFT	8.795	623940	20.814 ng/ml
Target Compounds			
-----			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB101124\  
 Data File : FB031001.D  
 Signal(s) : FID2B.CH  
 Acq On : 11 Oct 2024 9:44  
 Operator : YP/AJ  
 Sample : VBF1011S2 50X  
 Misc : 5.00G/5.00 ML DI WATER  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :  
 VBF1011S2

Integration File: Calibration.e  
 Quant Time: Oct 14 01:40:11 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB100424.M  
 Quant Title :  
 QLast Update : Fri Oct 04 11:53:51 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

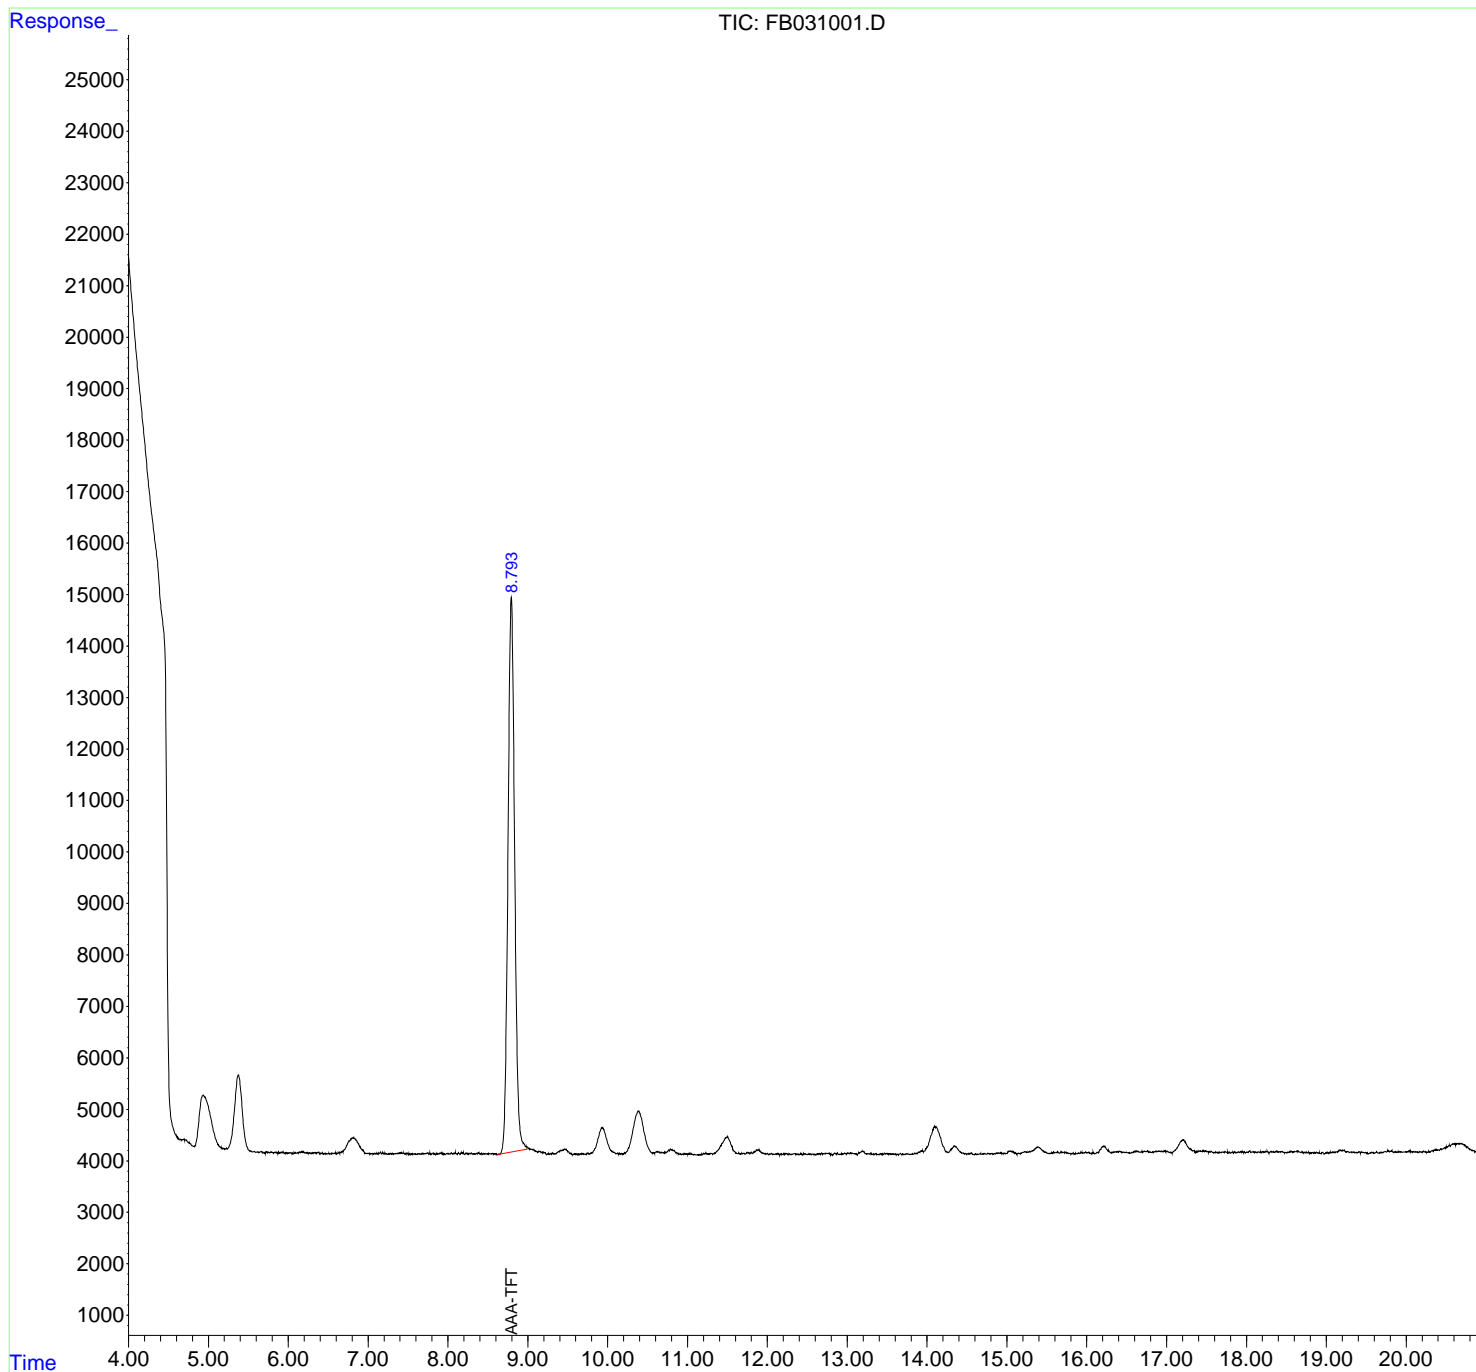

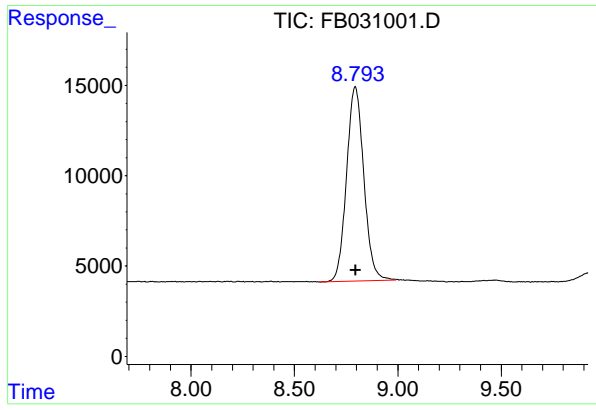

#5 AAA-TFT

R.T.: 8.795 min  
Delta R.T.: 0.000 min  
Response: 623940  
Conc: 20.81 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
VBF1011S2