

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101124\
 Data File : FB031002.D
 Signal(s) : FID2B.CH
 Acq On : 11 Oct 2024 10:11
 Operator : YP/AJ
 Sample : BSF1011S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1011S1

Integration File: Calibration.e
 Quant Time: Oct 14 01:40:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
 Quant Title :
 QLast Update : Fri Oct 04 11:53:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	647420	21.597 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.724	1044468	28.945 ng/ml
2) t 2,2,4-Trimethylpentane	7.430	1352137	28.374 ng/ml
3) t n-Heptane	7.755	416495	9.234 ng/ml
4) t Benzene	7.895	523679	9.528 ng/ml
6) t Toluene	10.624	1537089	28.454 ng/ml
7) t Ethylbenzene	13.060	456235	9.625 ng/ml
8) t m-Xylene	13.194	984343	18.869 ng/ml
9) t O-Xylene	13.922	924972	19.015 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	698188	21.307 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101124\
Data File : FB031002.D
Signal(s) : FID2B.CH
Acq On : 11 Oct 2024 10:11
Operator : YP/AJ
Sample : BSF1011S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1011S1

Integration File: Calibration.e
Quant Time: Oct 14 01:40:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
Quant Title :
QLast Update : Fri Oct 04 11:53:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

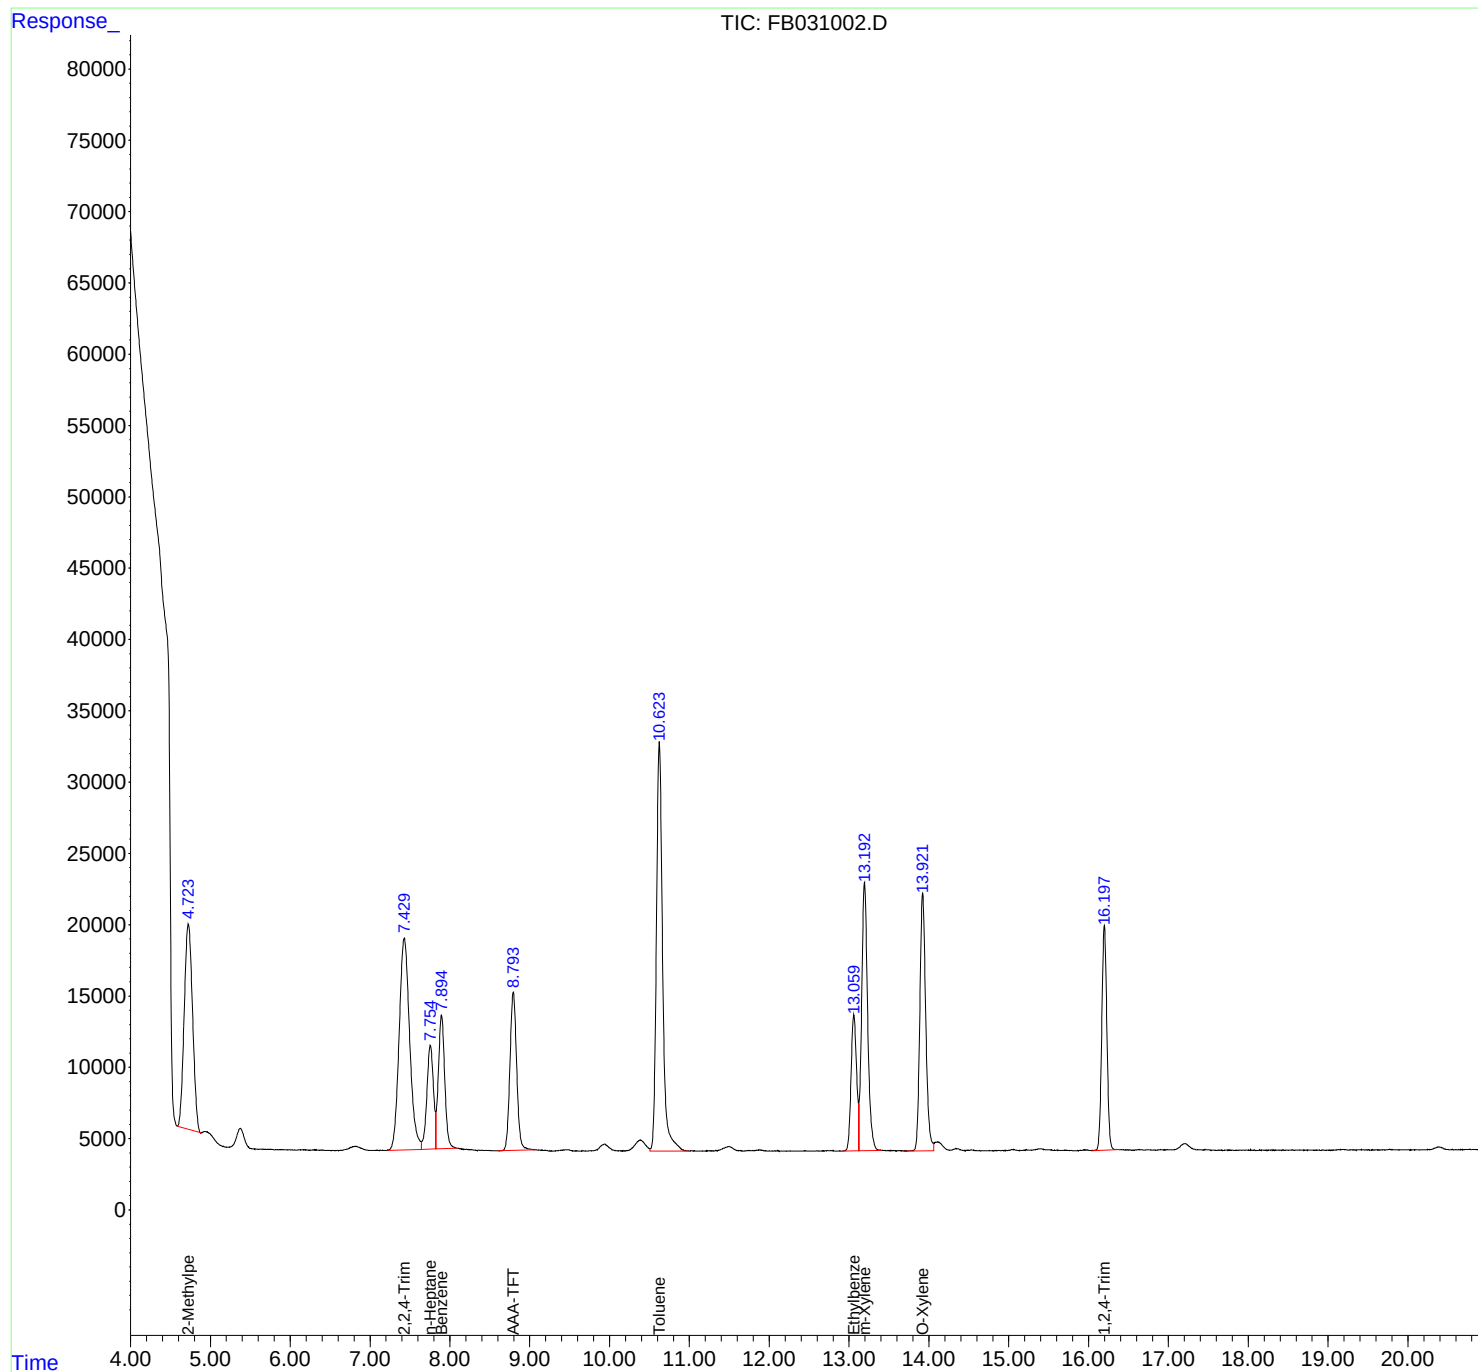


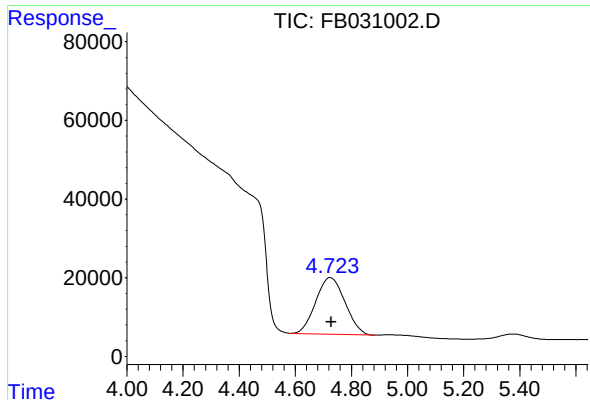

#1 2-Methylpentane


R.T.: 4.724 min
Delta R.T.: -0.004 min
Response: 1044468
Conc: 28.94 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1011S1

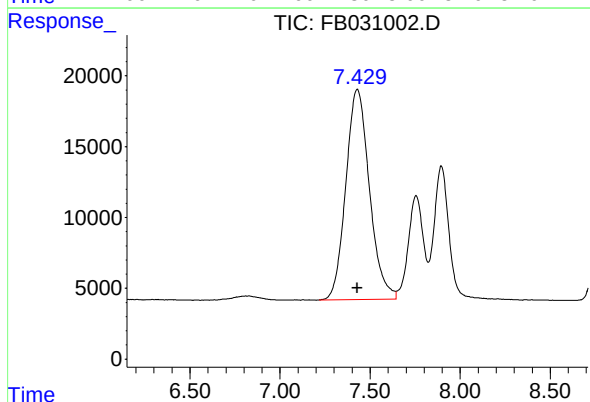


#2 2,2,4-Trimethylpentane

R.T.: 7.430 min
Delta R.T.: 0.002 min
Response: 1352137
Conc: 28.37 ng/ml

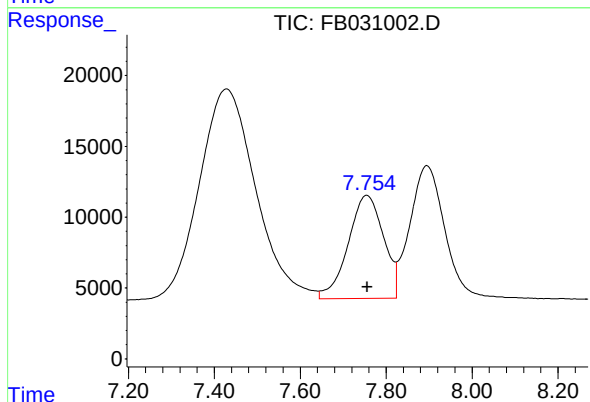


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.001 min
Response: 416495
Conc: 9.23 ng/ml

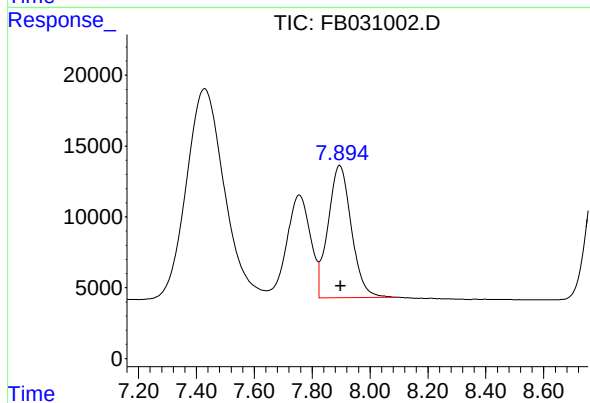

#4 Benzene


R.T.: 7.895 min
Delta R.T.: -0.002 min
Response: 523679
Conc: 9.53 ng/ml

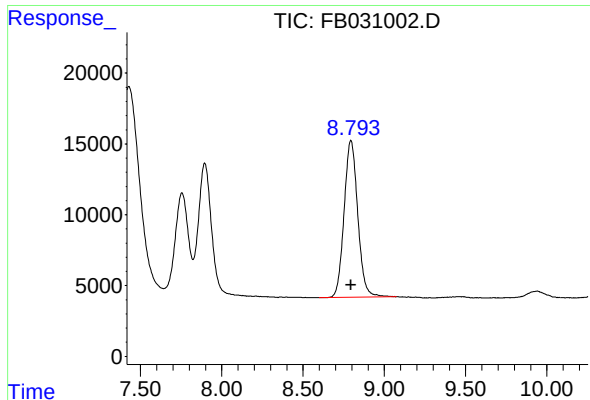

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.000 min
Response: 647420
Conc: 21.60 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1011S1

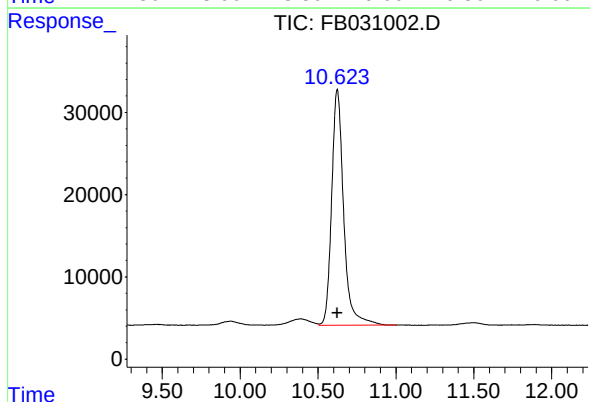


#6 Toluene

R.T.: 10.624 min
Delta R.T.: 0.000 min
Response: 1537089
Conc: 28.45 ng/ml

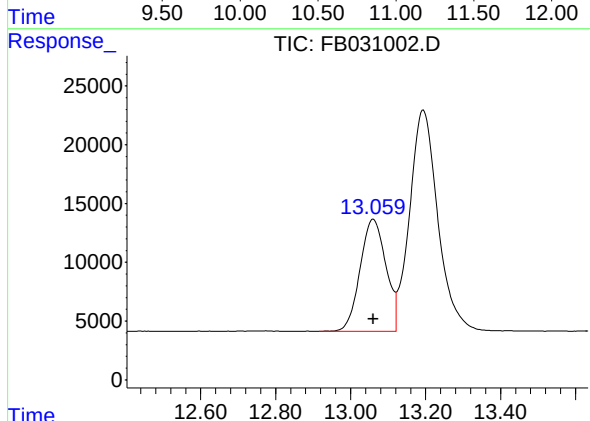


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.000 min
Response: 456235
Conc: 9.63 ng/ml

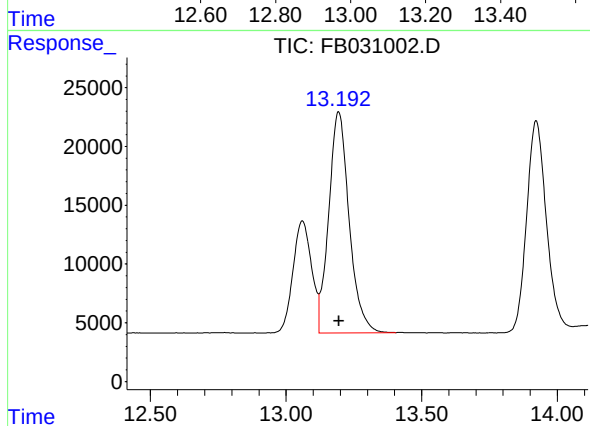

#8 m-Xylene


R.T.: 13.194 min
Delta R.T.: 0.000 min
Response: 984343
Conc: 18.87 ng/ml

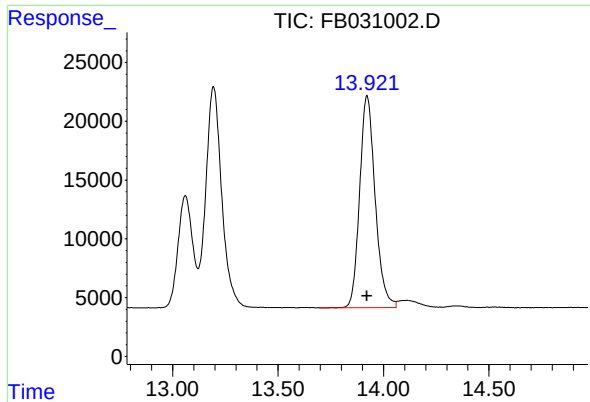

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.000 min
Response: 924972
Conc: 19.01 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1011S1

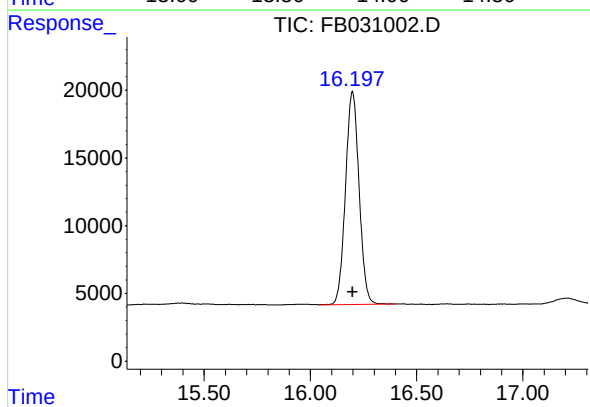

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.000 min
Response: 698188
Conc: 21.31 ng/ml