

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101218\
 Data File : FB018225.D
 Signal(s) : FID2B.CH
 Acq On : 12 Oct 2018 16:59
 Operator : MJ/SJ
 Sample : J5450-02MSD
 Misc : 5.01g/5.00mL DI Water
 ALS Vial : 14 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 15 07:49:49 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.110	181068	21.023 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.963	441323	28.855 ng/ml
2) t 2,2,4-Trimethylpentane	7.728	461316	31.219 ng/ml
3) t n-Heptane	8.066	136620	9.641 ng/ml
4) t Benzene	8.207	195269	10.482 ng/ml
6) t Toluene	10.961	472977	31.034 ng/ml
7) t Ethylbenzene	13.411	156993	9.895 ng/ml
8) t m-Xylene	13.543	332729	19.997 ng/ml
9) t O-Xylene	14.275	357978	20.078 ng/ml
10) t 1,2,4-Trimethylbenzene	16.559	401905	19.756 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101218\
Data File : FB018225.D
Signal(s) : FID2B.CH
Acq On : 12 Oct 2018 16:59
Operator : MJ/SJ
Sample : J5450-02MSD
Misc : 5.01g/5.00mL DI Water
ALS Vial : 14 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 15 07:49:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

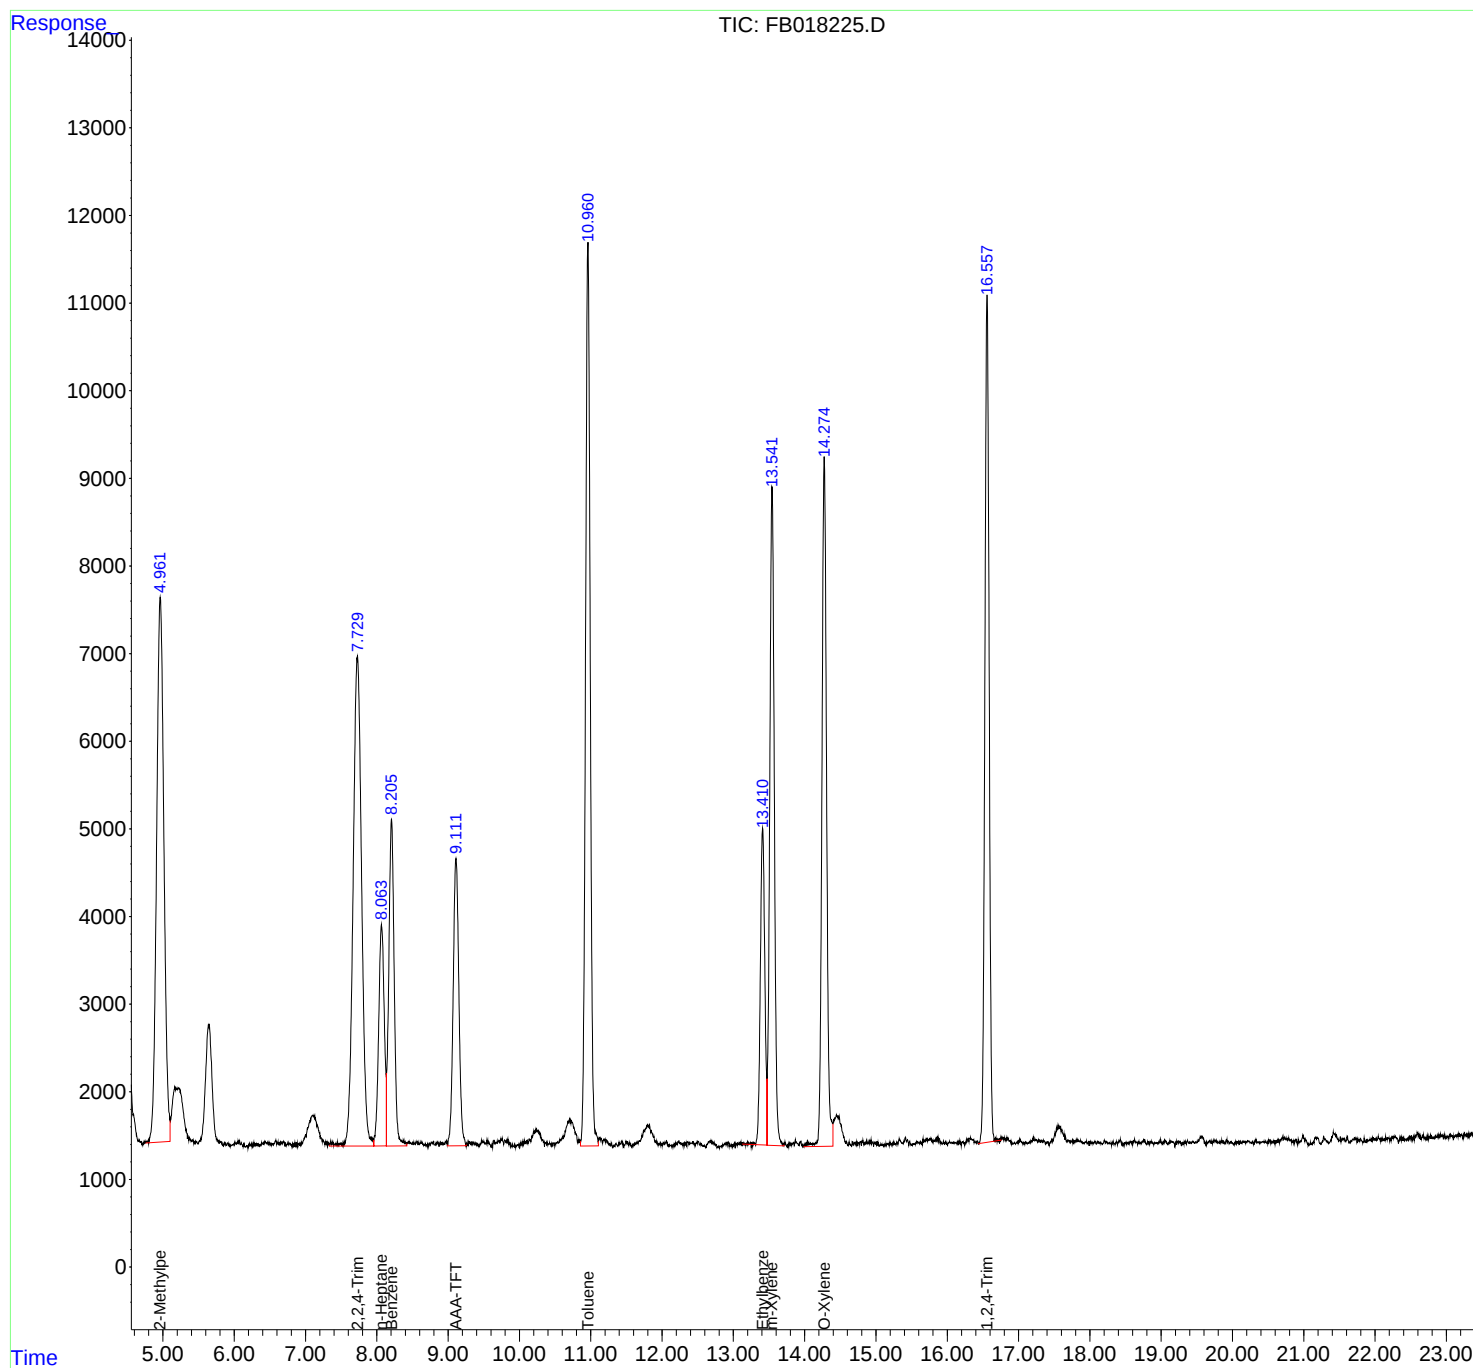

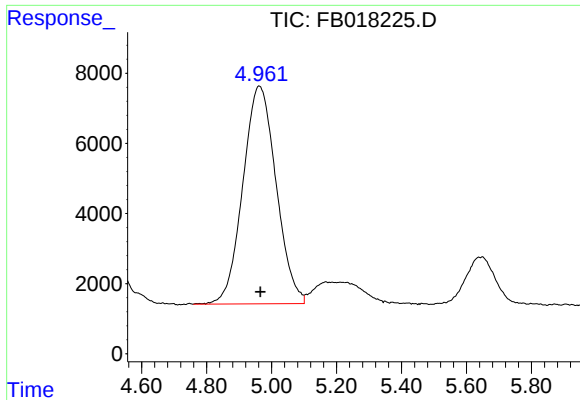


#1 2-Methylpentane

R.T.: 4.963 min
Delta R.T.: -0.002 min
Response: 441323
Conc: 28.86 ng/ml

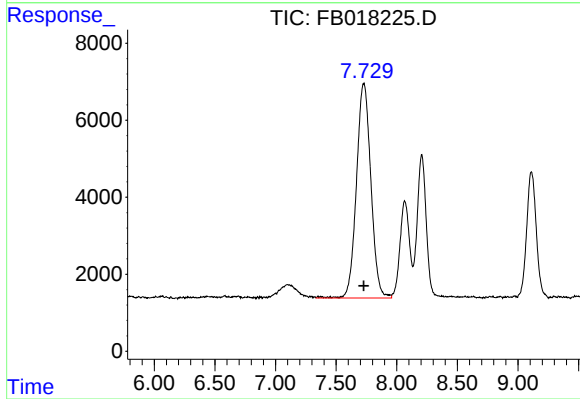


#2 2,2,4-Trimethylpentane

R.T.: 7.728 min
Delta R.T.: 0.000 min
Response: 461316
Conc: 31.22 ng/ml

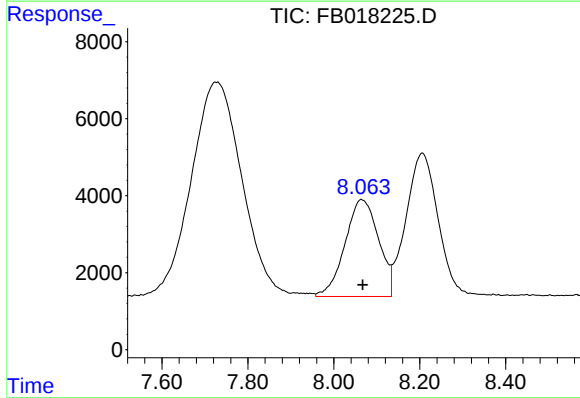


#3 n-Heptane

R.T.: 8.066 min
Delta R.T.: -0.002 min
Response: 136620
Conc: 9.64 ng/ml

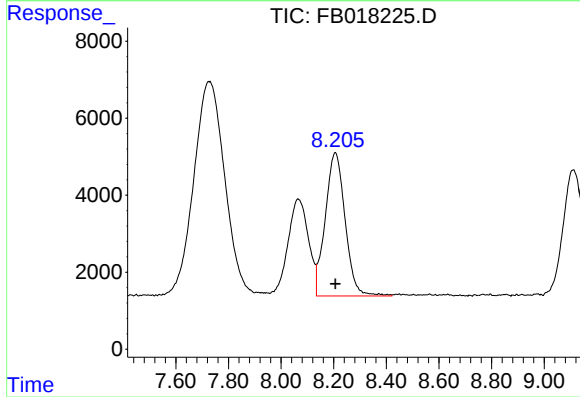


#4 Benzene

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 195269
Conc: 10.48 ng/ml

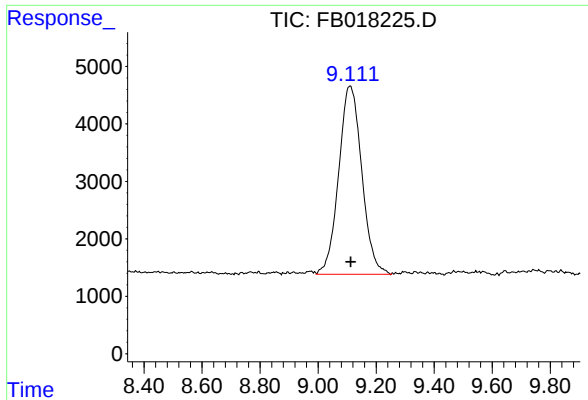


#5 AAA-TFT

R.T.: 9.110 min
Delta R.T.: -0.002 min
Response: 181068
Conc: 21.02 ng/ml

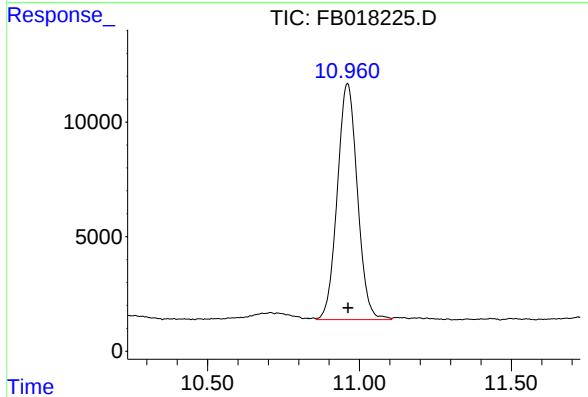


#6 Toluene

R.T.: 10.961 min
Delta R.T.: 0.000 min
Response: 472977
Conc: 31.03 ng/ml

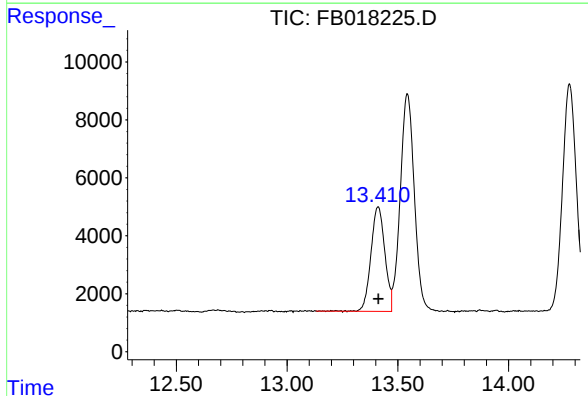


#7 Ethylbenzene

R.T.: 13.411 min
Delta R.T.: 0.000 min
Response: 156993
Conc: 9.90 ng/ml

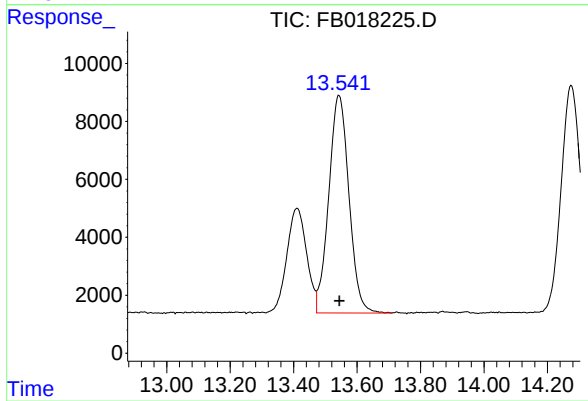


#8 m-Xylene

R.T.: 13.543 min
Delta R.T.: 0.000 min
Response: 332729
Conc: 20.00 ng/ml

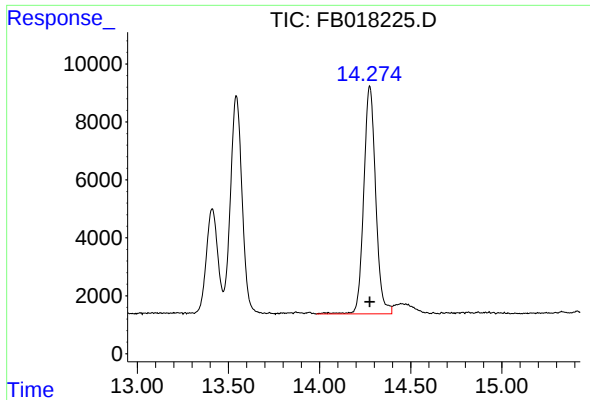

#9 O-Xylene

R.T.: 14.275 min
Delta R.T.: -0.001 min
Response: 357978
Conc: 20.08 ng/ml

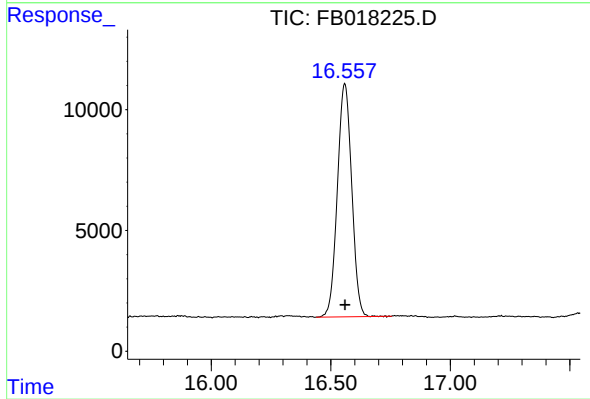

#10 1,2,4-Trimethylbenzene

R.T.: 16.559 min
Delta R.T.: 0.000 min
Response: 401905
Conc: 19.76 ng/ml