

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101320\
 Data File : FB025049.D
 Signal(s) : FID2B.CH
 Acq On : 13 Oct 2020 13:22
 Operator : DD/AJ
 Sample : BSF1013S1
 Misc : 5.02/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 14 00:38:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.801	439106	20.916 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.690	932290	31.000 ng/ml
2) t	2,2,4-Trimethylpentane	7.418	1000919	32.749 ng/ml
3) t	n-Heptane	7.760	326813	10.743 ng/ml
4) t	Benzene	7.894	392461	10.535 ng/ml
6) t	Toluene	10.633	1111940	31.852 ng/ml
7) t	Ethylbenzene	13.073	335402	10.347 ng/ml
8) t	m-Xylene	13.206	670649	21.112 ng/ml
9) t	O-Xylene	13.933	647220	21.299 ng/ml
10) t	1,2,4-Trimethylbenzene	16.210	542914	21.406 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101320\
Data File : FB025049.D
Signal(s) : FID2B.CH
Acq On : 13 Oct 2020 13:22
Operator : DD/AJ
Sample : BSF1013S1
Misc : 5.02/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 14 00:38:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

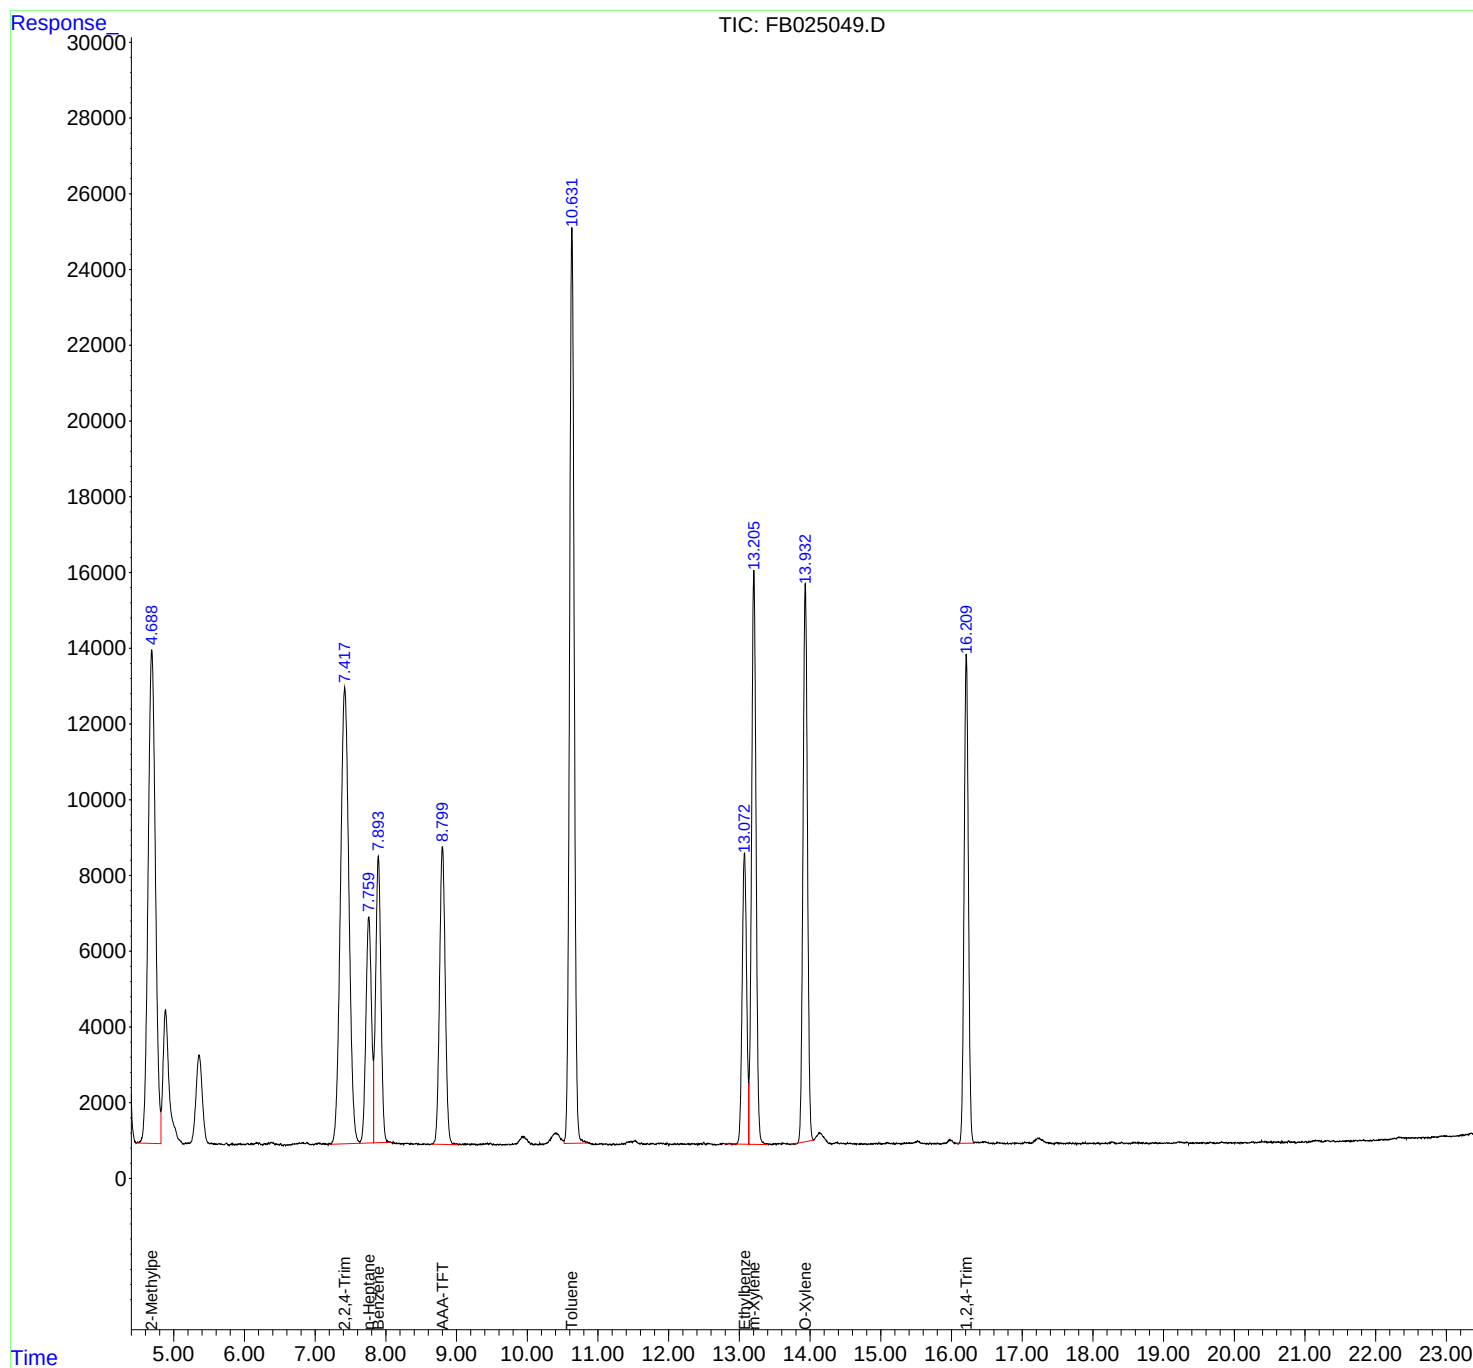

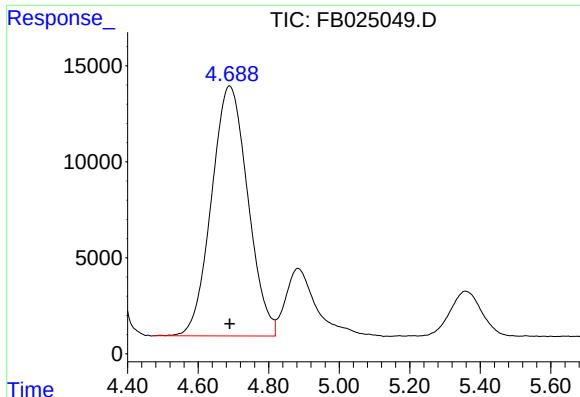


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: 0.000 min
Response: 932290
Conc: 31.00 ng/ml

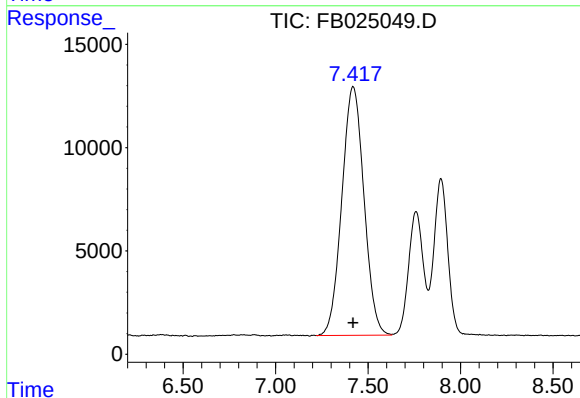


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 1000919
Conc: 32.75 ng/ml

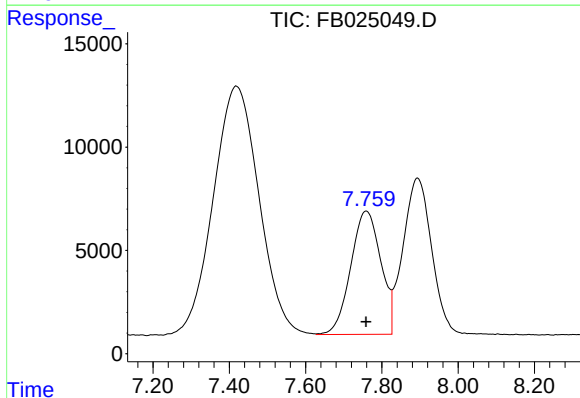


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 326813
Conc: 10.74 ng/ml

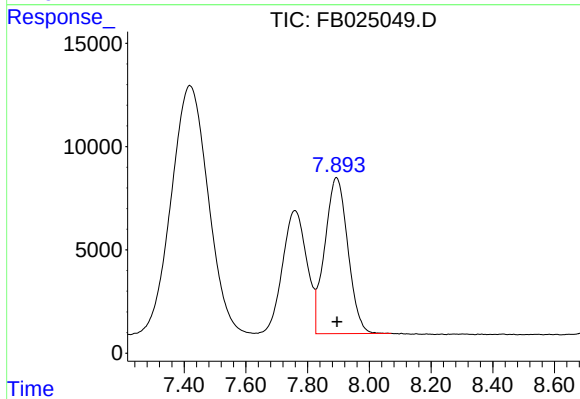


#4 Benzene

R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 392461
Conc: 10.54 ng/ml

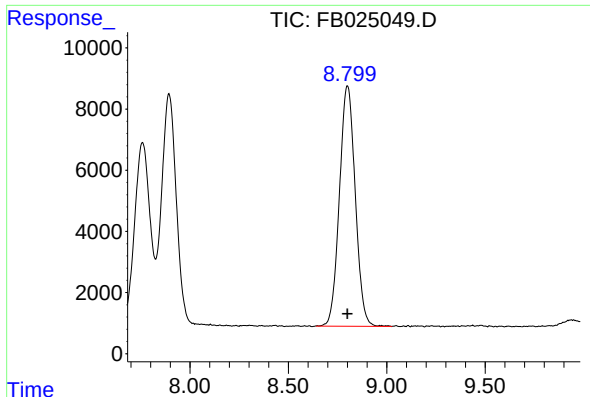


#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.000 min
Response: 439106
Conc: 20.92 ng/ml

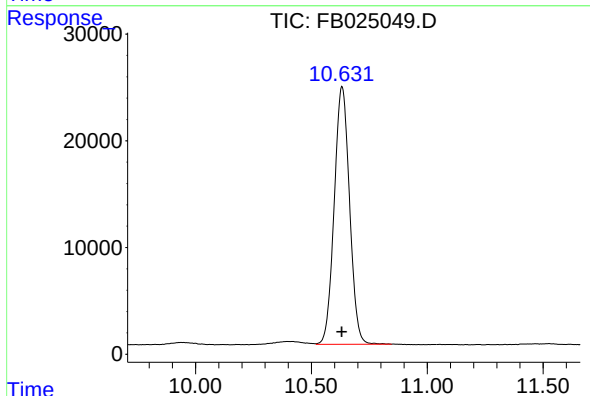


#6 Toluene

R.T.: 10.633 min
Delta R.T.: 0.000 min
Response: 1111940
Conc: 31.85 ng/ml

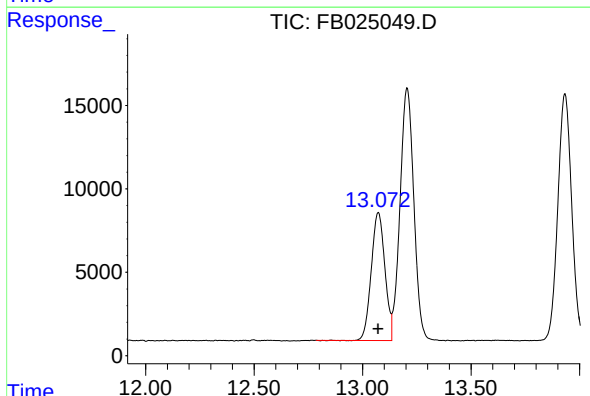


#7 Ethylbenzene

R.T.: 13.073 min
Delta R.T.: 0.001 min
Response: 335402
Conc: 10.35 ng/ml

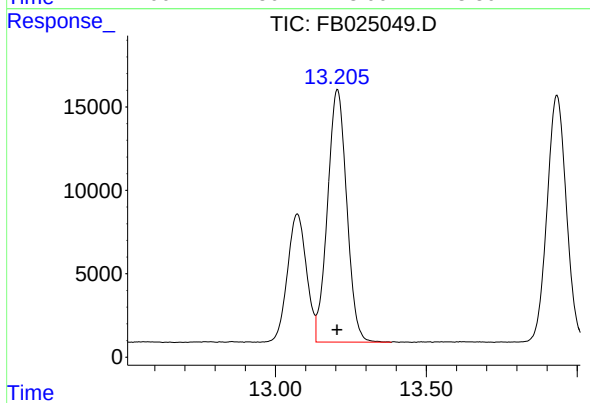


#8 m-Xylene

R.T.: 13.206 min
Delta R.T.: 0.002 min
Response: 670649
Conc: 21.11 ng/ml

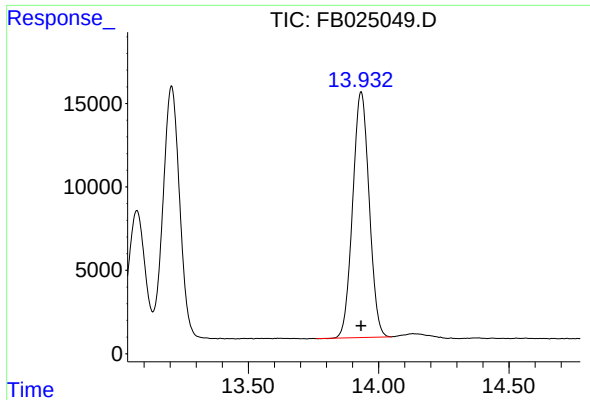

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.001 min
Response: 647220
Conc: 21.30 ng/ml

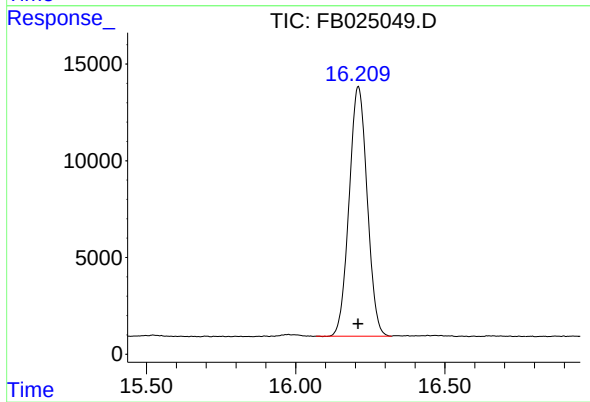

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 542914
Conc: 21.41 ng/ml