

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101320\
 Data File : FB025051.D
 Signal(s) : FID2B.CH
 Acq On : 13 Oct 2020 14:23
 Operator : DD/AJ
 Sample : L4217-02MS
 Misc : 5.08/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 14 00:38:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	436875	20.809 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	834349	27.744 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	810392	26.515 ng/ml
3) t n-Heptane	7.759	262129	8.617 ng/ml
4) t Benzene	7.895	395190	10.609 ng/ml
6) t Toluene	10.632	1076853	30.847 ng/ml
7) t Ethylbenzene	13.072	328176	10.124 ng/ml
8) t m-Xylene	13.205	640679	20.169 ng/ml
9) t O-Xylene	13.933	633009	20.831 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	500403	19.730 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101320\
Data File : FB025051.D
Signal(s) : FID2B.CH
Acq On : 13 Oct 2020 14:23
Operator : DD/AJ
Sample : L4217-02MS
Misc : 5.08/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 14 00:38:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

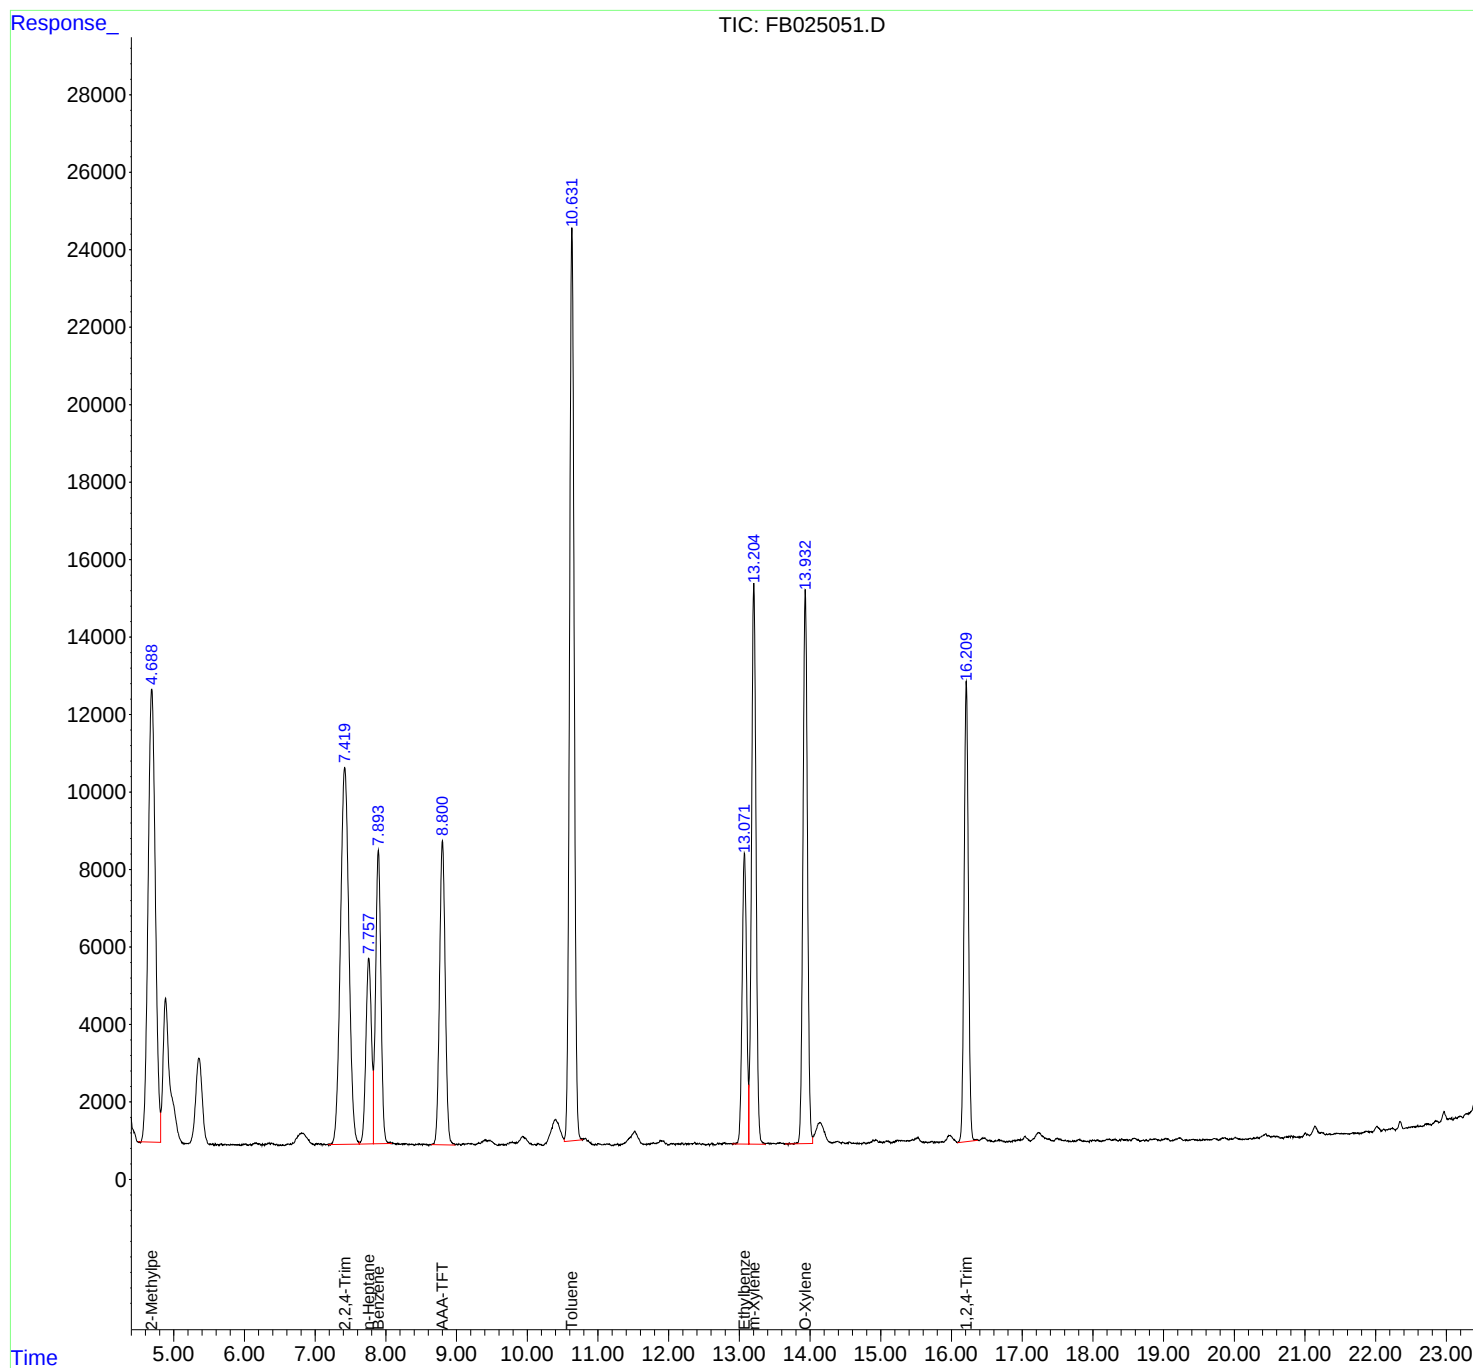

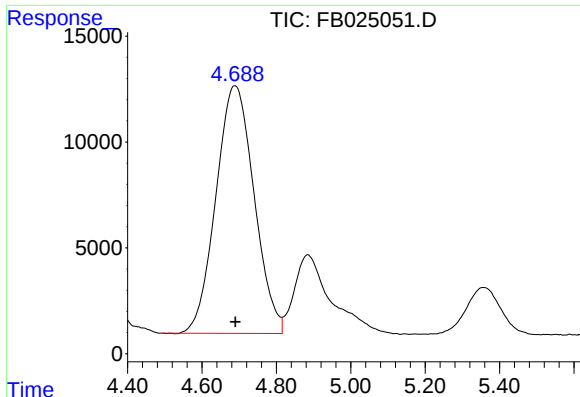


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: -0.001 min
Response: 834349
Conc: 27.74 ng/ml

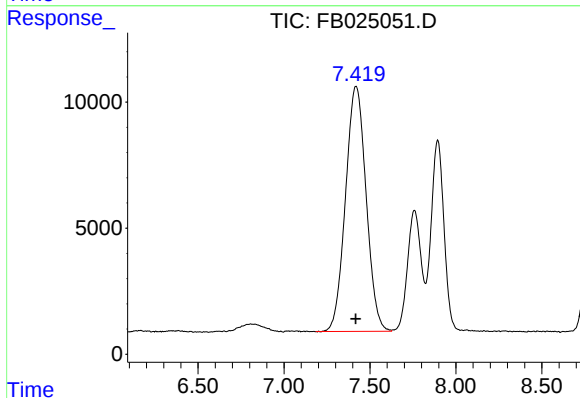


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 810392
Conc: 26.51 ng/ml

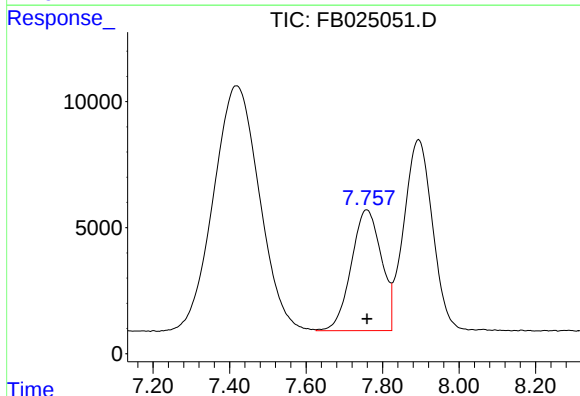


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 262129
Conc: 8.62 ng/ml

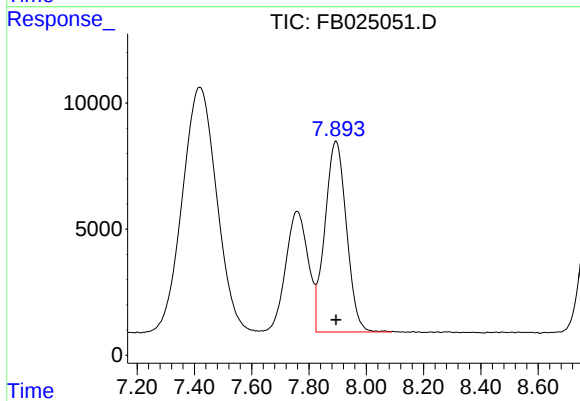


#4 Benzene

R.T.: 7.895 min
Delta R.T.: 0.000 min
Response: 395190
Conc: 10.61 ng/ml

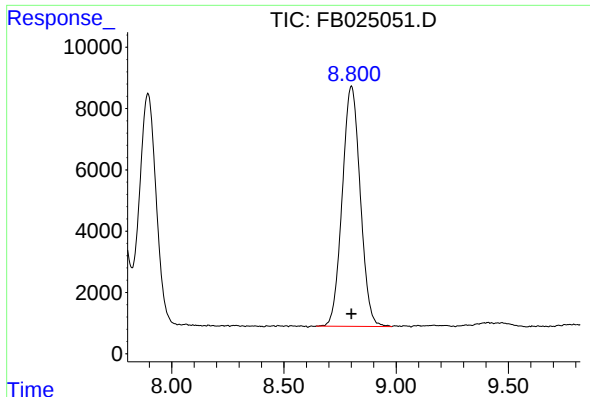


#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.000 min
Response: 436875
Conc: 20.81 ng/ml

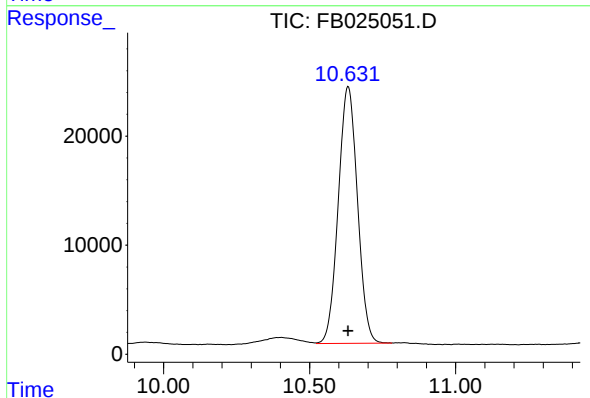


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 1076853
Conc: 30.85 ng/ml

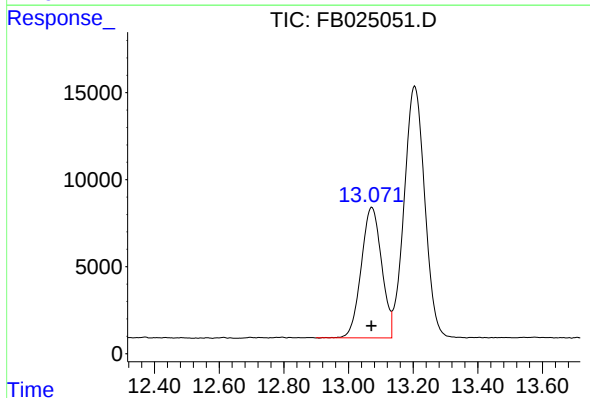


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 328176
Conc: 10.12 ng/ml

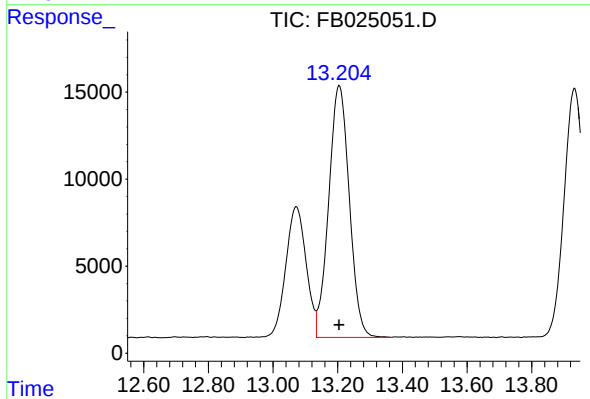


#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.000 min
Response: 640679
Conc: 20.17 ng/ml

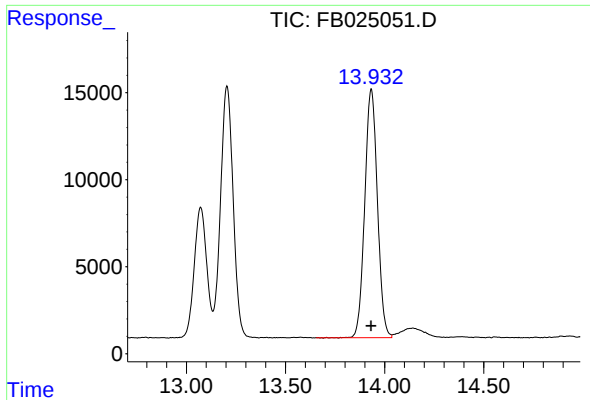

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.000 min
Response: 633009
Conc: 20.83 ng/ml

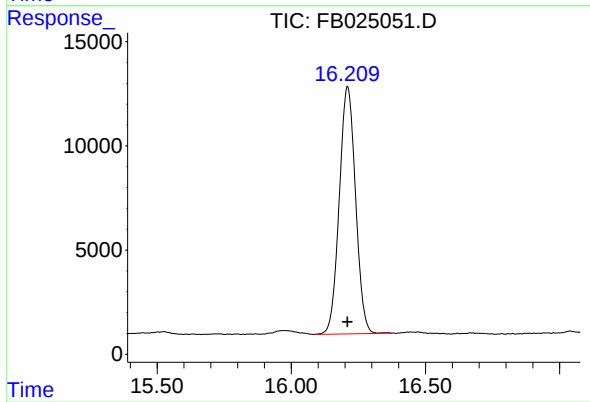

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 500403
Conc: 19.73 ng/ml