

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101419\
 Data File : FB022711.D
 Signal(s) : FID2B.CH
 Acq On : 14 Oct 2019 20:07
 Operator : DD/AJ
 Sample : BSF1014S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 15 01:30:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100919.M
 Quant Title :
 QLast Update : Wed Oct 09 11:21:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	506889	19.706 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	1050842	30.925 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	1140894	31.539 ng/ml
3) t n-Heptane	7.758	378710	10.509 ng/ml
4) t Benzene	7.893	446088	10.379 ng/ml
6) t Toluene	10.630	1297836	30.740 ng/ml
7) t Ethylbenzene	13.070	414741	10.472 ng/ml
8) t m-Xylene	13.203	784075	21.093 ng/ml
9) t O-Xylene	13.931	740494	21.107 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	587891	21.410 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101419\
Data File : FB022711.D
Signal(s) : FID2B.CH
Acq On : 14 Oct 2019 20:07
Operator : DD/AJ
Sample : BSF1014S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 15 01:30:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100919.M
Quant Title :
QLast Update : Wed Oct 09 11:21:39 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

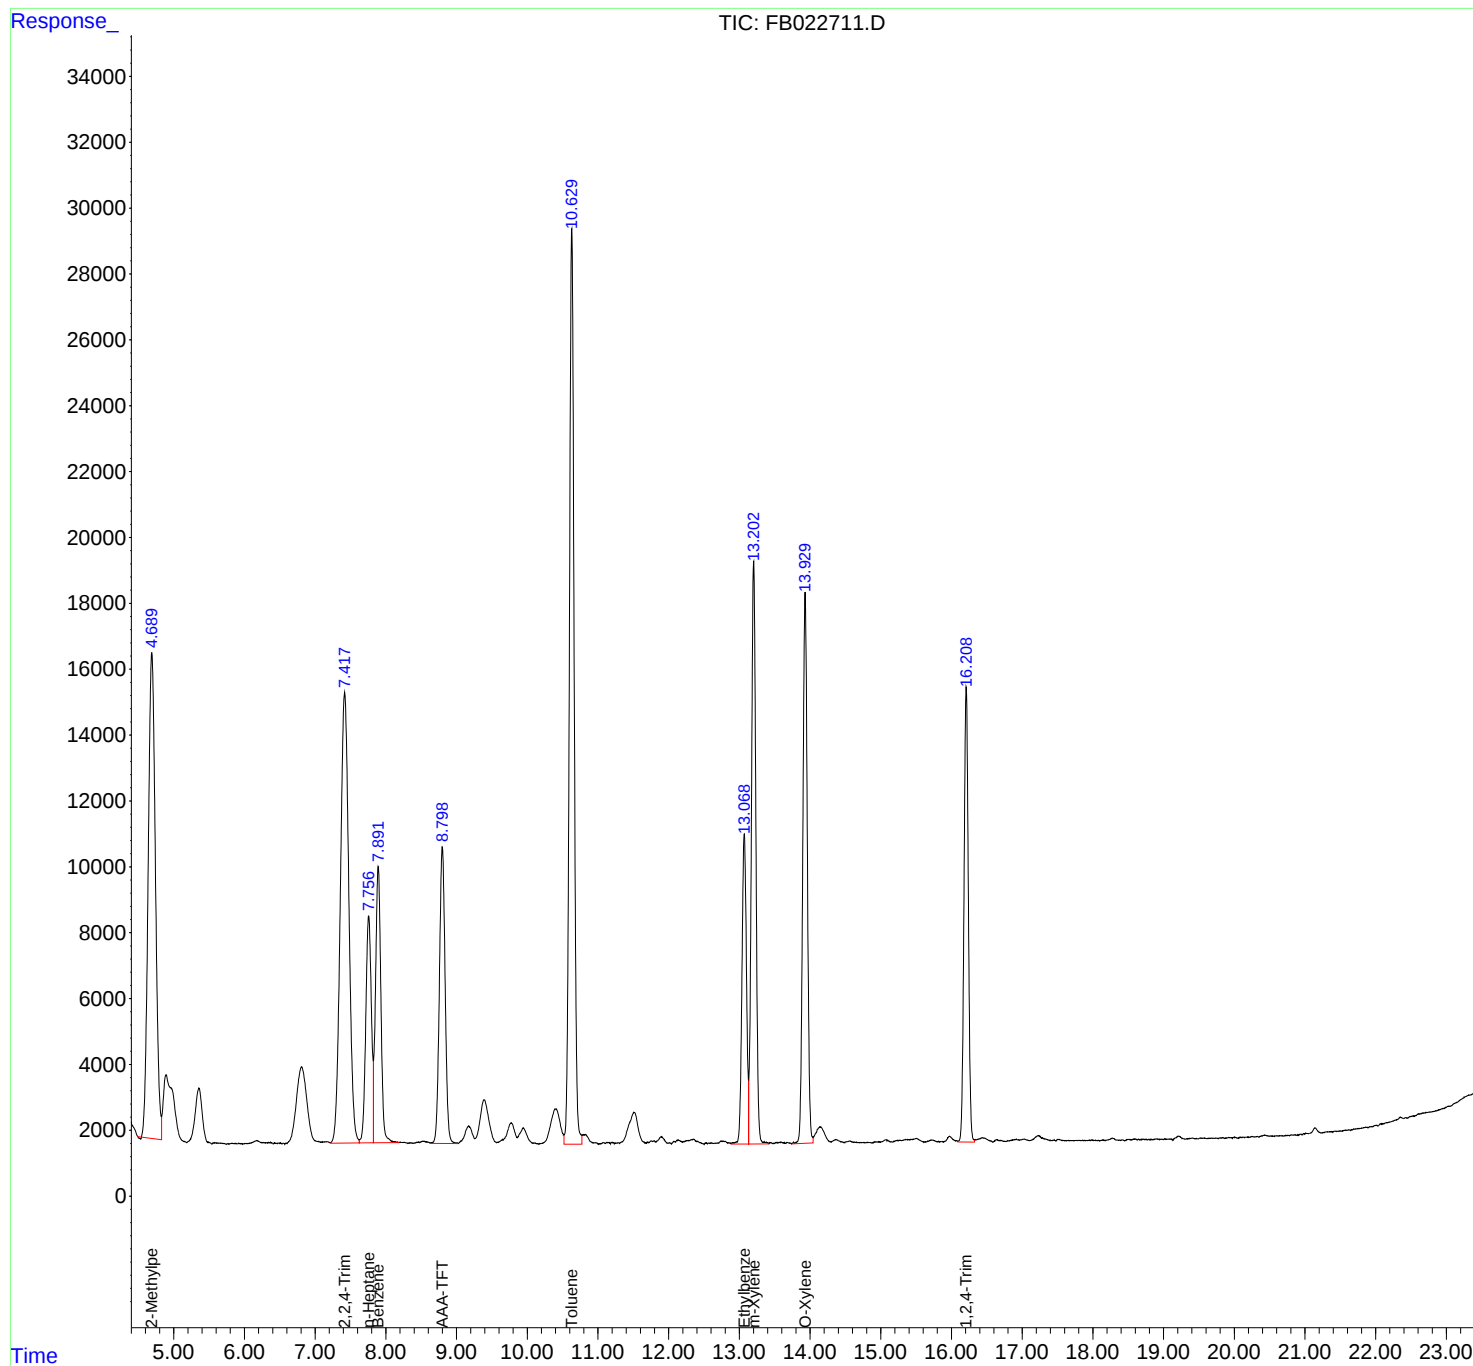

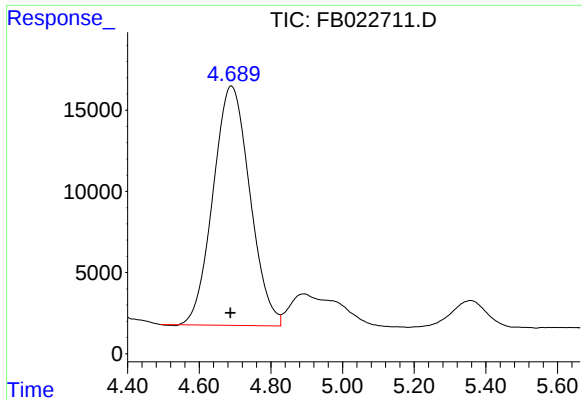


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: 0.003 min
Response: 1050842
Conc: 30.93 ng/ml

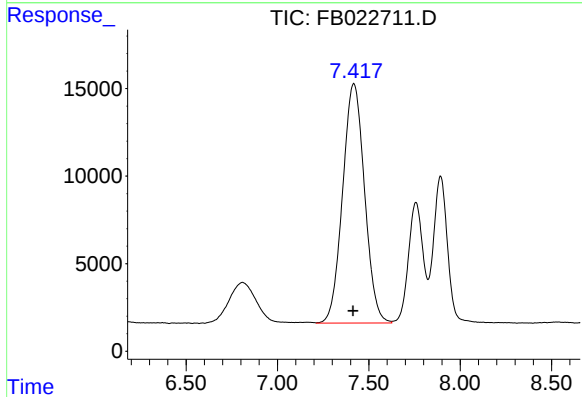


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.004 min
Response: 1140894
Conc: 31.54 ng/ml

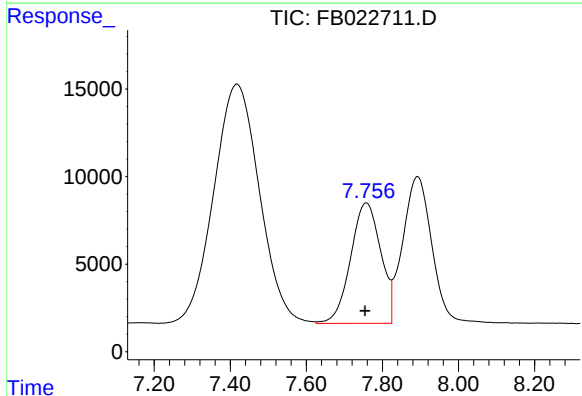


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.004 min
Response: 378710
Conc: 10.51 ng/ml

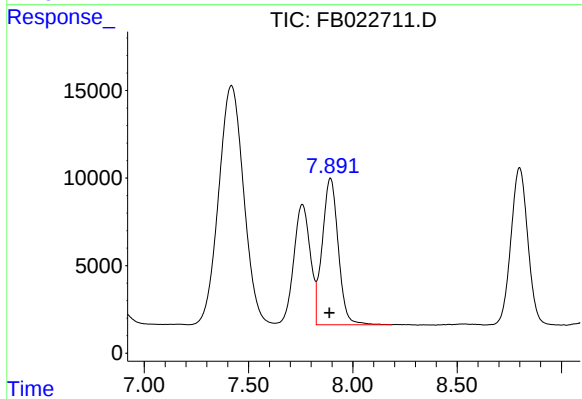


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.004 min
Response: 446088
Conc: 10.38 ng/ml

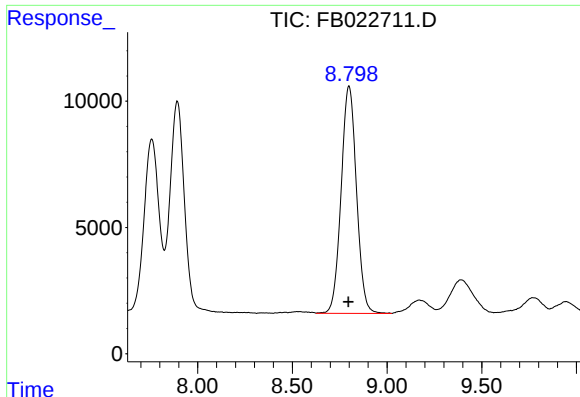


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.003 min
Response: 506889
Conc: 19.71 ng/ml

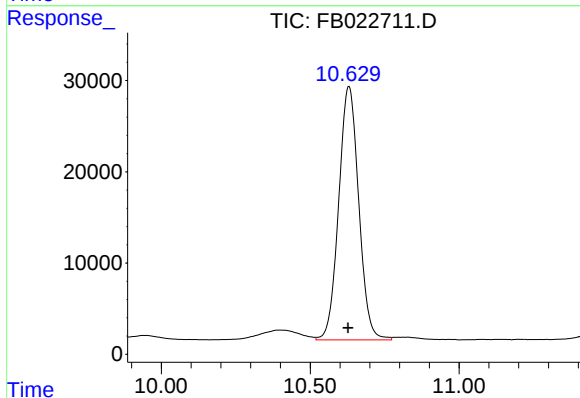


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.003 min
Response: 1297836
Conc: 30.74 ng/ml

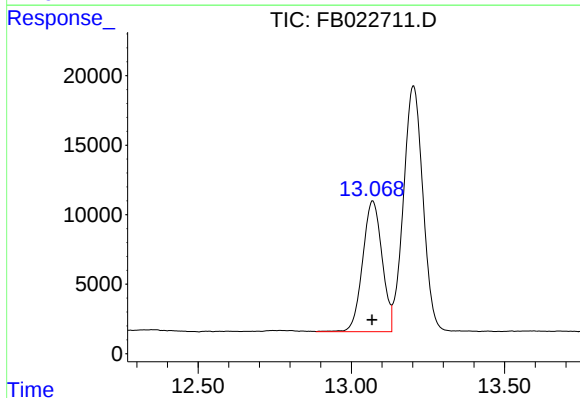


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.003 min
Response: 414741
Conc: 10.47 ng/ml

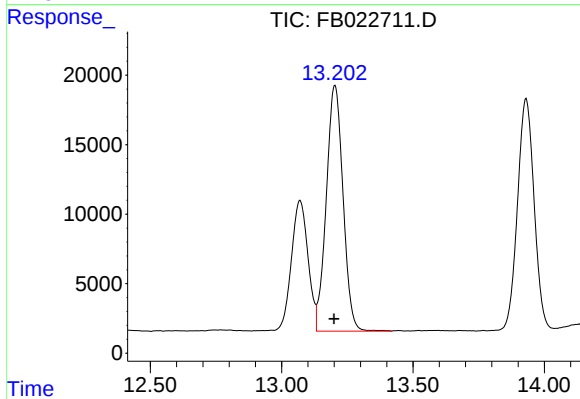


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.003 min
Response: 784075
Conc: 21.09 ng/ml

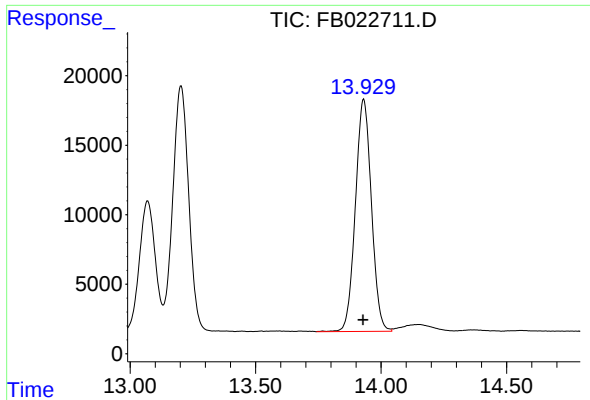

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.003 min
Response: 740494
Conc: 21.11 ng/ml

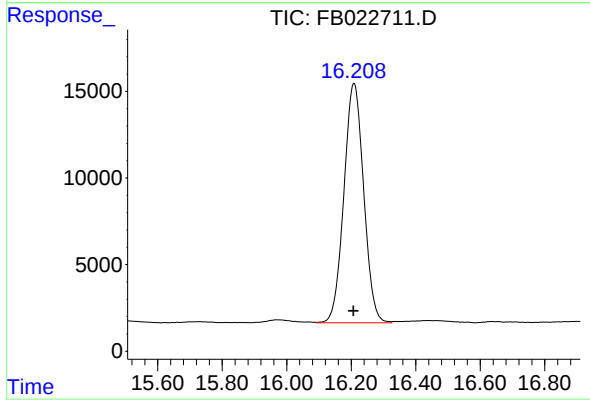

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.003 min
Response: 587891
Conc: 21.41 ng/ml