

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101420\
 Data File : FB025060.D
 Signal(s) : FID2B.CH
 Acq On : 14 Oct 2020 12:46
 Operator : DD/AJ
 Sample : L4226-14MSD
 Misc : 5.03/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 14 15:22:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	419797	19.996 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	762542	25.356 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	738692	24.169 ng/ml
3) t n-Heptane	7.760	235905	7.755 ng/ml
4) t Benzene	7.894	359472	9.650 ng/ml
6) t Toluene	10.632	961689	27.548 ng/ml
7) t Ethylbenzene	13.072	281289	8.678 ng/ml
8) t m-Xylene	13.205	565767	17.810 ng/ml
9) t O-Xylene	13.932	549264	18.075 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	429689	16.942 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101420\
Data File : FB025060.D
Signal(s) : FID2B.CH
Acq On : 14 Oct 2020 12:46
Operator : DD/AJ
Sample : L4226-14MSD
Misc : 5.03/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 14 15:22:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

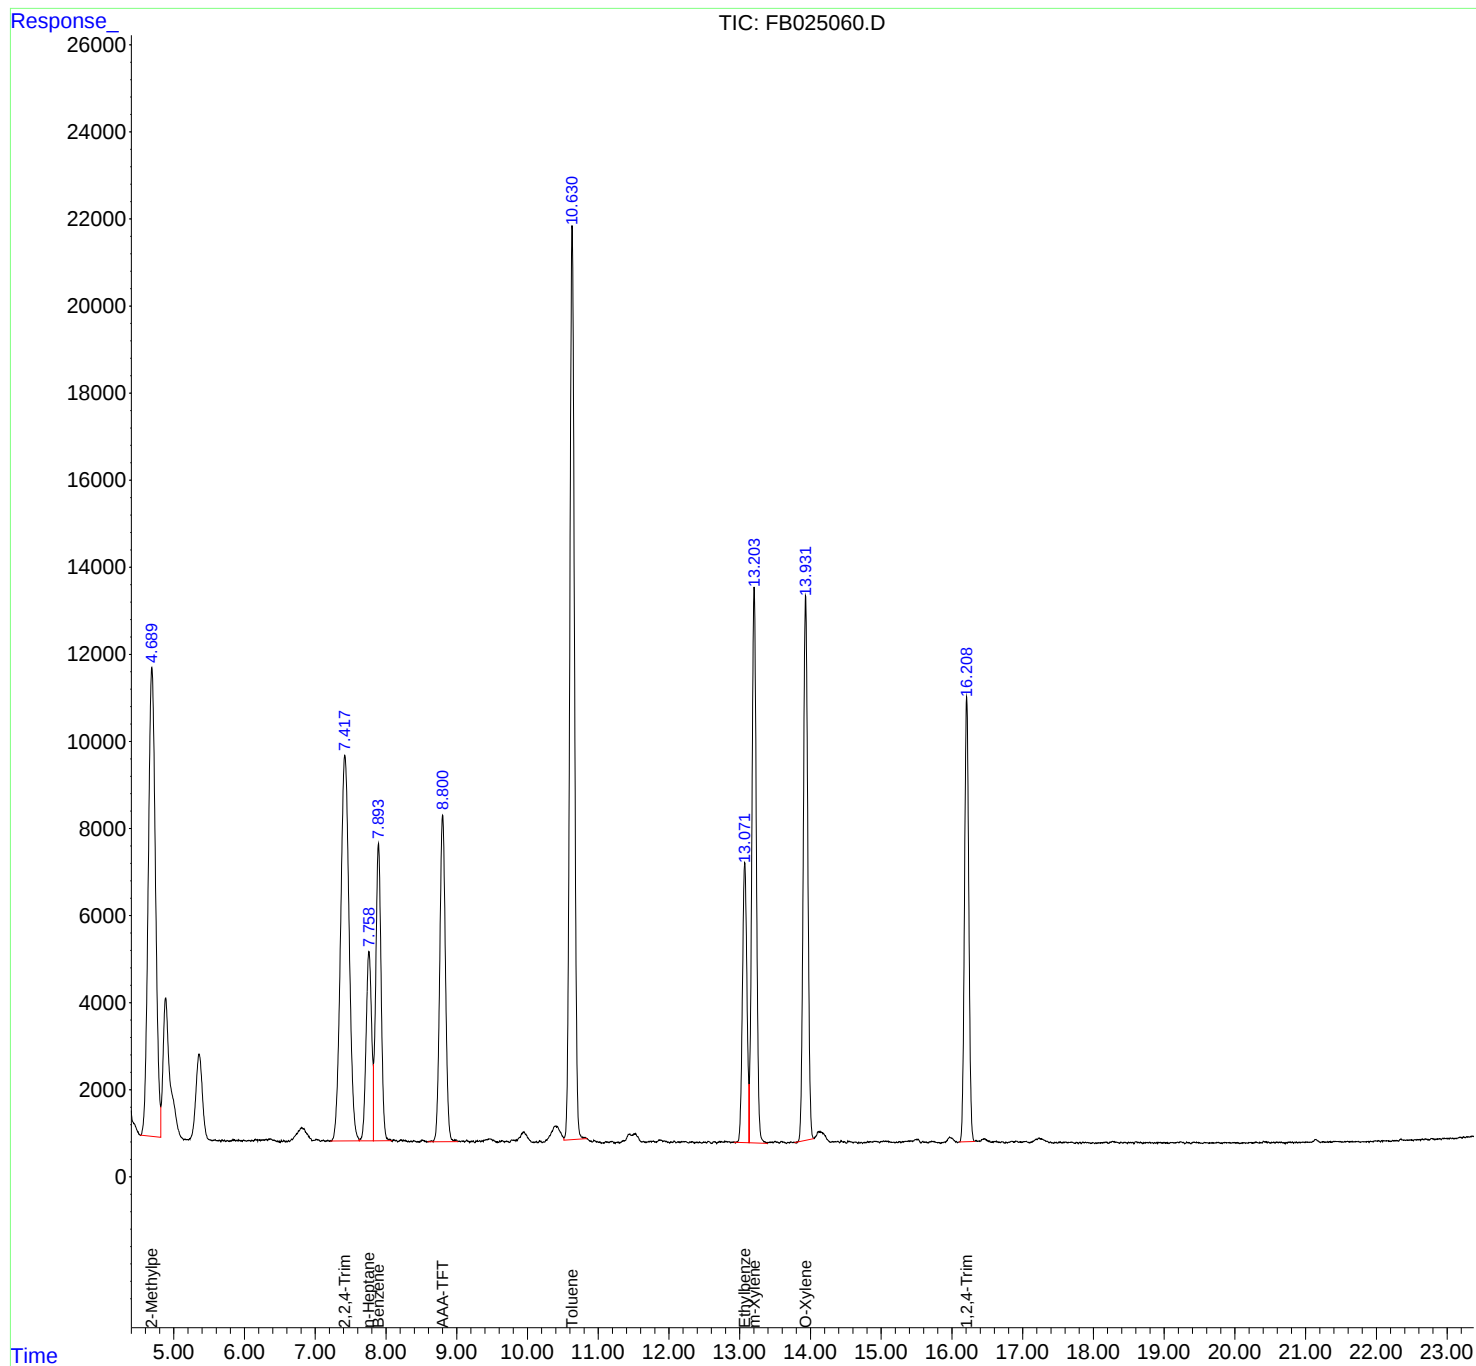

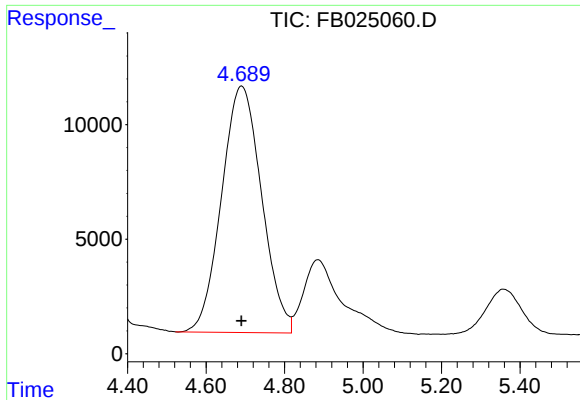


#1 2-Methylpentane

R.T.: 4.691 min
Delta R.T.: 0.000 min
Response: 762542
Conc: 25.36 ng/ml

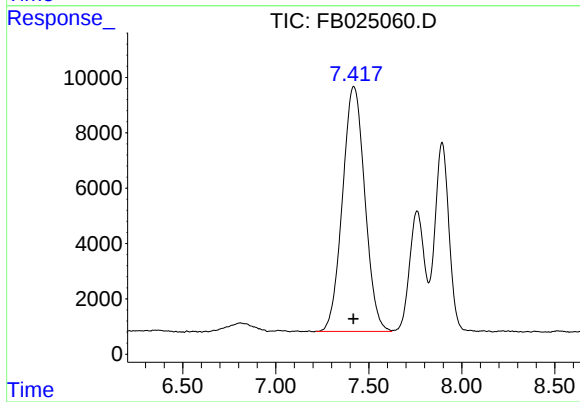


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 738692
Conc: 24.17 ng/ml

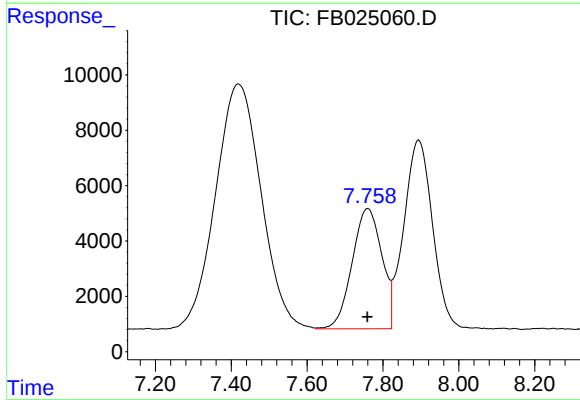


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.001 min
Response: 235905
Conc: 7.75 ng/ml

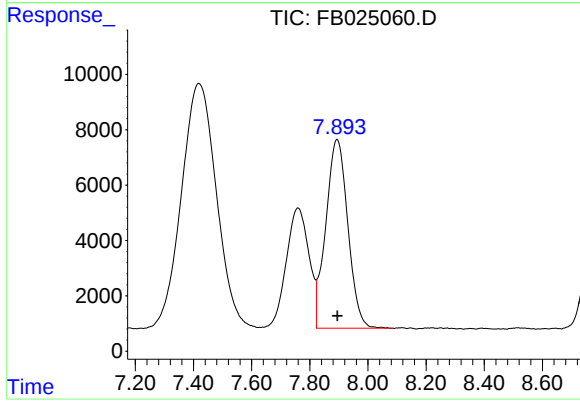


#4 Benzene

R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 359472
Conc: 9.65 ng/ml

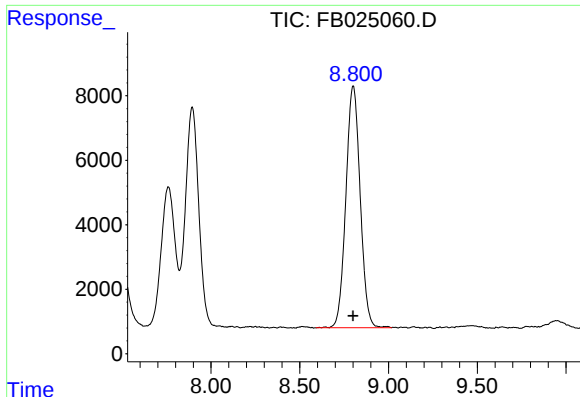


#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.000 min
Response: 419797
Conc: 20.00 ng/ml

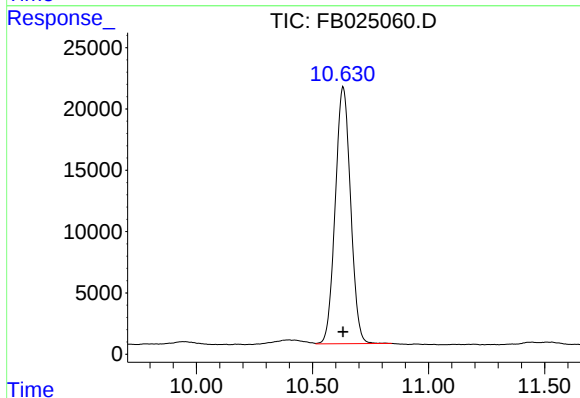


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 961689
Conc: 27.55 ng/ml

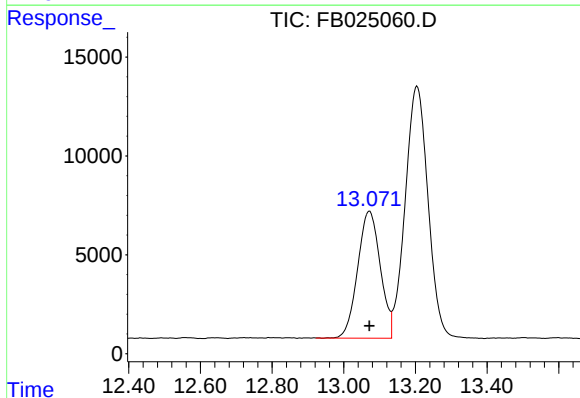


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 281289
Conc: 8.68 ng/ml

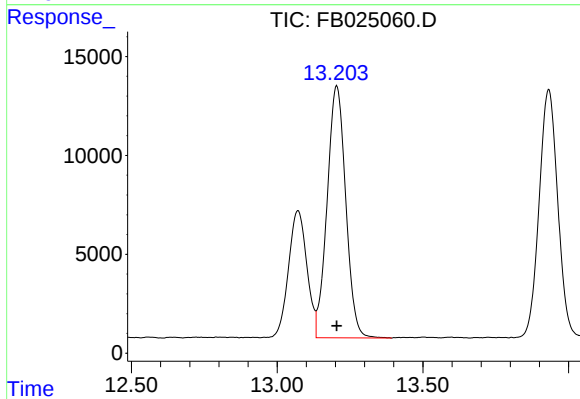

#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.000 min
Response: 565767
Conc: 17.81 ng/ml

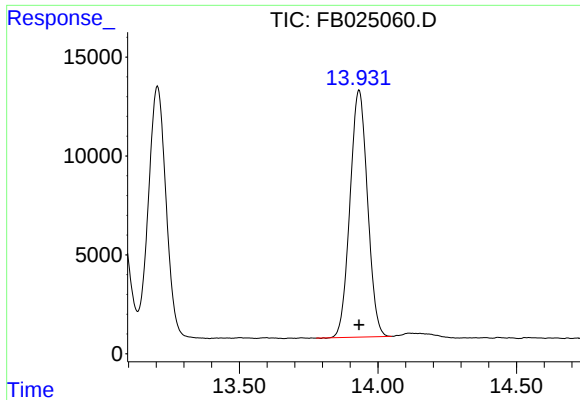


#9 O-Xylene

R.T.: 13.932 min

Delta R.T.: 0.000 min

Response: 549264

Conc: 18.08 ng/ml

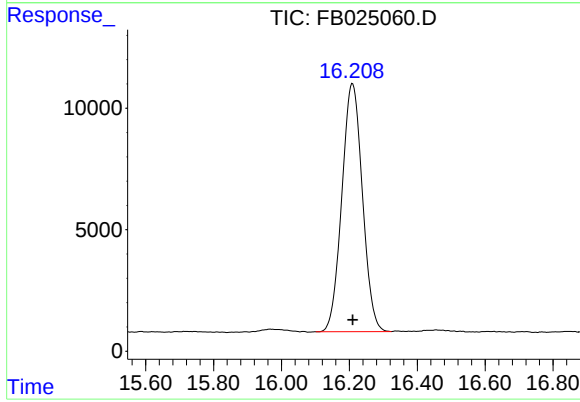

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min

Delta R.T.: 0.000 min

Response: 429689

Conc: 16.94 ng/ml