

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101420\
 Data File : FB025056.D
 Signal(s) : FID2B.CH
 Acq On : 14 Oct 2020 10:43
 Operator : DD/AJ
 Sample : BSF1014S1
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 14 15:22:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	458615	21.845 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.692	898826	29.888 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	988837	32.353 ng/ml
3) t n-Heptane	7.760	323558	10.636 ng/ml
4) t Benzene	7.895	388127	10.419 ng/ml
6) t Toluene	10.633	1105876	31.678 ng/ml
7) t Ethylbenzene	13.073	331778	10.235 ng/ml
8) t m-Xylene	13.205	660790	20.802 ng/ml
9) t O-Xylene	13.933	633538	20.849 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	526581	20.762 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101420\
Data File : FB025056.D
Signal(s) : FID2B.CH
Acq On : 14 Oct 2020 10:43
Operator : DD/AJ
Sample : BSF1014S1
Misc : 5.01/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 14 15:22:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

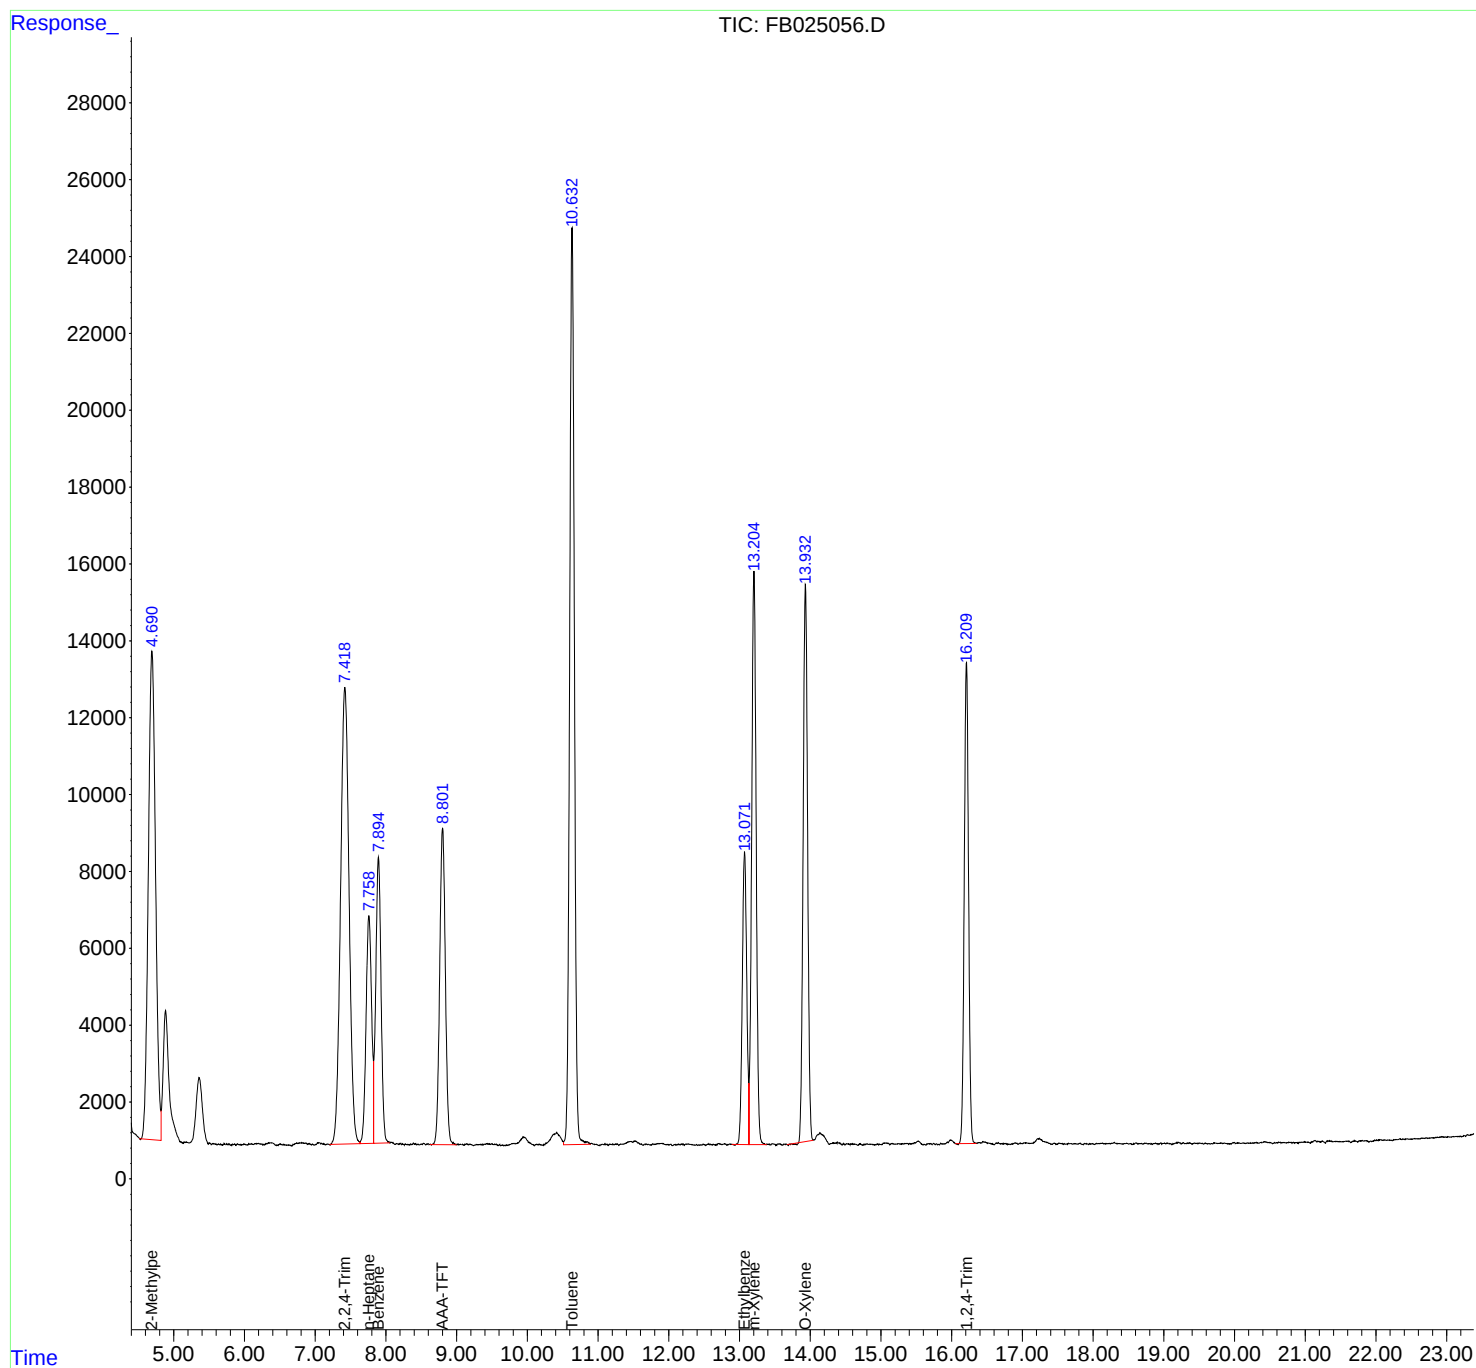

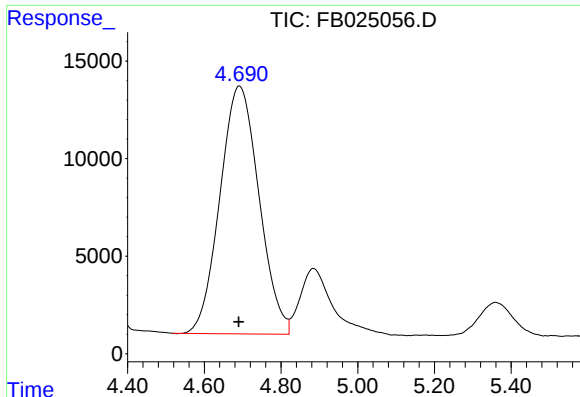


#1 2-Methylpentane

R.T.: 4.692 min
Delta R.T.: 0.002 min
Response: 898826
Conc: 29.89 ng/ml

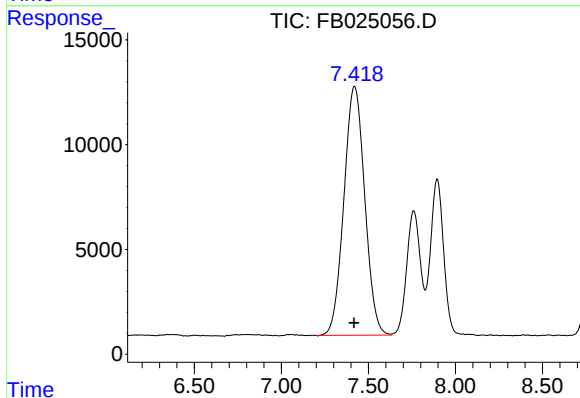


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.002 min
Response: 988837
Conc: 32.35 ng/ml

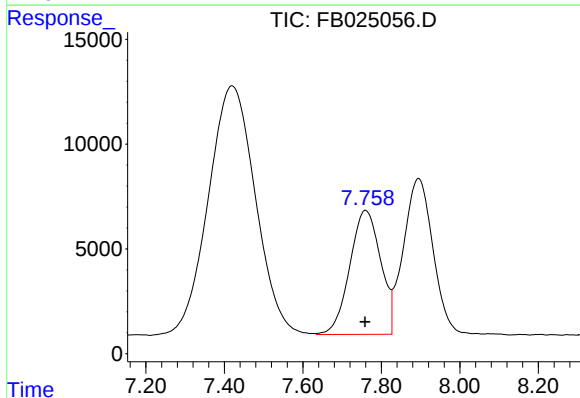


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 323558
Conc: 10.64 ng/ml

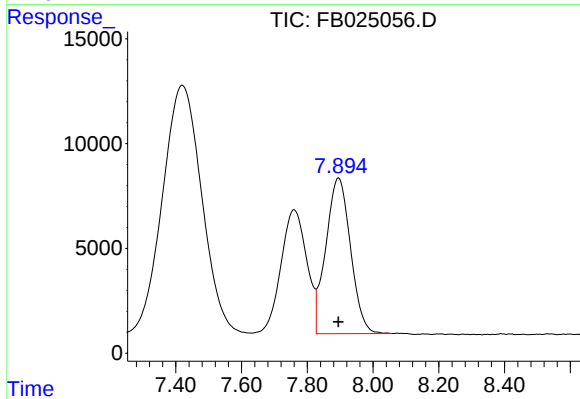


#4 Benzene

R.T.: 7.895 min
Delta R.T.: 0.000 min
Response: 388127
Conc: 10.42 ng/ml

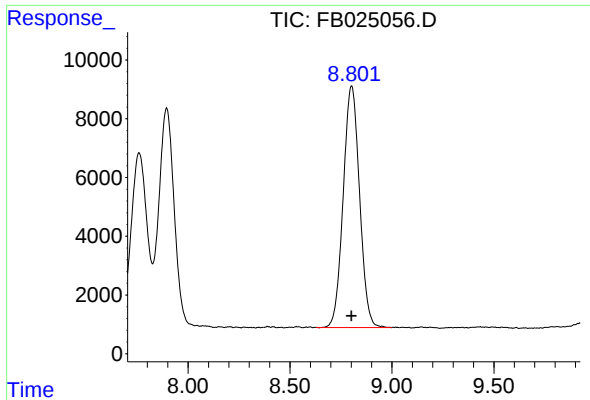


#5 AAA-TFT

R.T.: 8.802 min
Delta R.T.: 0.002 min
Response: 458615
Conc: 21.84 ng/ml

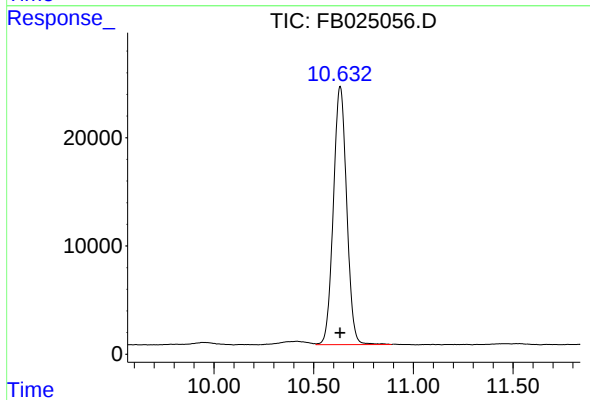


#6 Toluene

R.T.: 10.633 min
Delta R.T.: 0.002 min
Response: 1105876
Conc: 31.68 ng/ml

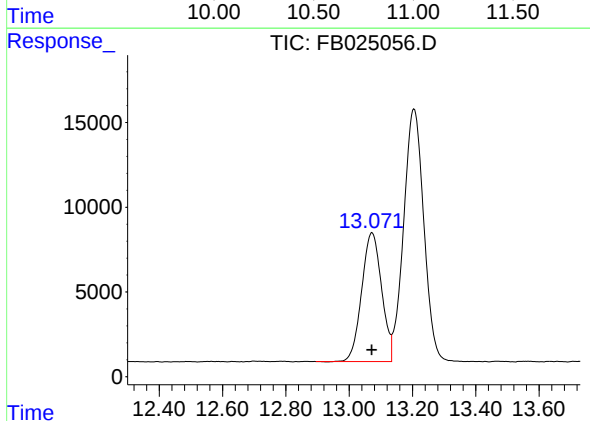


#7 Ethylbenzene

R.T.: 13.073 min
Delta R.T.: 0.001 min
Response: 331778
Conc: 10.24 ng/ml

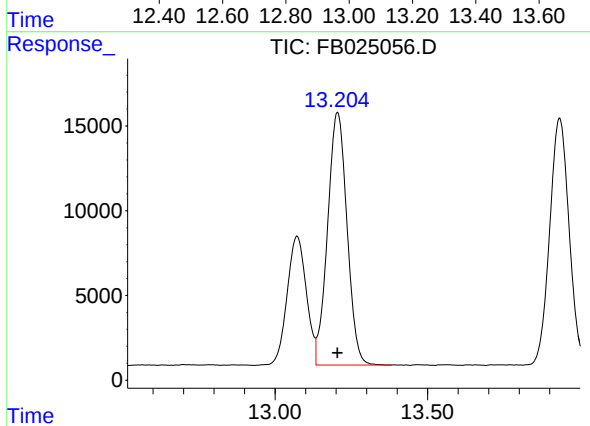


#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.001 min
Response: 660790
Conc: 20.80 ng/ml

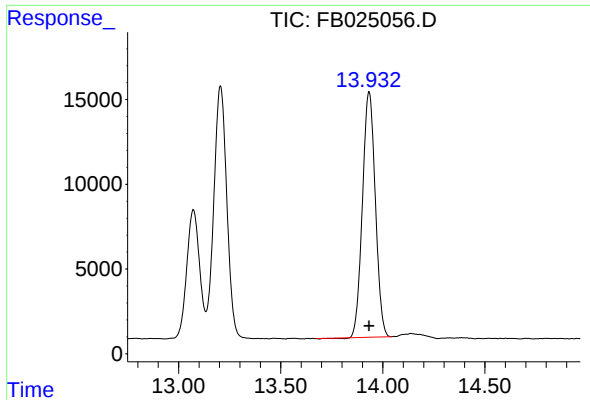

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.000 min
Response: 633538
Conc: 20.85 ng/ml

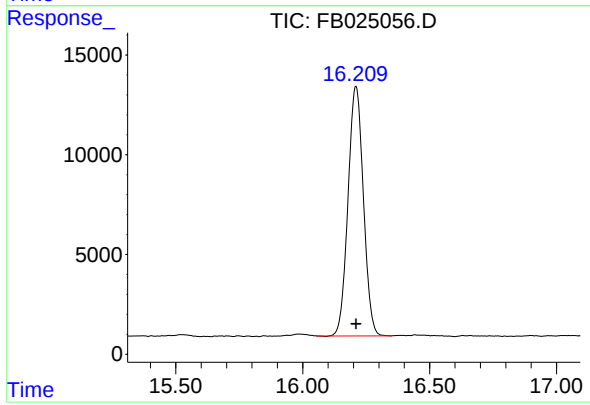

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 526581
Conc: 20.76 ng/ml