

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101421\
 Data File : FB026283.D
 Signal(s) : FID2B.CH
 Acq On : 14 Oct 2021 11:49
 Operator : AJ/MA
 Sample : BSF1014S1
 Misc : 5.01G\5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1014S1

Integration File: Calibration.e
 Quant Time: Oct 14 14:53:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100821.M
 Quant Title :
 QLast Update : Fri Oct 08 14:30:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.847	254174	16.866 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.854	467177	26.838 ng/ml
2) t 2,2,4-Trimethylpentane	7.524	596719	28.888 ng/ml
3) t n-Heptane	7.822	189074	8.070 ng/ml
4) t Benzene	7.961	218436	8.348 ng/ml
6) t Toluene	10.660	644903	24.892 ng/ml
7) t Ethylbenzene	13.082	197779	8.659 ng/ml
8) t m-Xylene	13.214	397883	17.737 ng/ml
9) t O-Xylene	13.940	382297	18.071 ng/ml
10) t 1,2,4-Trimethylbenzene	16.212	424470	18.241 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101421\
Data File : FB026283.D
Signal(s) : FID2B.CH
Acq On : 14 Oct 2021 11:49
Operator : AJ/MA
Sample : BSF1014S1
Misc : 5.01G\5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1014S1

Integration File: Calibration.e
Quant Time: Oct 14 14:53:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100821.M
Quant Title :
QLast Update : Fri Oct 08 14:30:36 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

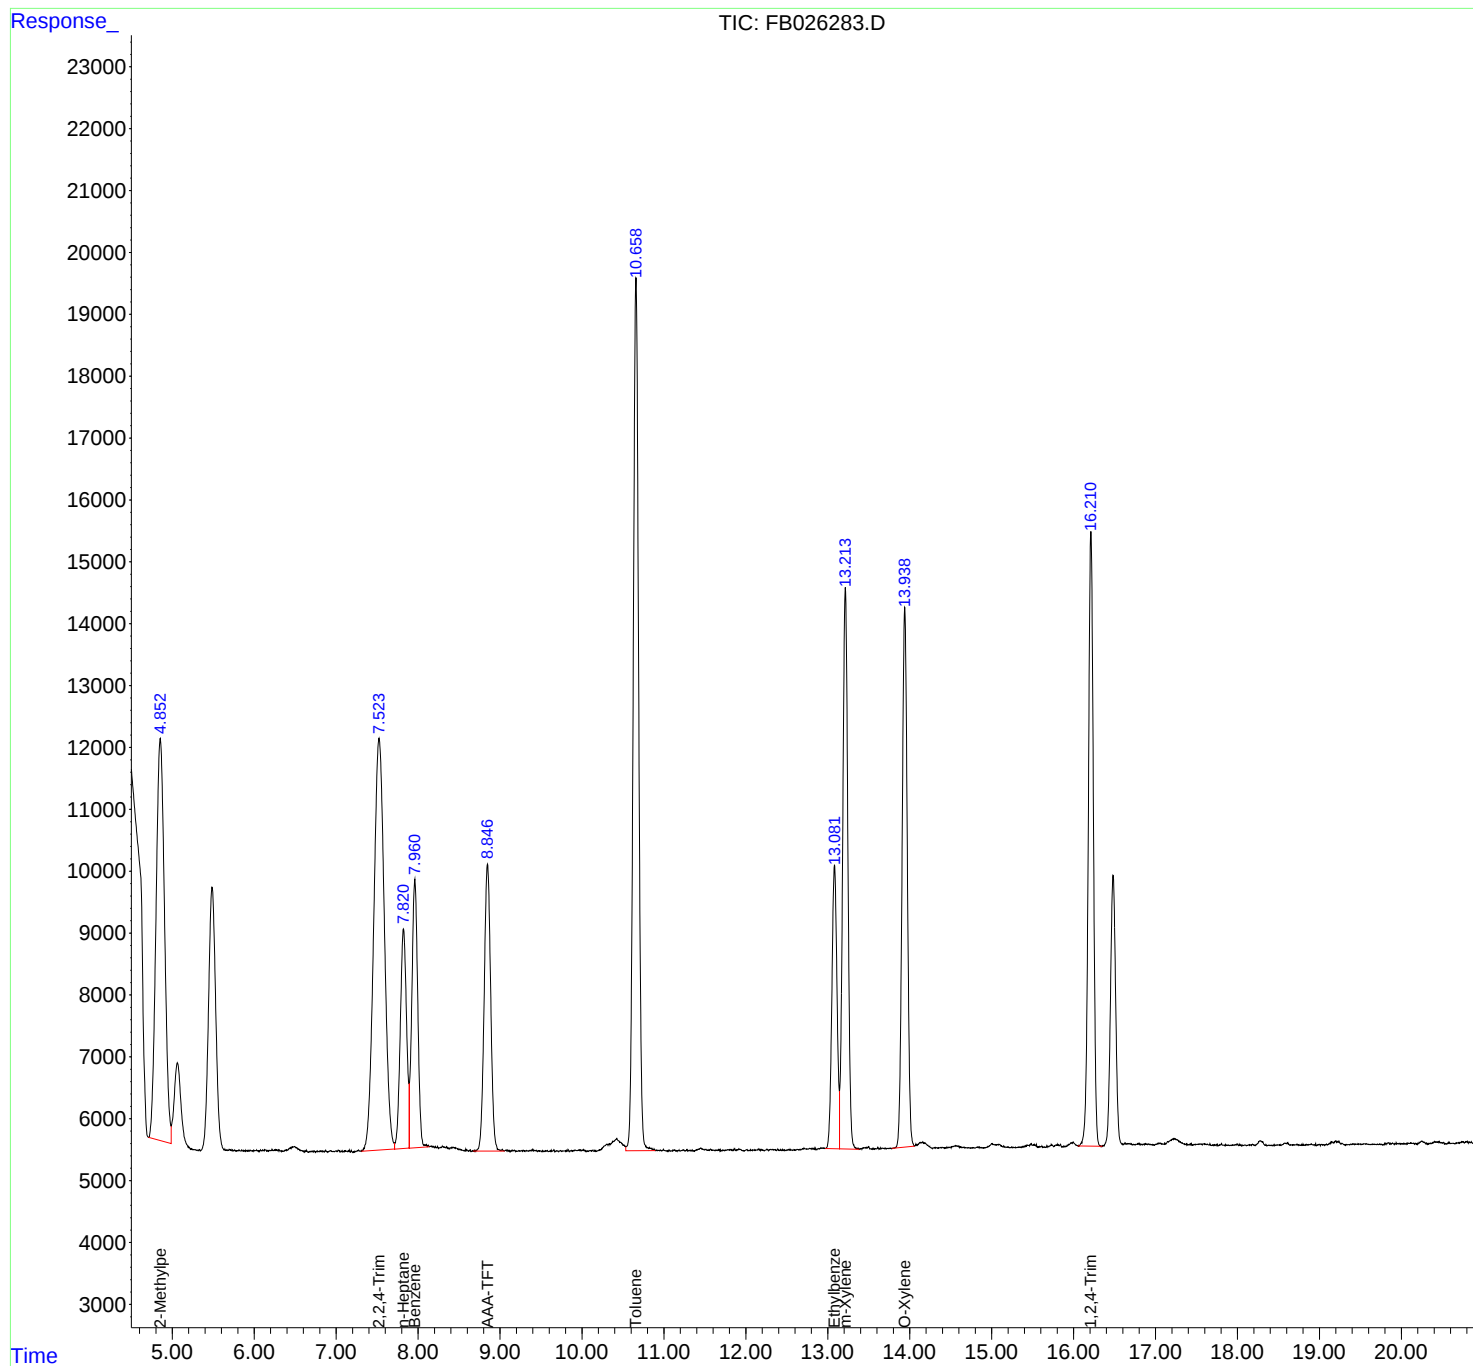


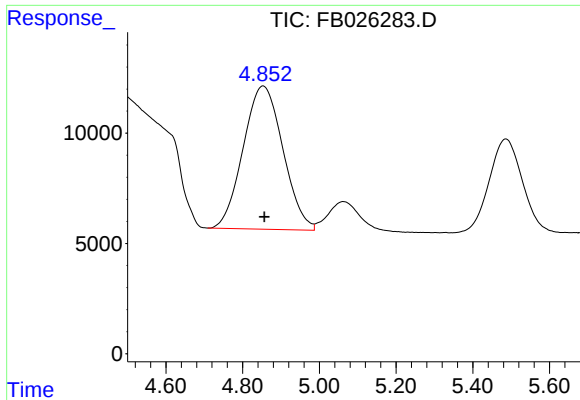

#1 2-Methylpentane


R.T.: 4.854 min
Delta R.T.: -0.003 min
Response: 467177
Conc: 26.84 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1014S1

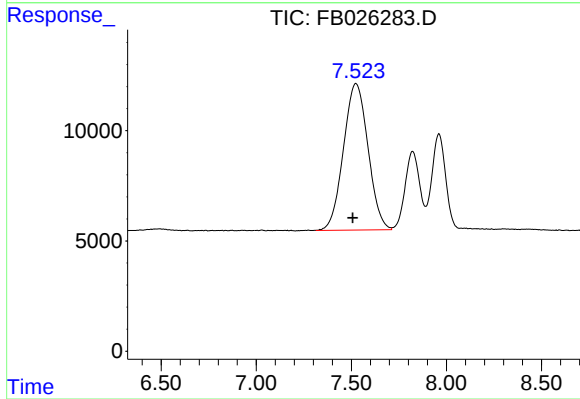


#2 2,2,4-Trimethylpentane

R.T.: 7.524 min
Delta R.T.: 0.018 min
Response: 596719
Conc: 28.89 ng/ml

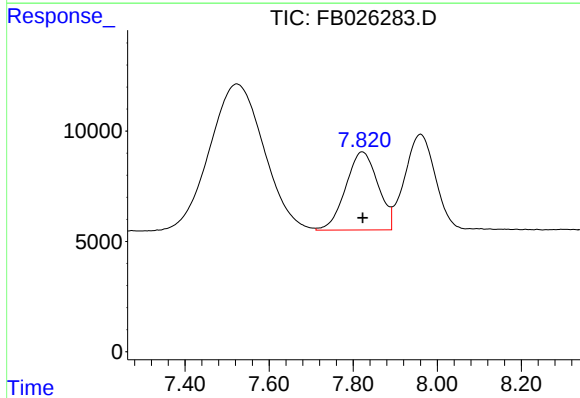


#3 n-Heptane

R.T.: 7.822 min
Delta R.T.: -0.001 min
Response: 189074
Conc: 8.07 ng/ml

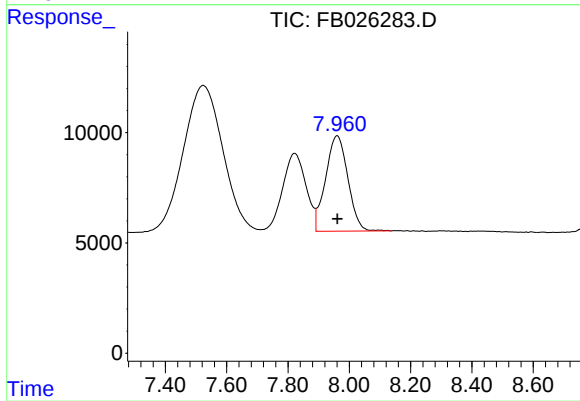

#4 Benzene


R.T.: 7.961 min
Delta R.T.: 0.000 min
Response: 218436
Conc: 8.35 ng/ml

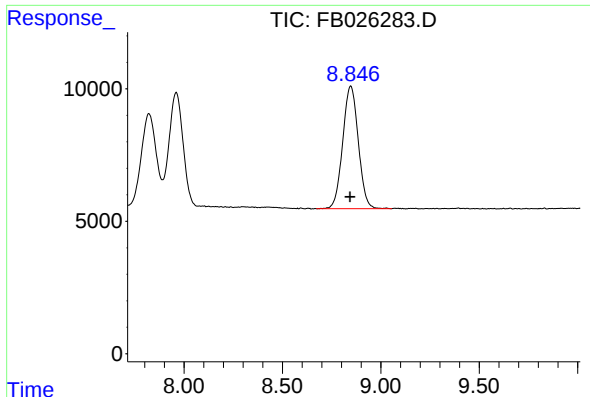

#5 AAA-TFT


R.T.: 8.847 min
Delta R.T.: 0.003 min
Response: 254174
Conc: 16.87 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1014S1

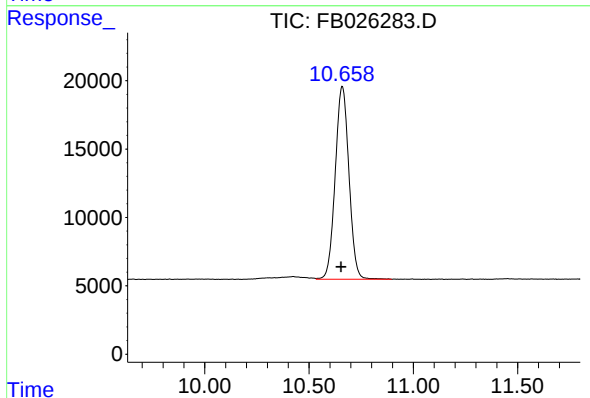


#6 Toluene

R.T.: 10.660 min
Delta R.T.: 0.007 min
Response: 644903
Conc: 24.89 ng/ml

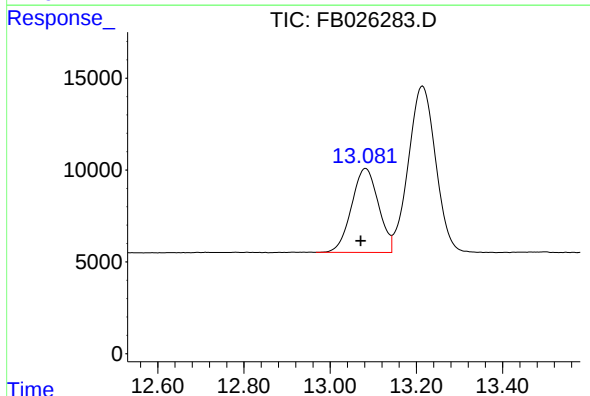


#7 Ethylbenzene

R.T.: 13.082 min
Delta R.T.: 0.012 min
Response: 197779
Conc: 8.66 ng/ml

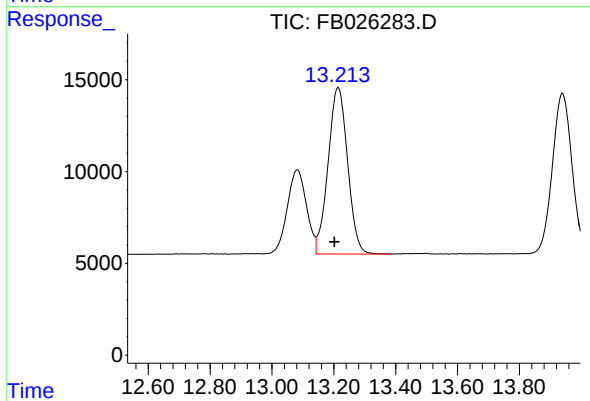

#8 m-Xylene

R.T.: 13.214 min
Delta R.T.: 0.012 min
Response: 397883
Conc: 17.74 ng/ml

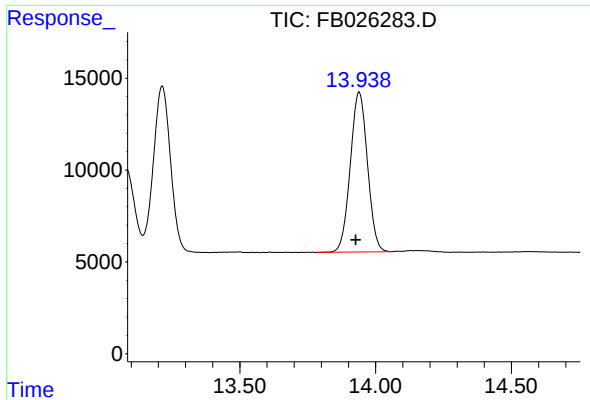

#9 O-Xylene


R.T.: 13.940 min

Delta R.T.: 0.013 min

Response: 382297

Conc: 18.07 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1014S1

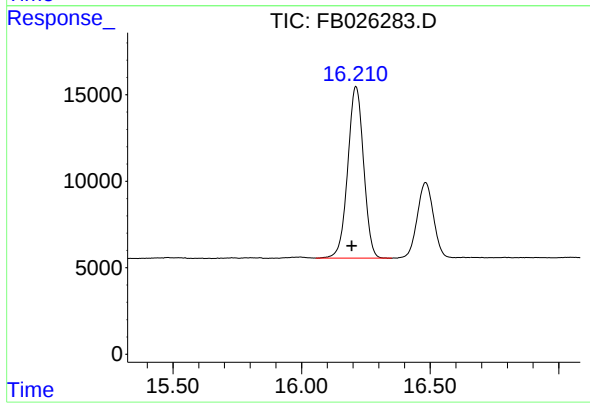

#10 1,2,4-Trimethylbenzene

R.T.: 16.212 min

Delta R.T.: 0.017 min

Response: 424470

Conc: 18.24 ng/ml