

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101422\
 Data File : FB028613.D
 Signal(s) : FID2B.CH
 Acq On : 14 Oct 2022 11:33
 Operator : AJ/MA
 Sample : BSF1014S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1014S1

Integration File: SAMPLE.e
 Quant Time: Oct 15 14:22:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	261493	20.213 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	527160	32.224 ng/ml
2) t 2,2,4-Trimethylpentane	7.428	559413	30.955 ng/ml
3) t n-Heptane	7.753	185854	10.972 ng/ml
4) t Benzene	7.890	220141	10.023 ng/ml
6) t Toluene	10.623	637940	30.436 ng/ml
7) t Ethylbenzene	13.059	195199	9.835 ng/ml
8) t m-Xylene	13.192	387344	19.661 ng/ml
9) t O-Xylene	13.919	369348	18.985 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	363721	18.788 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101422\
Data File : FB028613.D
Signal(s) : FID2B.CH
Acq On : 14 Oct 2022 11:33
Operator : AJ/MA
Sample : BSF1014S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1014S1

Integration File: SAMPLE.e
Quant Time: Oct 15 14:22:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

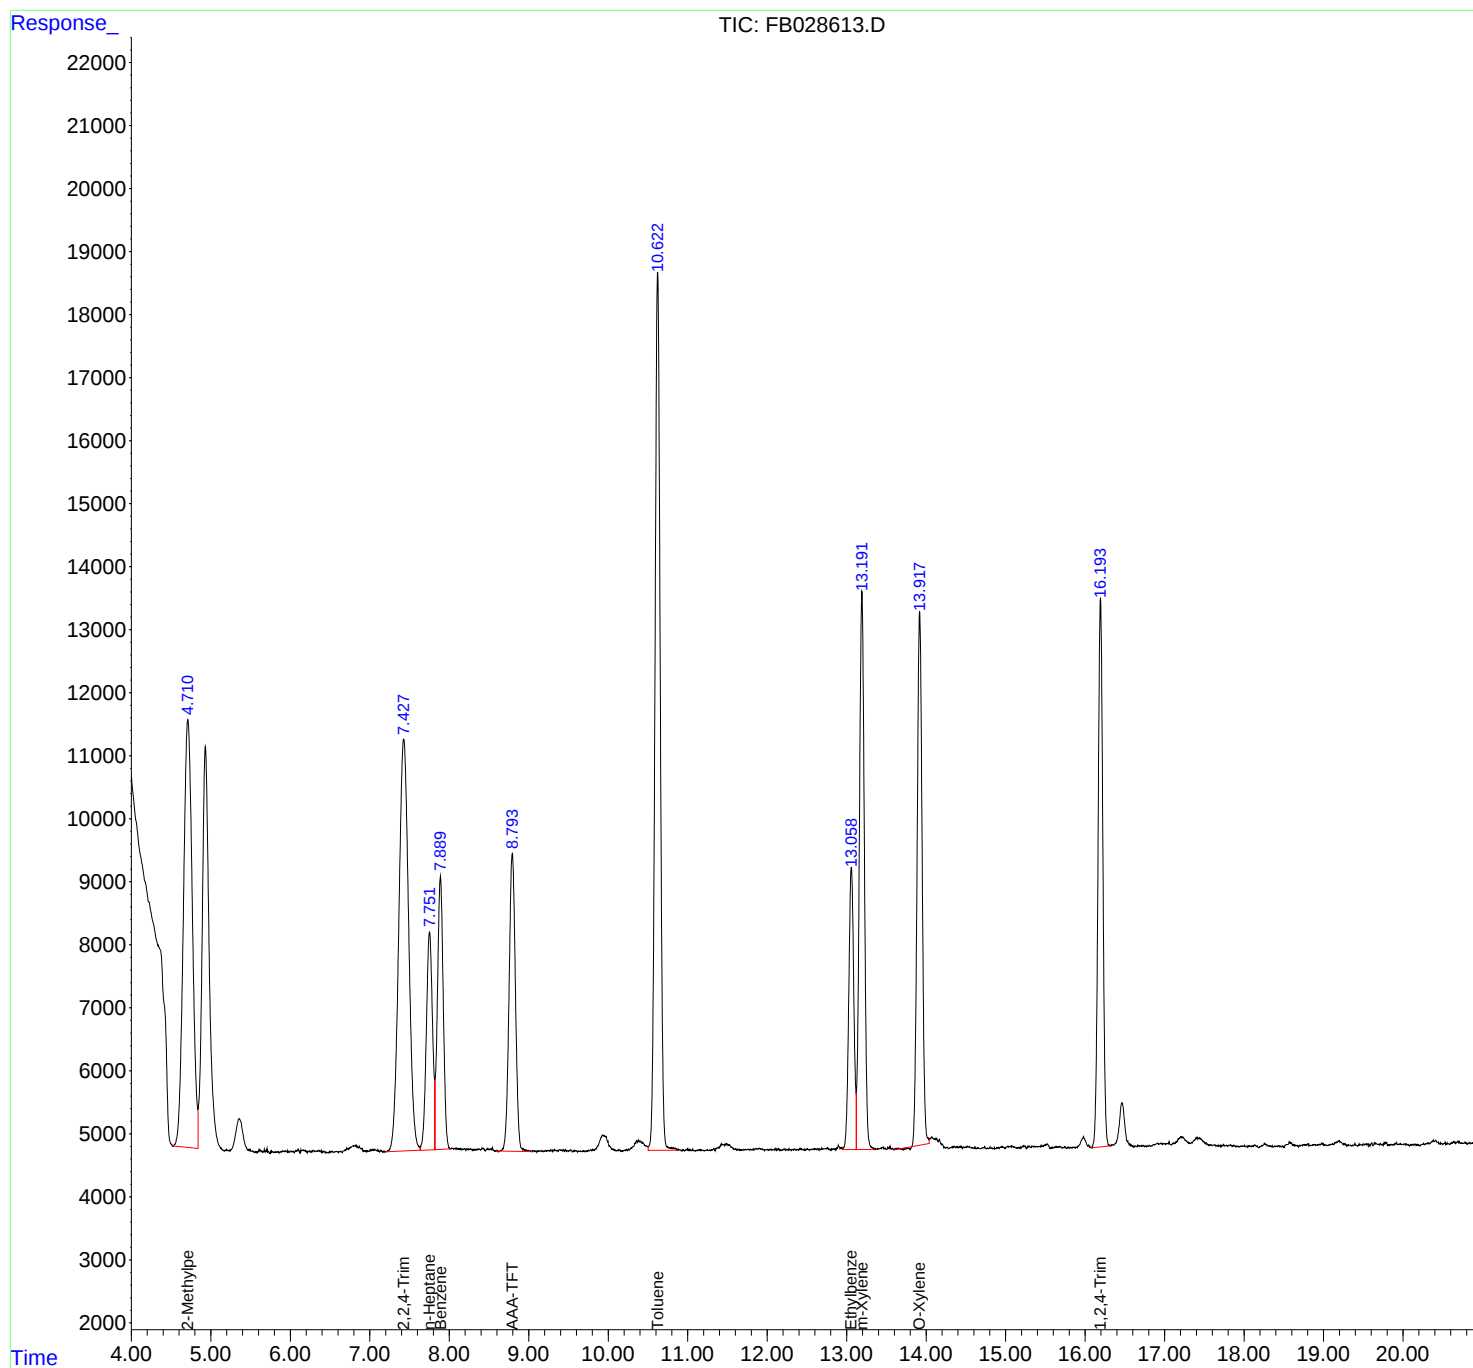


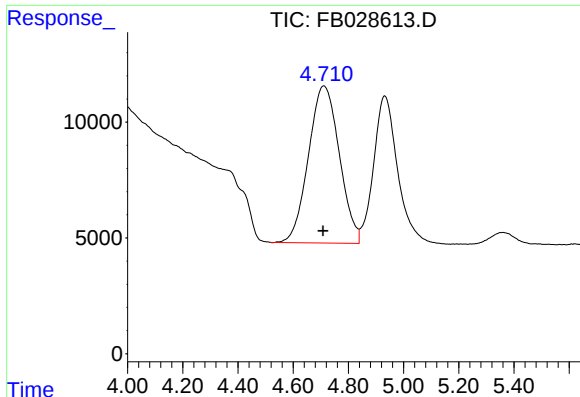

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: 0.004 min
Response: 527160
Conc: 32.22 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1014S1

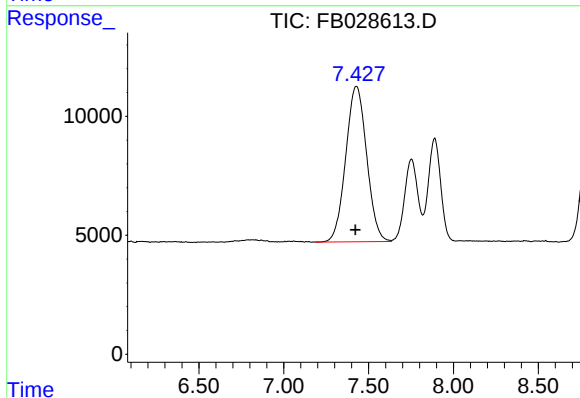


#2 2,2,4-Trimethylpentane

R.T.: 7.428 min
Delta R.T.: 0.005 min
Response: 559413
Conc: 30.95 ng/ml

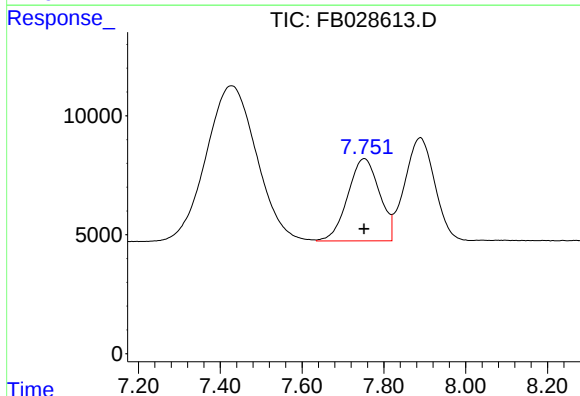


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.002 min
Response: 185854
Conc: 10.97 ng/ml

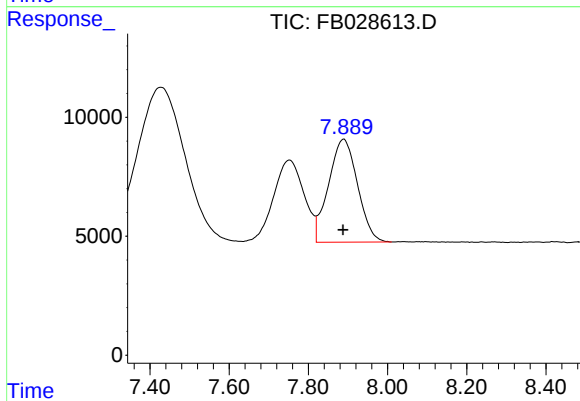

#4 Benzene


R.T.: 7.890 min
Delta R.T.: 0.002 min
Response: 220141
Conc: 10.02 ng/ml

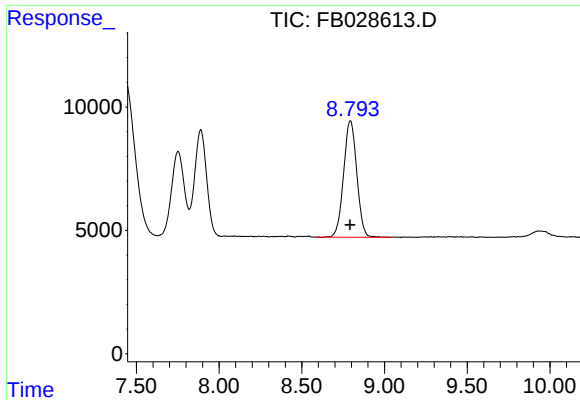

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.001 min
Response: 261493
Conc: 20.21 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1014S1

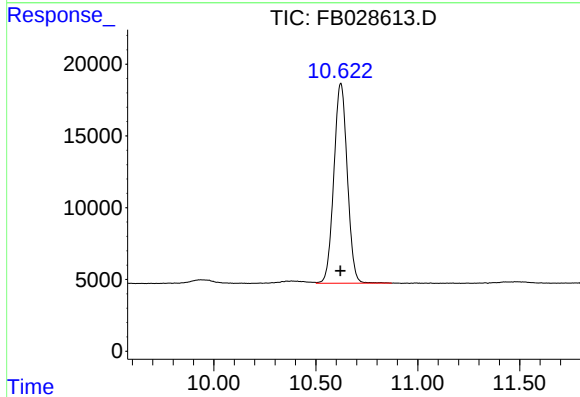


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.002 min
Response: 637940
Conc: 30.44 ng/ml

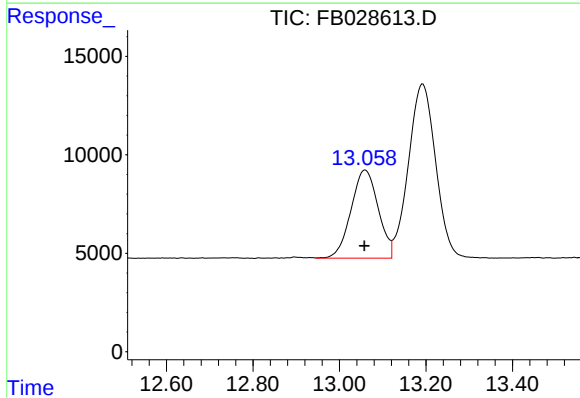


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.001 min
Response: 195199
Conc: 9.84 ng/ml

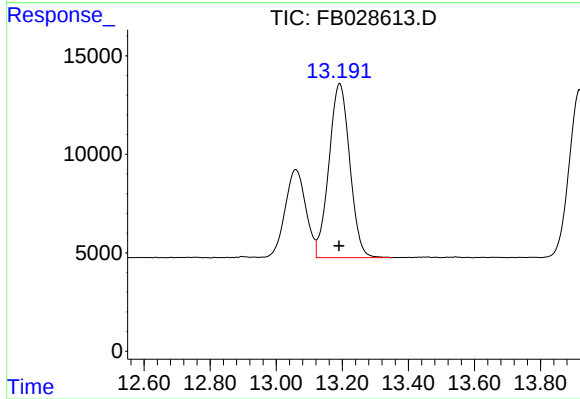

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: 0.002 min
Response: 387344
Conc: 19.66 ng/ml

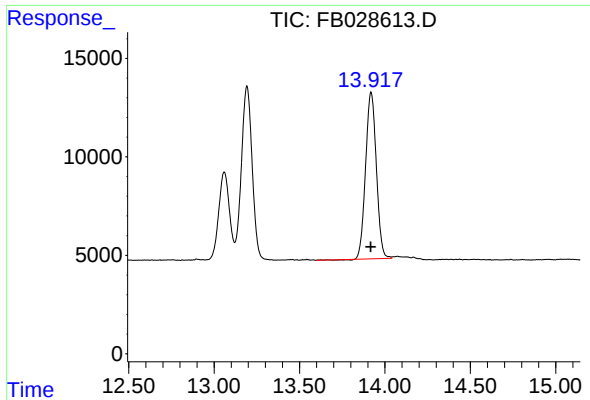

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.002 min
Response: 369348
Conc: 18.99 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1014S1

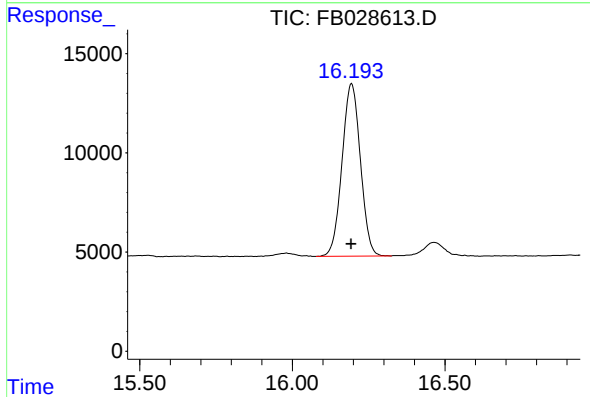

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.002 min
Response: 363721
Conc: 18.79 ng/ml