

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101518\
 Data File : FB018229.D
 Signal(s) : FID2B.CH
 Acq On : 15 Oct 2018 9:15
 Operator : MJ/SJ
 Sample : BSF1015S1
 Misc : 5.01g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 15 13:52:06 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.108	138228	16.049 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.960	366480	23.962 ng/ml
2) t 2,2,4-Trimethylpentane	7.726	383585	25.959 ng/ml
3) t n-Heptane	8.063	120915	8.532 ng/ml
4) t Benzene	8.203	164356	8.823 ng/ml
6) t Toluene	10.958	386920	25.387 ng/ml
7) t Ethylbenzene	13.407	126884	7.997 ng/ml
8) t m-Xylene	13.540	271603	16.323 ng/ml
9) t O-Xylene	14.271	287977	16.152 ng/ml
10) t 1,2,4-Trimethylbenzene	16.554	338601	16.644 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101518\
Data File : FB018229.D
Signal(s) : FID2B.CH
Acq On : 15 Oct 2018 9:15
Operator : MJ/SJ
Sample : BSF1015S1
Misc : 5.01g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 15 13:52:06 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

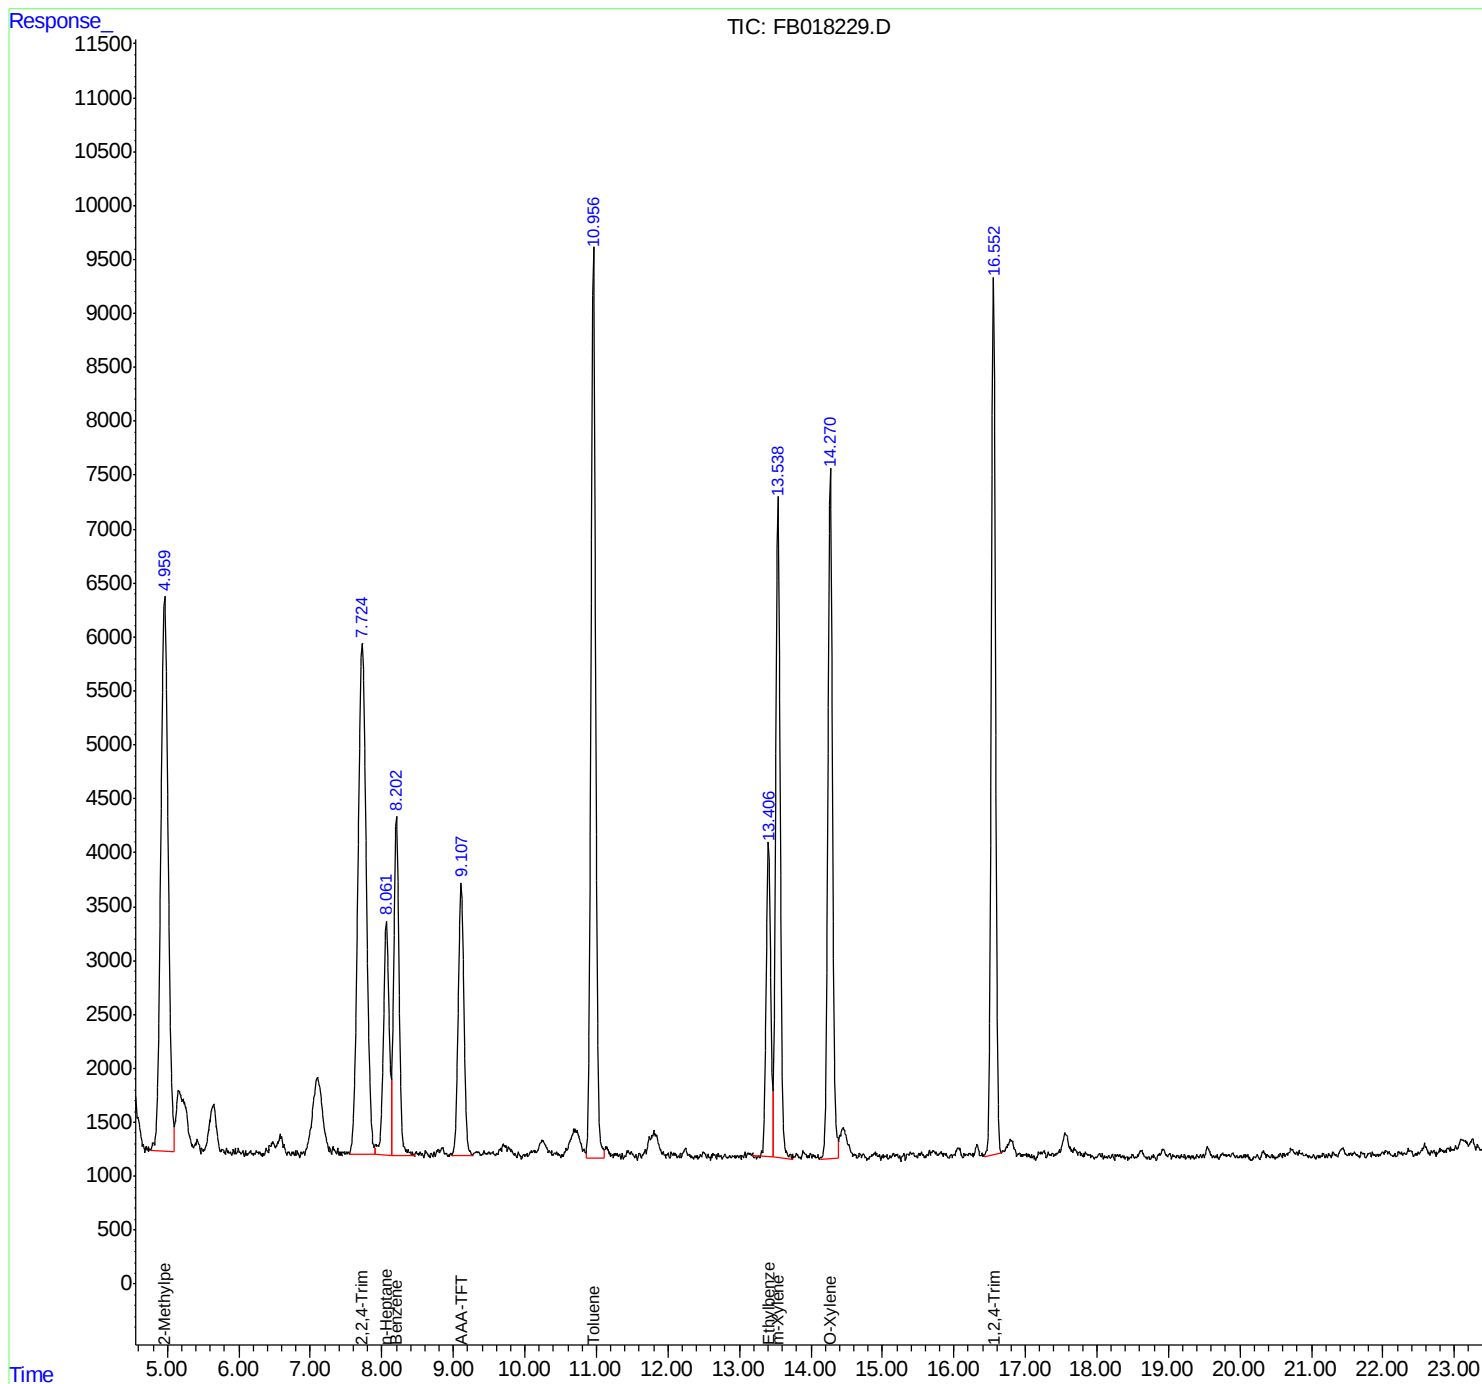

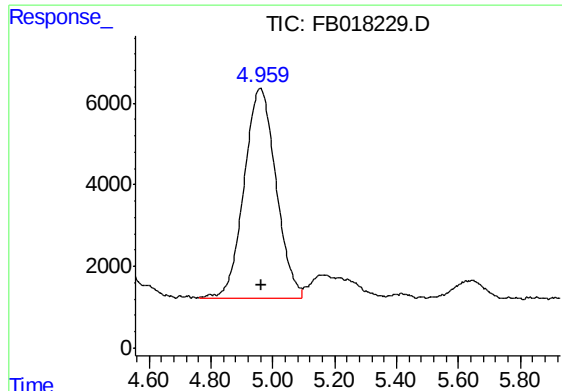


#1 2-Methylpentane

R.T.: 4.960 min
Delta R.T.: -0.005 min
Response: 366480
Conc: 23.96 ng/ml

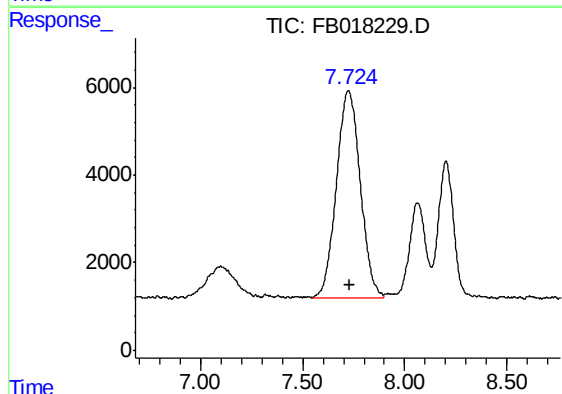


#2 2,2,4-Trimethylpentane

R.T.: 7.726 min
Delta R.T.: -0.003 min
Response: 383585
Conc: 25.96 ng/ml

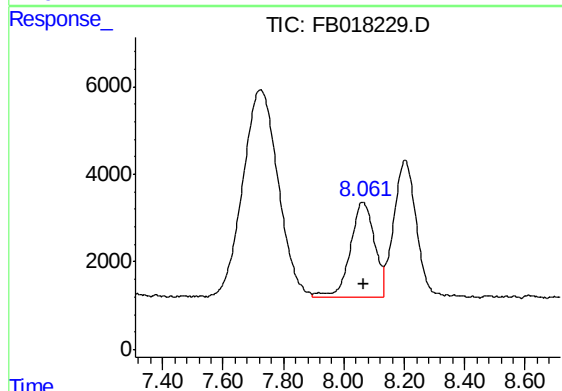


#3 n-Heptane

R.T.: 8.063 min
Delta R.T.: -0.005 min
Response: 120915
Conc: 8.53 ng/ml

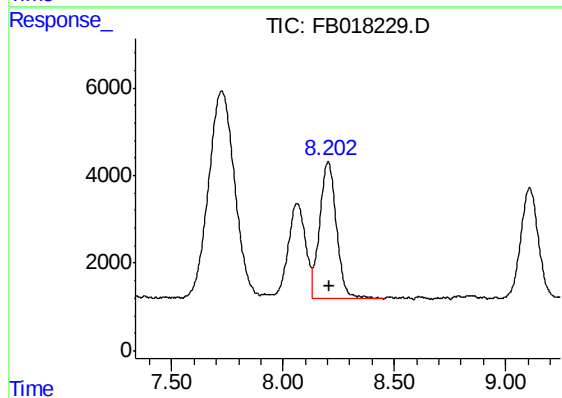


#4 Benzene

R.T.: 8.203 min
Delta R.T.: -0.004 min
Response: 164356
Conc: 8.82 ng/ml

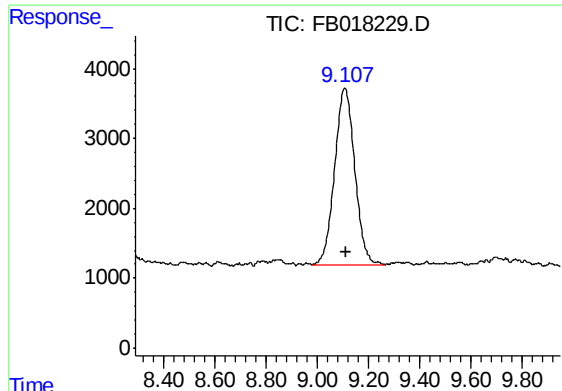


#5 AAA-TFT

R.T.: 9.108 min
Delta R.T.: -0.004 min
Response: 138228
Conc: 16.05 ng/ml

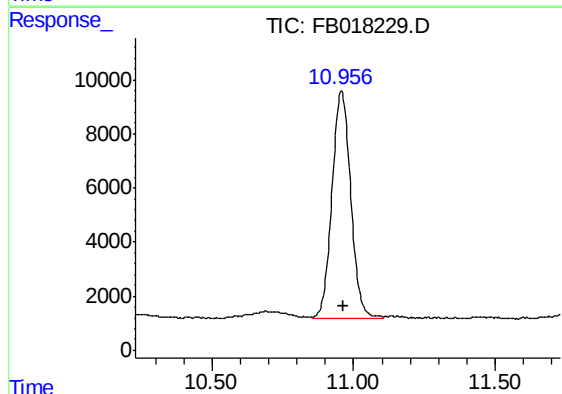


#6 Toluene

R.T.: 10.958 min
Delta R.T.: -0.005 min
Response: 386920
Conc: 25.39 ng/ml

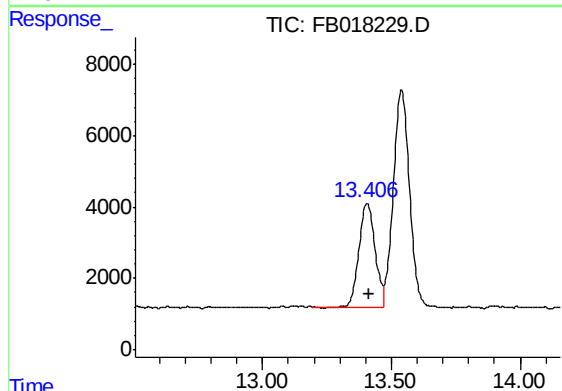


#7 Ethylbenzene

R.T.: 13.407 min
Delta R.T.: -0.005 min
Response: 126884
Conc: 8.00 ng/ml

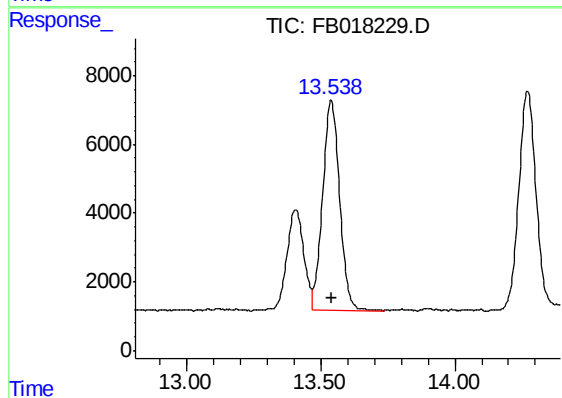


#8 m-Xylene

R.T.: 13.540 min
Delta R.T.: -0.005 min
Response: 271603
Conc: 16.32 ng/ml

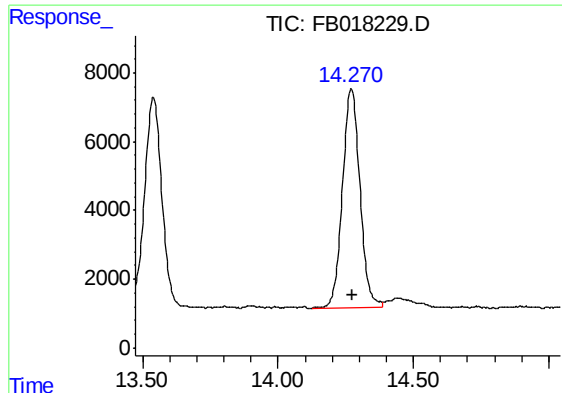

#9 O-Xylene

R.T.: 14.271 min
Delta R.T.: -0.005 min
Response: 287977
Conc: 16.15 ng/ml

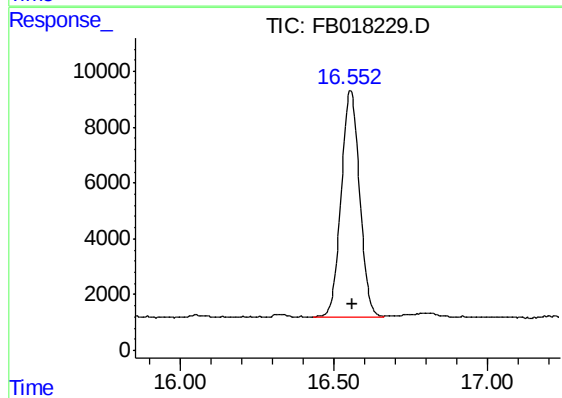

#10 1,2,4-Trimethylbenzene

R.T.: 16.554 min
Delta R.T.: -0.005 min
Response: 338601
Conc: 16.64 ng/ml