

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101520\
 Data File : FB025073.D
 Signal(s) : FID2B.CH
 Acq On : 15 Oct 2020 14:32
 Operator : DD/AJ
 Sample : L4223-02MSD
 Misc : 5.07/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 16 00:38:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.802	440116	20.964 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.691	772512	25.687 ng/ml
2) t	2,2,4-Trimethylpentane	7.420	806009	26.371 ng/ml
3) t	n-Heptane	7.760	260553	8.565 ng/ml
4) t	Benzene	7.896	373601	10.029 ng/ml
6) t	Toluene	10.633	1013908	29.044 ng/ml
7) t	Ethylbenzene	13.073	303856	9.374 ng/ml
8) t	m-Xylene	13.205	597567	18.811 ng/ml
9) t	O-Xylene	13.933	577296	18.998 ng/ml
10) t	1,2,4-Trimethylbenzene	16.211	453778	17.891 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101520\
Data File : FB025073.D
Signal(s) : FID2B.CH
Acq On : 15 Oct 2020 14:32
Operator : DD/AJ
Sample : L4223-02MSD
Misc : 5.07/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 16 00:38:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

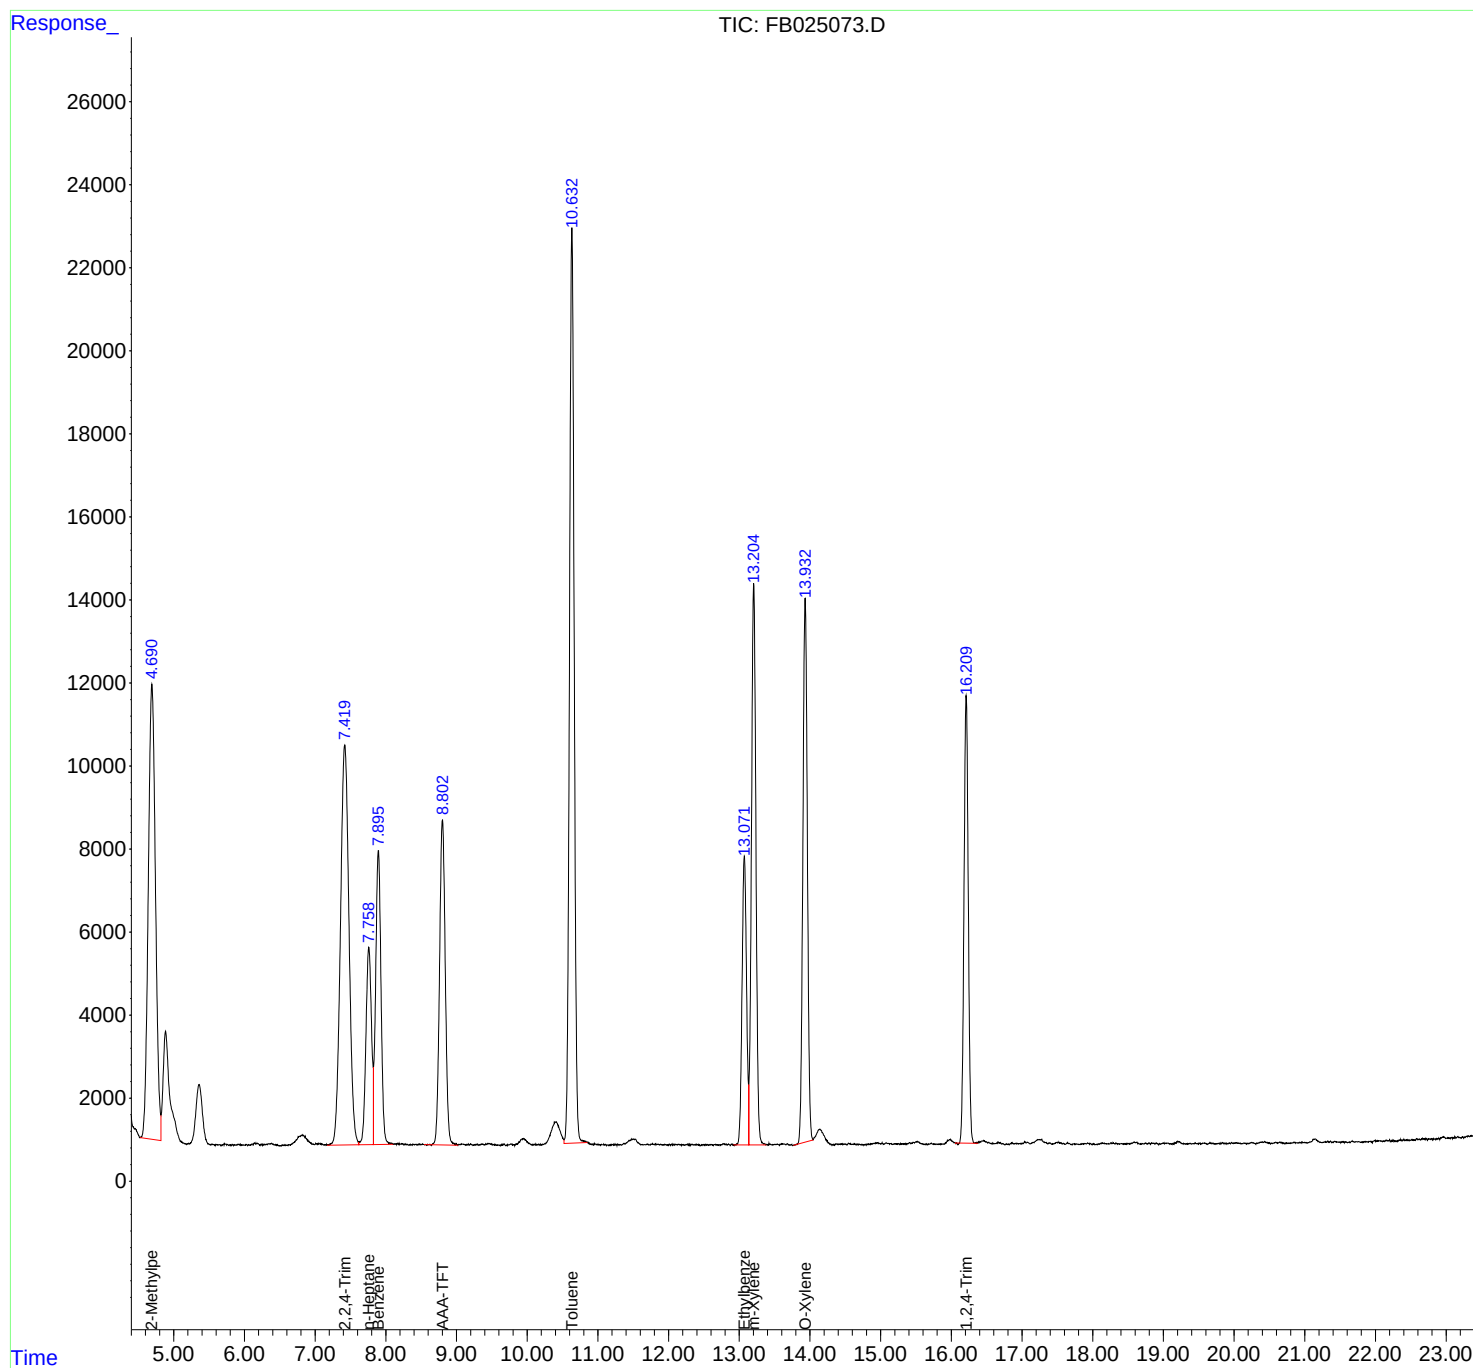

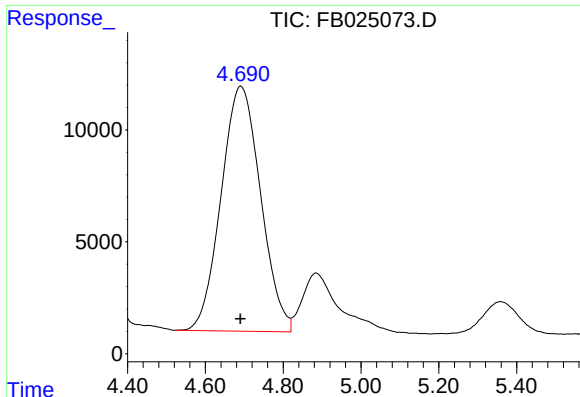


#1 2-Methylpentane

R.T.: 4.691 min
Delta R.T.: 0.001 min
Response: 772512
Conc: 25.69 ng/ml

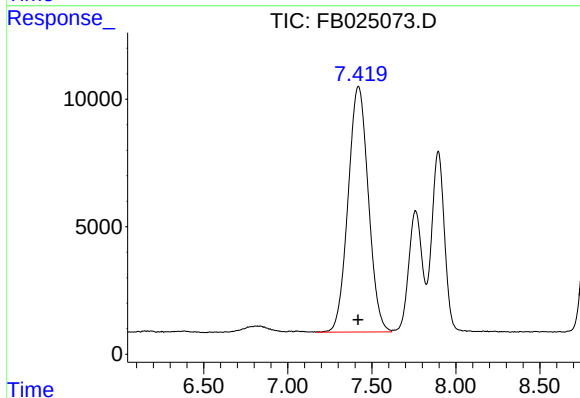


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.002 min
Response: 806009
Conc: 26.37 ng/ml

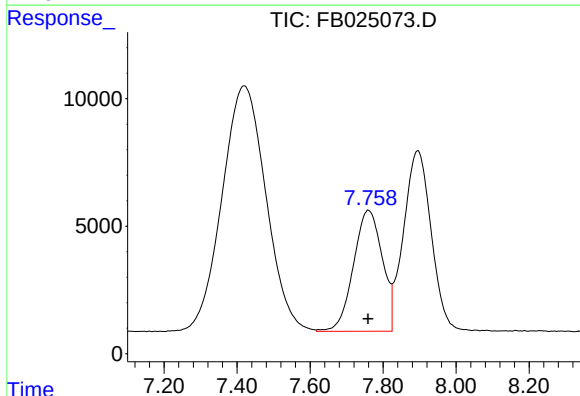


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 260553
Conc: 8.56 ng/ml

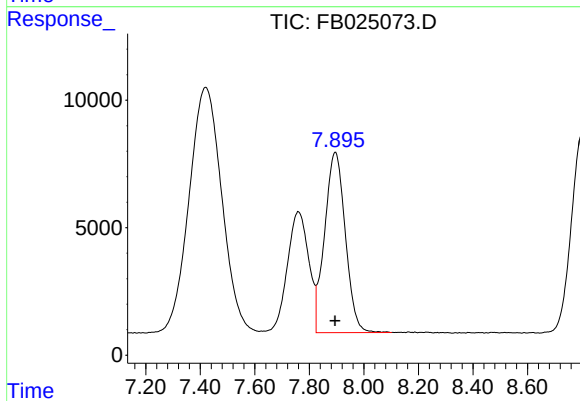


#4 Benzene

R.T.: 7.896 min
Delta R.T.: 0.000 min
Response: 373601
Conc: 10.03 ng/ml

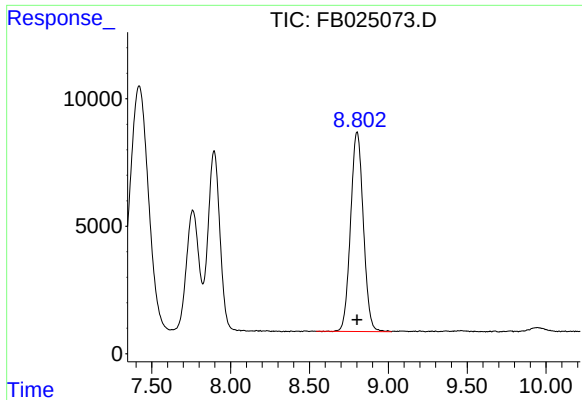


#5 AAA-TFT

R.T.: 8.802 min
Delta R.T.: 0.002 min
Response: 440116
Conc: 20.96 ng/ml

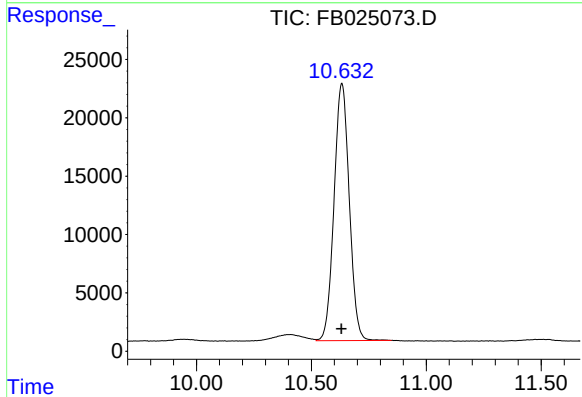


#6 Toluene

R.T.: 10.633 min
Delta R.T.: 0.002 min
Response: 1013908
Conc: 29.04 ng/ml

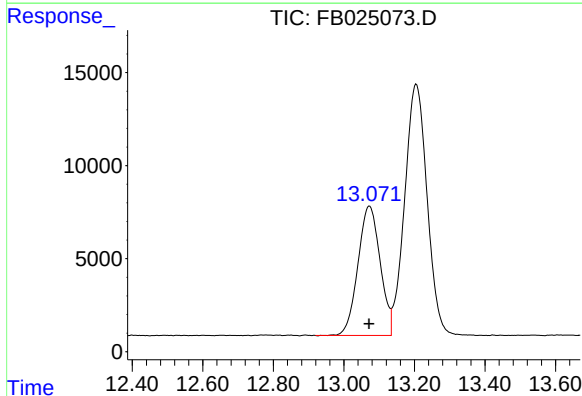


#7 Ethylbenzene

R.T.: 13.073 min
Delta R.T.: 0.001 min
Response: 303856
Conc: 9.37 ng/ml

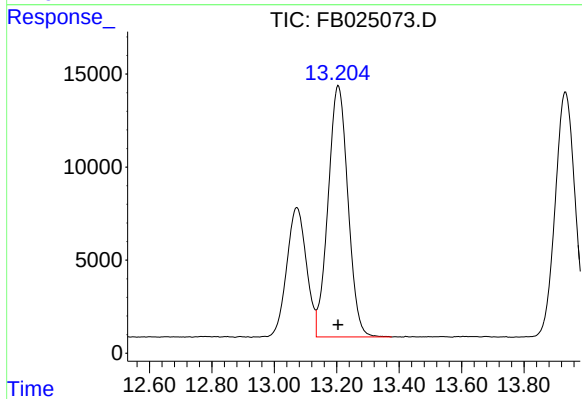


#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.001 min
Response: 597567
Conc: 18.81 ng/ml

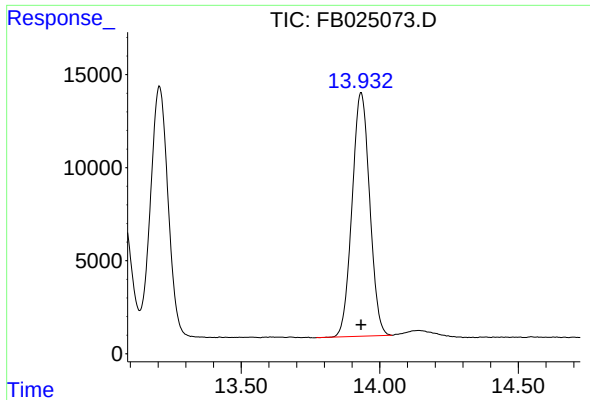

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.001 min
Response: 577296
Conc: 19.00 ng/ml

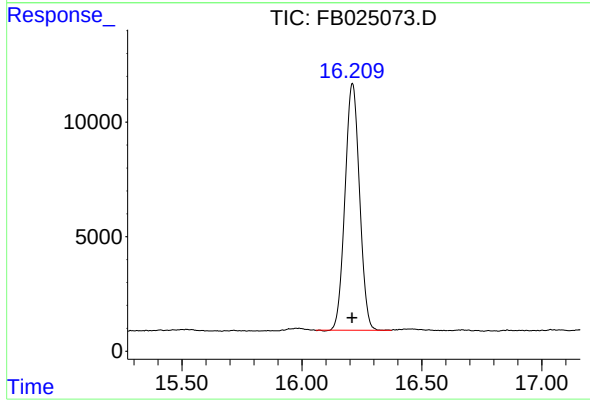

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.001 min
Response: 453778
Conc: 17.89 ng/ml