

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101520\
 Data File : FB025067.D
 Signal(s) : FID2B.CH
 Acq On : 15 Oct 2020 11:28
 Operator : DD/AJ
 Sample : BSF1015S1
 Misc : 5.00/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 16 00:37:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.802	422768	20.137 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.693	867858	28.858 ng/ml
2) t	2,2,4-Trimethylpentane	7.420	965785	31.599 ng/ml
3) t	n-Heptane	7.760	315650	10.376 ng/ml
4) t	Benzene	7.896	383285	10.289 ng/ml
6) t	Toluene	10.633	1069975	30.650 ng/ml
7) t	Ethylbenzene	13.072	328193	10.125 ng/ml
8) t	m-Xylene	13.205	649487	20.446 ng/ml
9) t	O-Xylene	13.933	623057	20.504 ng/ml
10) t	1,2,4-Trimethylbenzene	16.210	507581	20.013 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101520\
Data File : FB025067.D
Signal(s) : FID2B.CH
Acq On : 15 Oct 2020 11:28
Operator : DD/AJ
Sample : BSF1015S1
Misc : 5.00/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 16 00:37:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

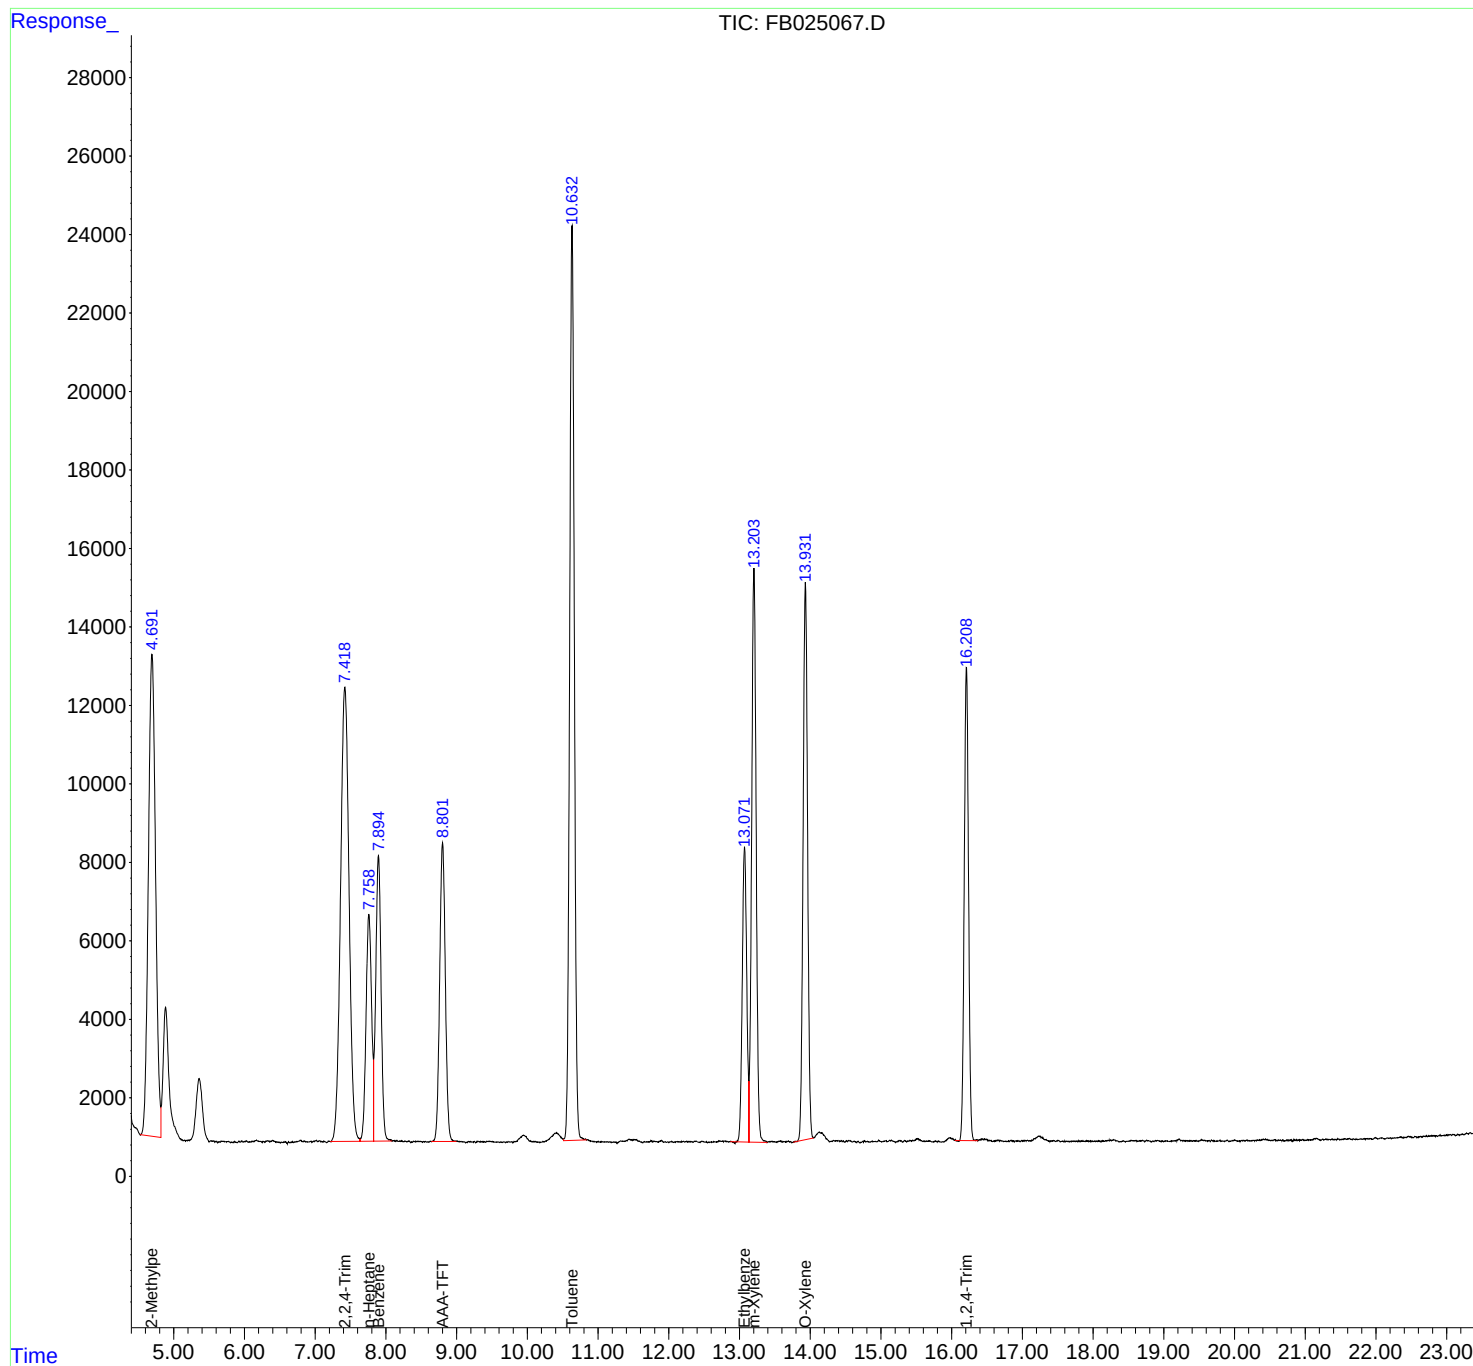

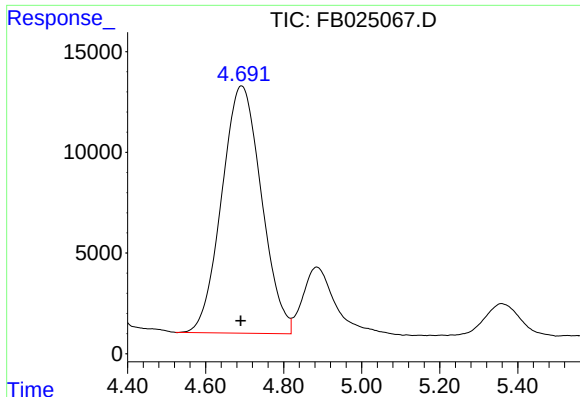


#1 2-Methylpentane

R.T.: 4.693 min
Delta R.T.: 0.003 min
Response: 867858
Conc: 28.86 ng/ml

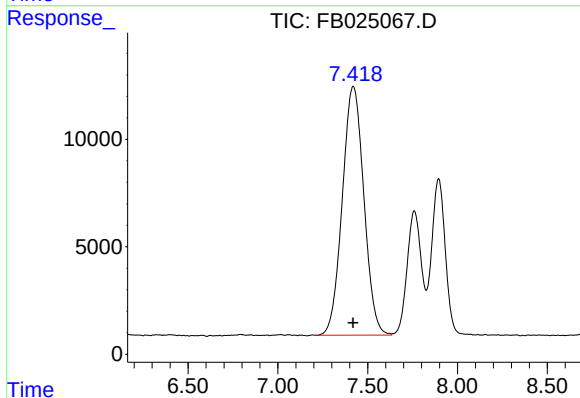


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.001 min
Response: 965785
Conc: 31.60 ng/ml

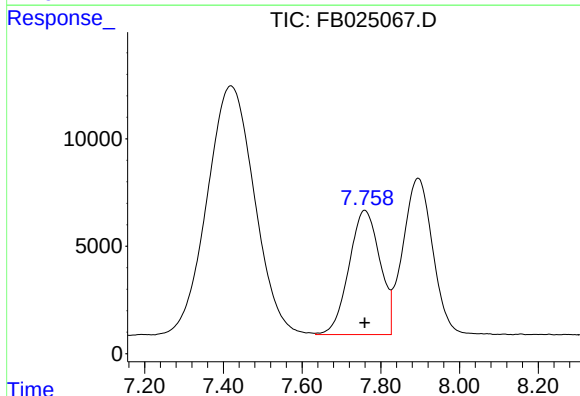


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 315650
Conc: 10.38 ng/ml

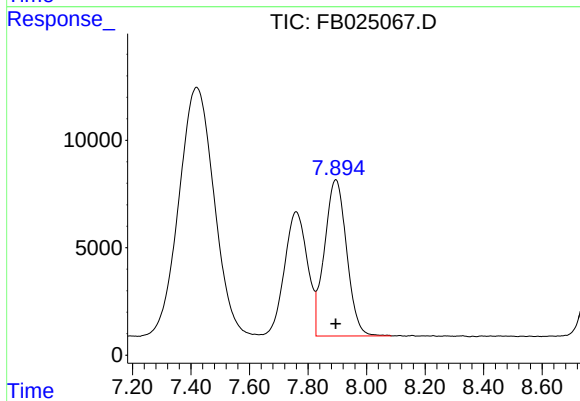


#4 Benzene

R.T.: 7.896 min
Delta R.T.: 0.000 min
Response: 383285
Conc: 10.29 ng/ml

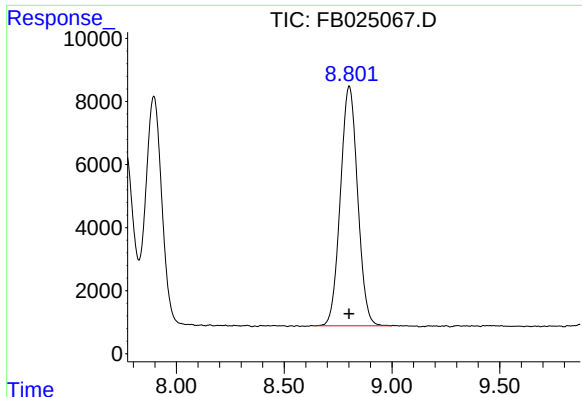


#5 AAA-TFT

R.T.: 8.802 min
Delta R.T.: 0.001 min
Response: 422768
Conc: 20.14 ng/ml

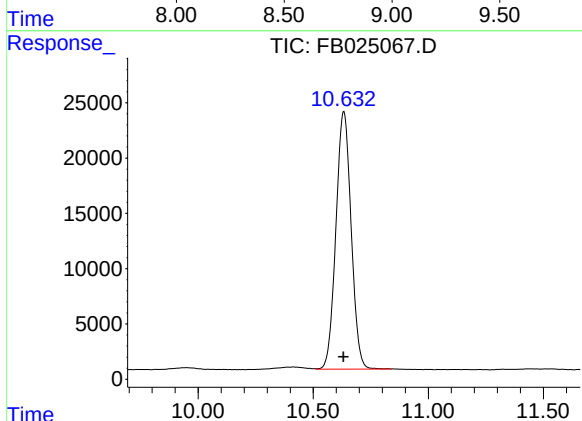


#6 Toluene

R.T.: 10.633 min
Delta R.T.: 0.001 min
Response: 1069975
Conc: 30.65 ng/ml

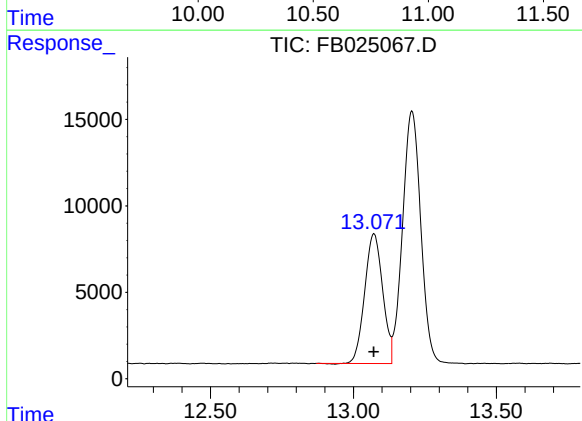


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 328193
Conc: 10.12 ng/ml

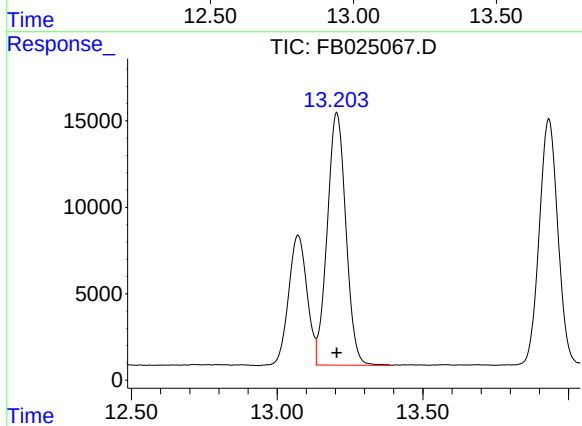


#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.000 min
Response: 649487
Conc: 20.45 ng/ml

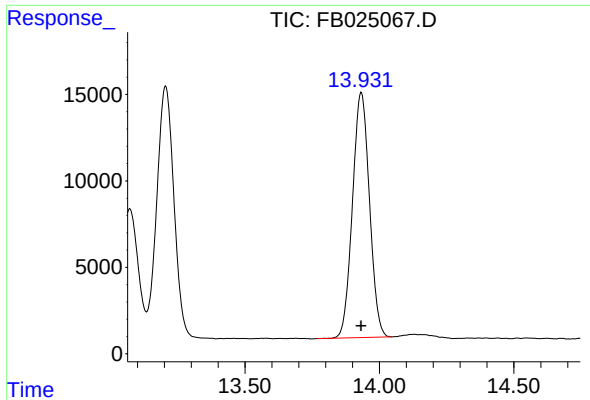

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.000 min
Response: 623057
Conc: 20.50 ng/ml

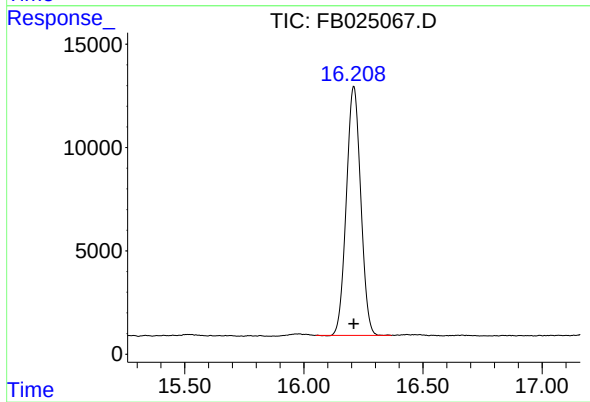

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 507581
Conc: 20.01 ng/ml