

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101618\
 Data File : FB018251.D
 Signal(s) : FID2B.CH
 Acq On : 16 Oct 2018 2:42 pm
 Operator : MJ/SJ
 Sample : J5524-07MSD
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 16 15:11:58 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.111	160048	18.583 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.962	465786	30.455 ng/ml
2) t 2,2,4-Trimethylpentane	7.726	448653	30.362 ng/ml
3) t n-Heptane	8.065	149456	10.546 ng/ml
4) t Benzene	8.204	188216	10.104 ng/ml
6) t Toluene	10.959	465745	30.559 ng/ml
7) t Ethylbenzene	13.409	162327	10.231 ng/ml
8) t m-Xylene	13.542	336663	20.233 ng/ml
9) t O-Xylene	14.273	358406	20.102 ng/ml
10) t 1,2,4-Trimethylbenzene	16.556	414003	20.351 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101618\
Data File : FB018251.D
Signal(s) : FID2B.CH
Acq On : 16 Oct 2018 2:42 pm
Operator : MJ/SJ
Sample : J5524-07MSD
Misc : 5.02g/5.00mL DI Water
ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 16 15:11:58 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

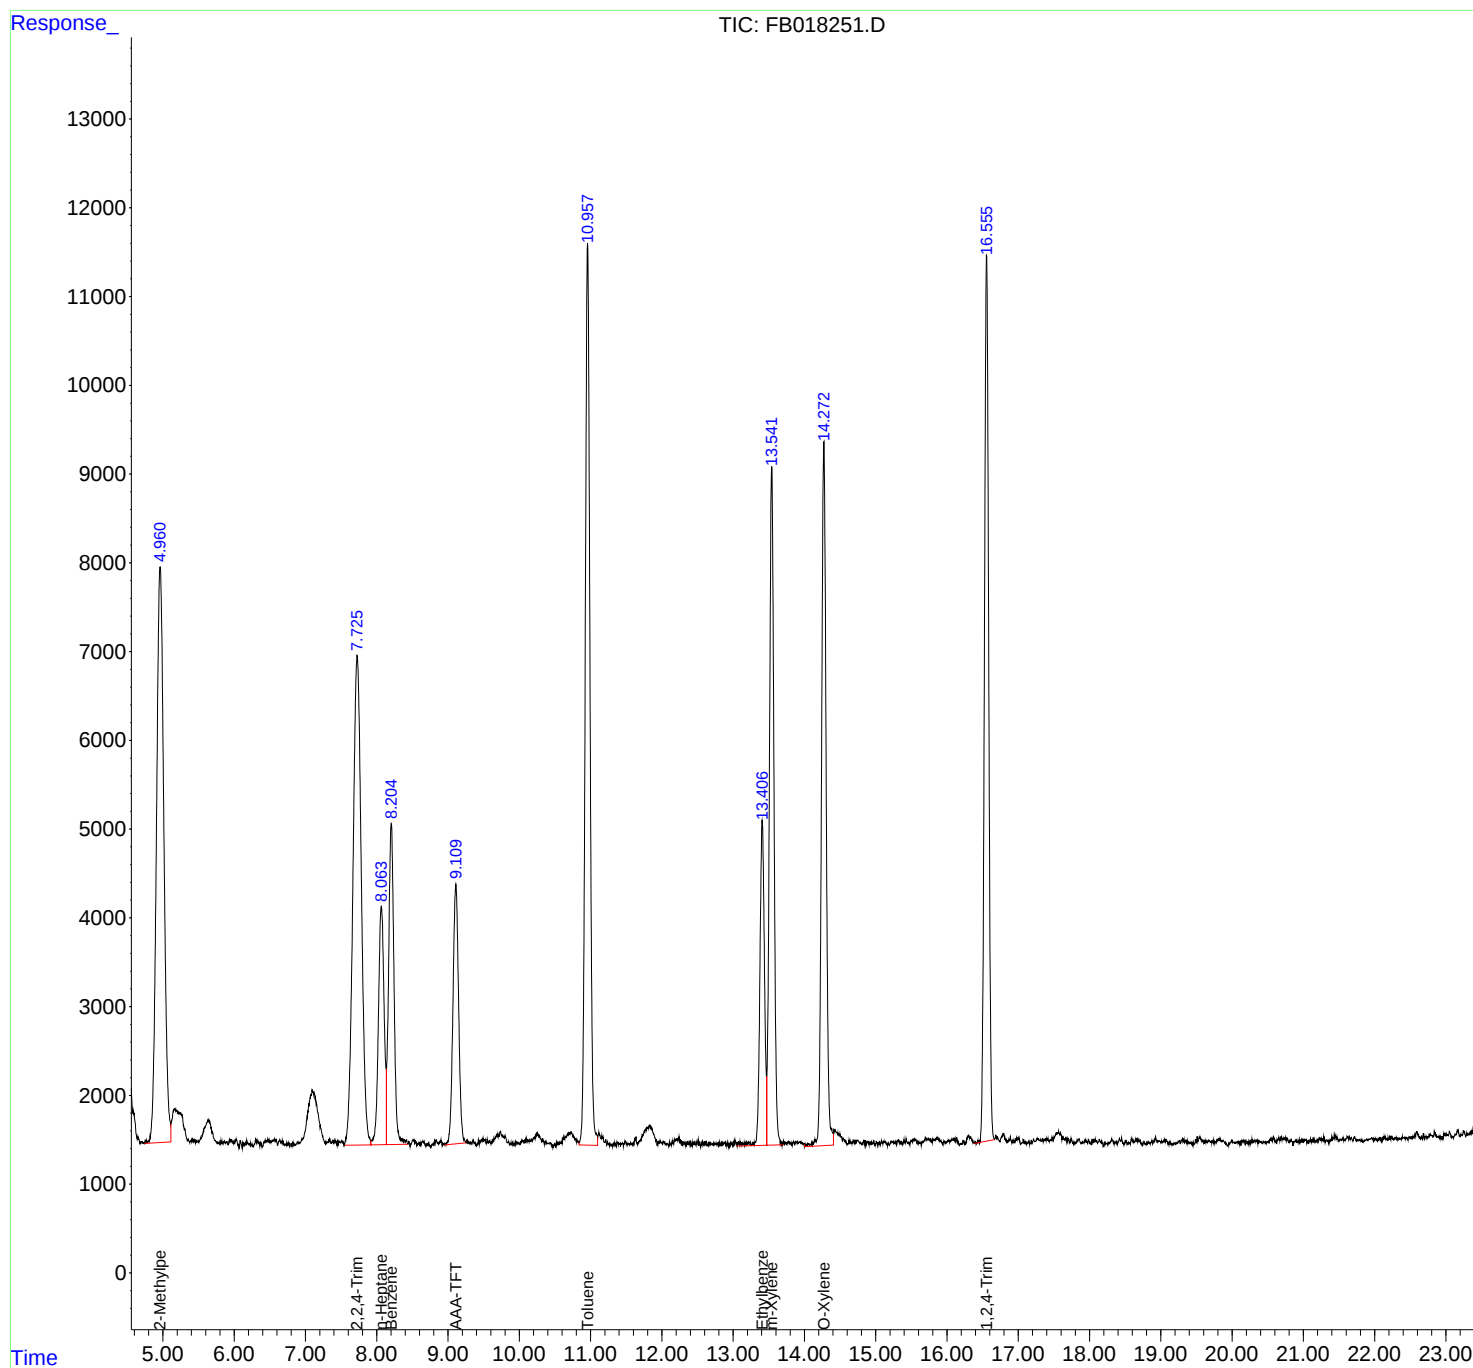

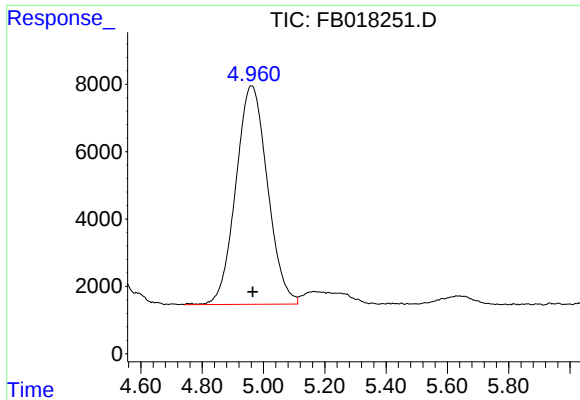


#1 2-Methylpentane

R.T.: 4.962 min
Delta R.T.: -0.003 min
Response: 465786
Conc: 30.45 ng/ml

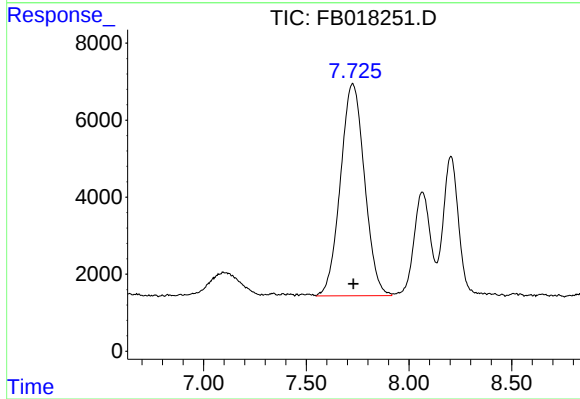


#2 2,2,4-Trimethylpentane

R.T.: 7.726 min
Delta R.T.: -0.003 min
Response: 448653
Conc: 30.36 ng/ml

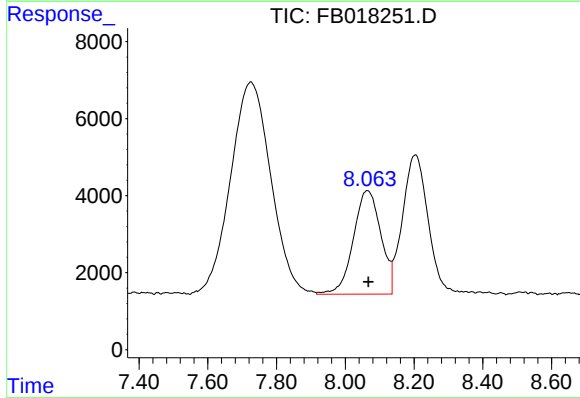


#3 n-Heptane

R.T.: 8.065 min
Delta R.T.: -0.003 min
Response: 149456
Conc: 10.55 ng/ml

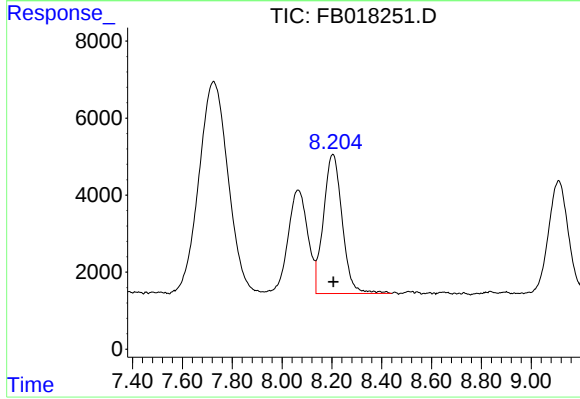


#4 Benzene

R.T.: 8.204 min
Delta R.T.: -0.003 min
Response: 188216
Conc: 10.10 ng/ml

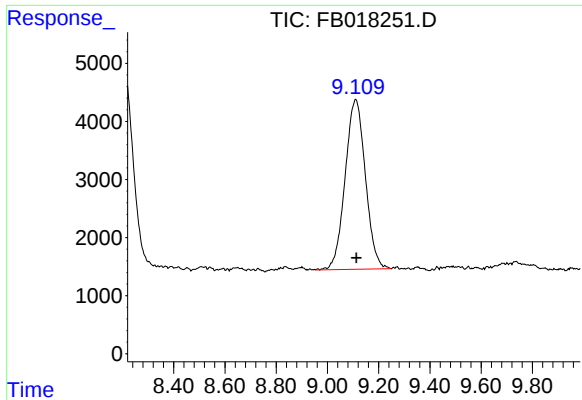


#5 AAA-TFT

R.T.: 9.111 min
Delta R.T.: -0.002 min
Response: 160048
Conc: 18.58 ng/ml

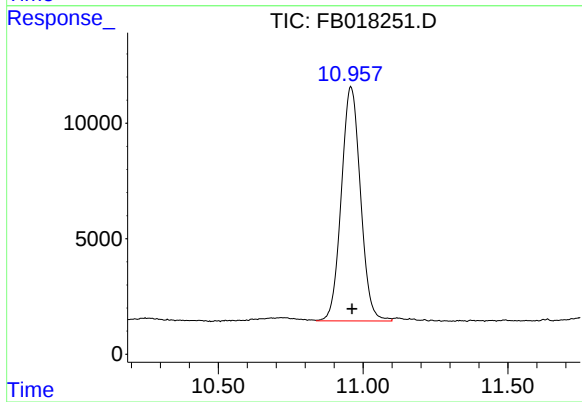


#6 Toluene

R.T.: 10.959 min
Delta R.T.: -0.003 min
Response: 465745
Conc: 30.56 ng/ml

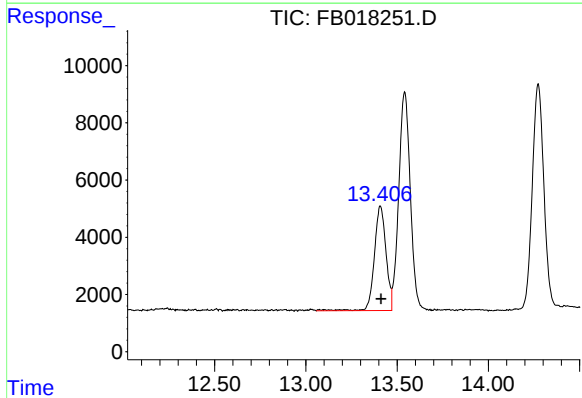


#7 Ethylbenzene

R.T.: 13.409 min
Delta R.T.: -0.004 min
Response: 162327
Conc: 10.23 ng/ml

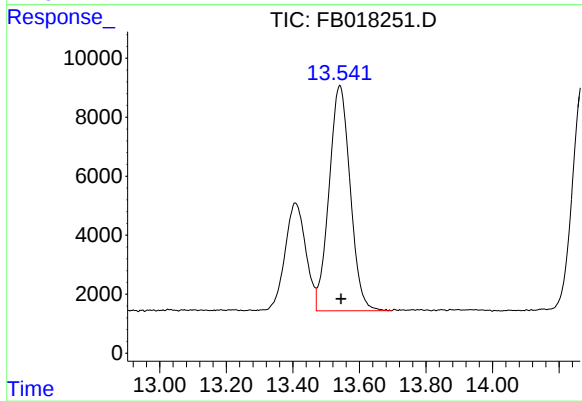


#8 m-Xylene

R.T.: 13.542 min
Delta R.T.: -0.003 min
Response: 336663
Conc: 20.23 ng/ml

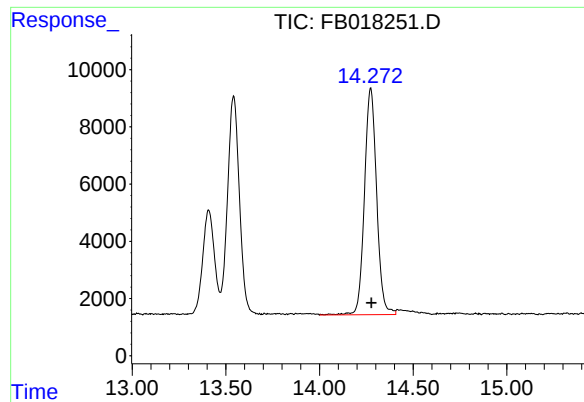

#9 O-Xylene

R.T.: 14.273 min
Delta R.T.: -0.003 min
Response: 358406
Conc: 20.10 ng/ml

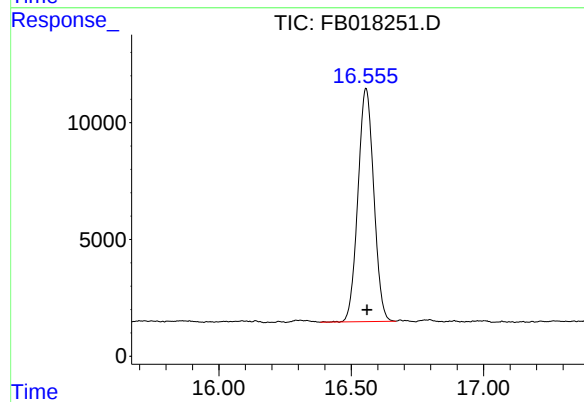

#10 1,2,4-Trimethylbenzene

R.T.: 16.556 min
Delta R.T.: -0.003 min
Response: 414003
Conc: 20.35 ng/ml