

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101619\
 Data File : FB022725.D
 Signal(s) : FID2B.CH
 Acq On : 16 Oct 2019 13:00
 Operator : DD/AJ
 Sample : BSF1016S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1016S1

Integration File: Calibration.e
 Quant Time: Oct 17 02:08:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
 Quant Title :
 QLast Update : Wed Oct 16 15:04:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	509230	20.124 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	1040194	30.608 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	1088743	29.921 ng/ml
3) t n-Heptane	7.759	362123	9.925 ng/ml
4) t Benzene	7.894	439049	9.944 ng/ml
6) t Toluene	10.632	1285158	29.818 ng/ml
7) t Ethylbenzene	13.072	404928	9.970 ng/ml
8) t m-Xylene	13.206	760194	19.758 ng/ml
9) t O-Xylene	13.934	715728	19.651 ng/ml
10) t 1,2,4-Trimethylbenzene	16.212	567056	19.900 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101619\
Data File : FB022725.D
Signal(s) : FID2B.CH
Acq On : 16 Oct 2019 13:00
Operator : DD/AJ
Sample : BSF1016S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1016S1

Integration File: Calibration.e
Quant Time: Oct 17 02:08:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

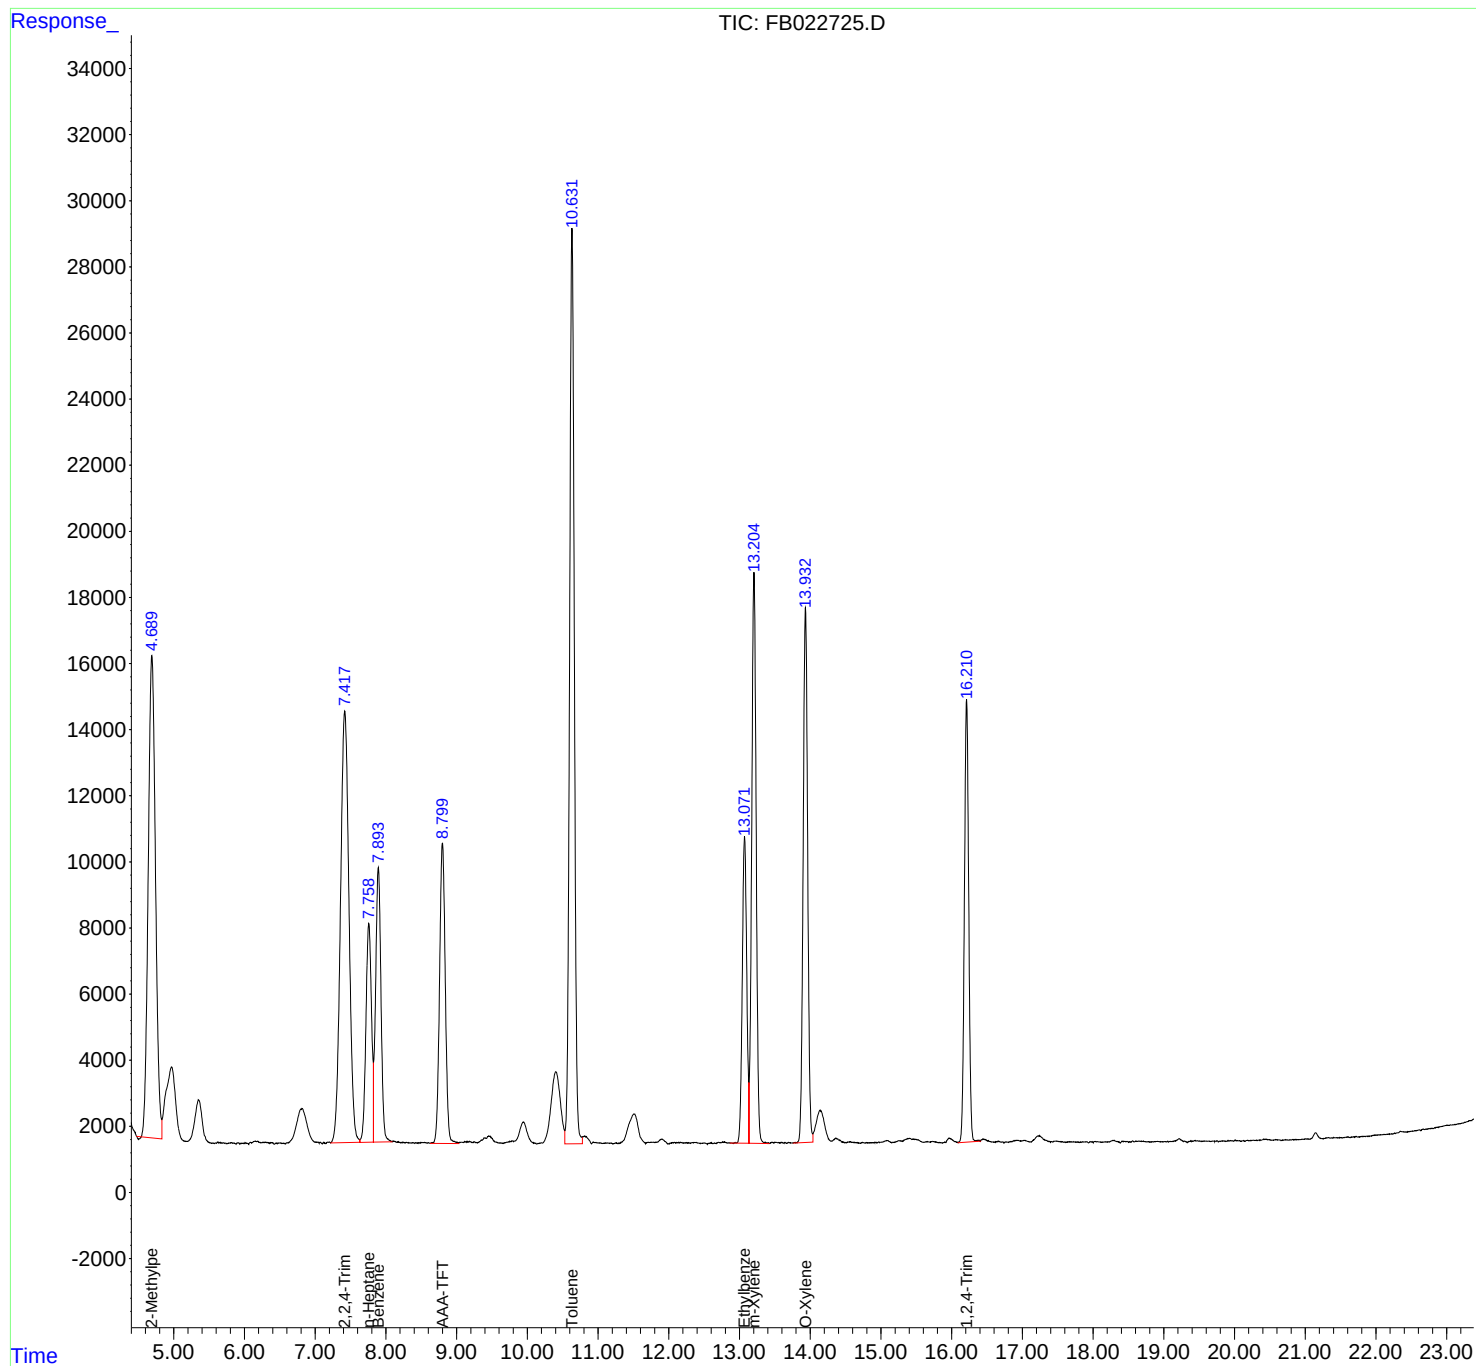


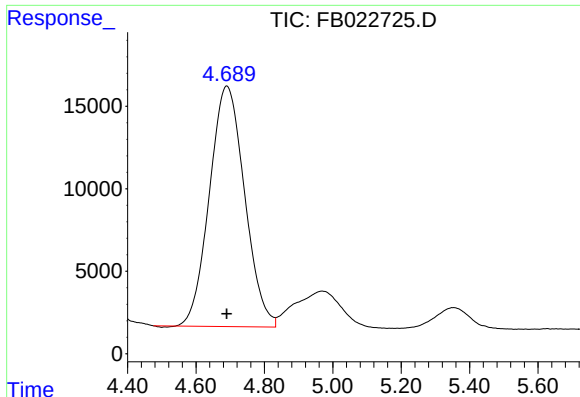

#1 2-Methylpentane


R.T.: 4.691 min
Delta R.T.: 0.000 min
Response: 1040194
Conc: 30.61 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1016S1

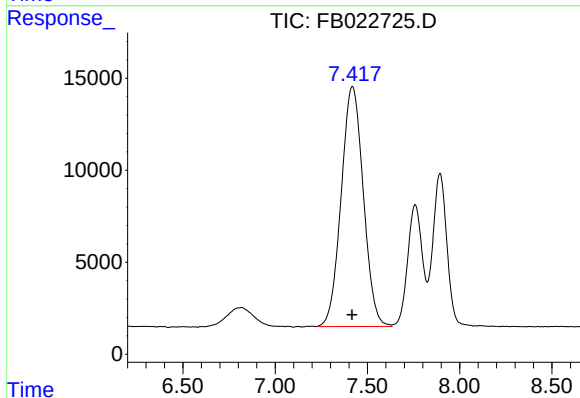


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.001 min
Response: 1088743
Conc: 29.92 ng/ml

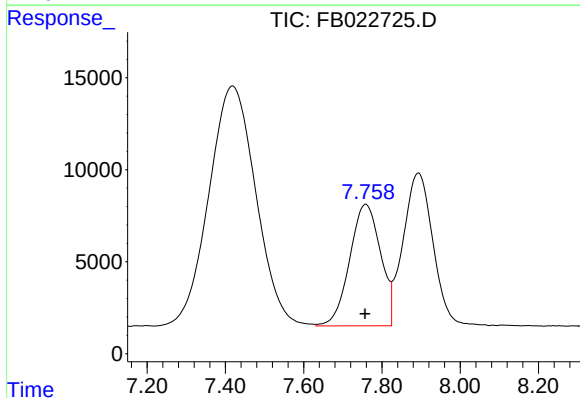


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.002 min
Response: 362123
Conc: 9.92 ng/ml

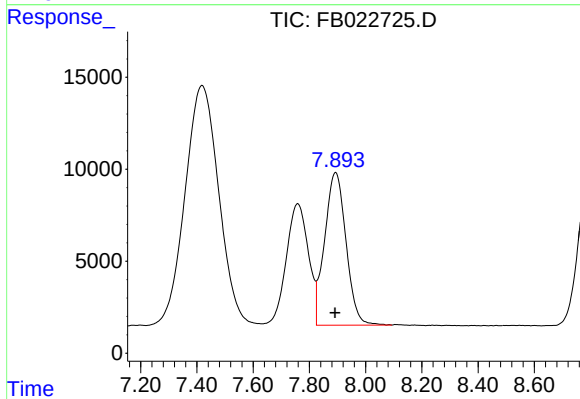

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.002 min
Response: 439049
Conc: 9.94 ng/ml

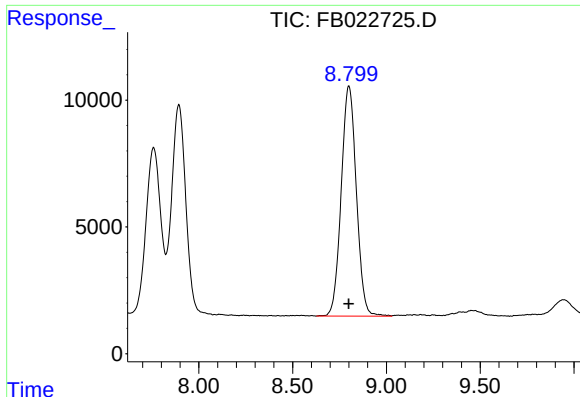

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.002 min
Response: 509230
Conc: 20.12 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1016S1

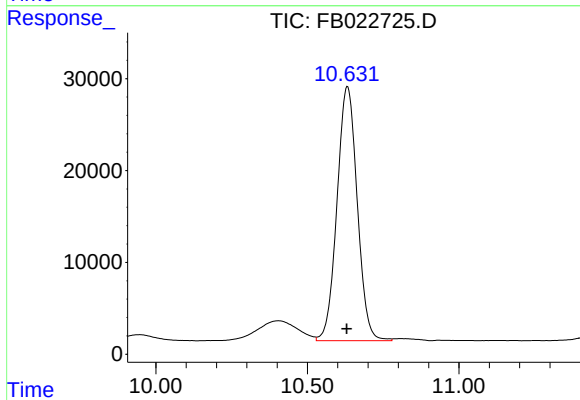


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.003 min
Response: 1285158
Conc: 29.82 ng/ml

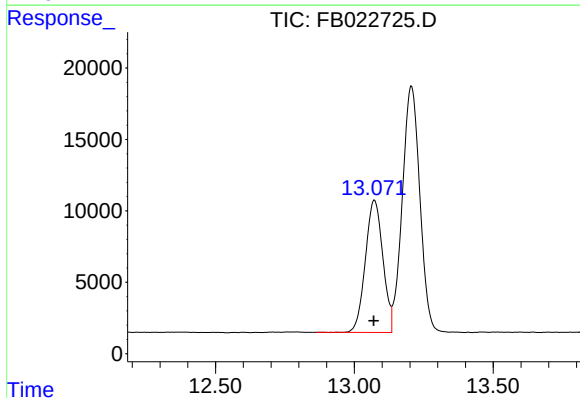


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.003 min
Response: 404928
Conc: 9.97 ng/ml

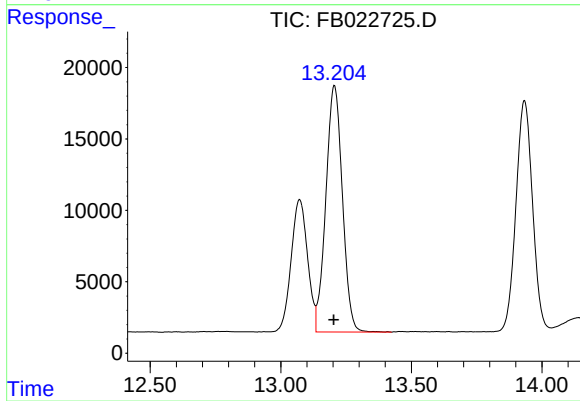

#8 m-Xylene


R.T.: 13.206 min
Delta R.T.: 0.003 min
Response: 760194
Conc: 19.76 ng/ml

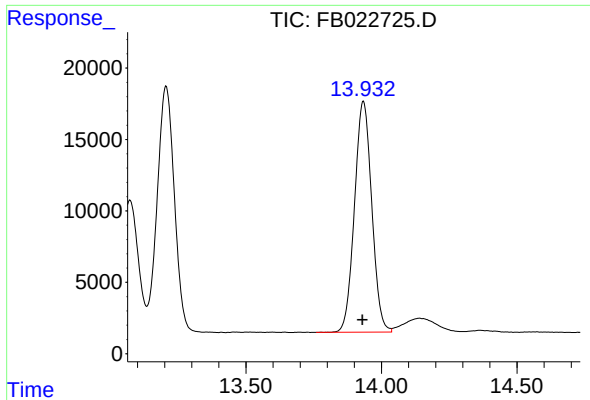

#9 O-Xylene

R.T.: 13.934 min
Delta R.T.: 0.003 min
Response: 715728
Conc: 19.65 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1016S1

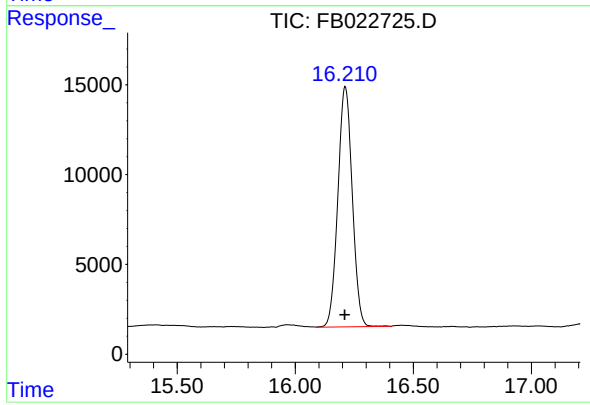

#10 1,2,4-Trimethylbenzene

R.T.: 16.212 min
Delta R.T.: 0.002 min
Response: 567056
Conc: 19.90 ng/ml