

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101619\
 Data File : FB022734.D
 Signal(s) : FID2B.CH
 Acq On : 16 Oct 2019 20:47
 Operator : DD/AJ
 Sample : K5153-02
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 17 02:09:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
 Quant Title :
 QLast Update : Wed Oct 16 15:04:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.803	546031	21.579 ng/ml
Target Compounds			
6) t Toluene	10.636	177289	4.113 ng/ml
7) t Ethylbenzene	13.076	23986	0.591 ng/ml
8) t m-Xylene	13.207	112013	2.911 ng/ml
9) t O-Xylene	13.937	43990	1.208 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101619\
Data File : FB022734.D
Signal(s) : FID2B.CH
Acq On : 16 Oct 2019 20:47
Operator : DD/AJ
Sample : K5153-02
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 17 02:09:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

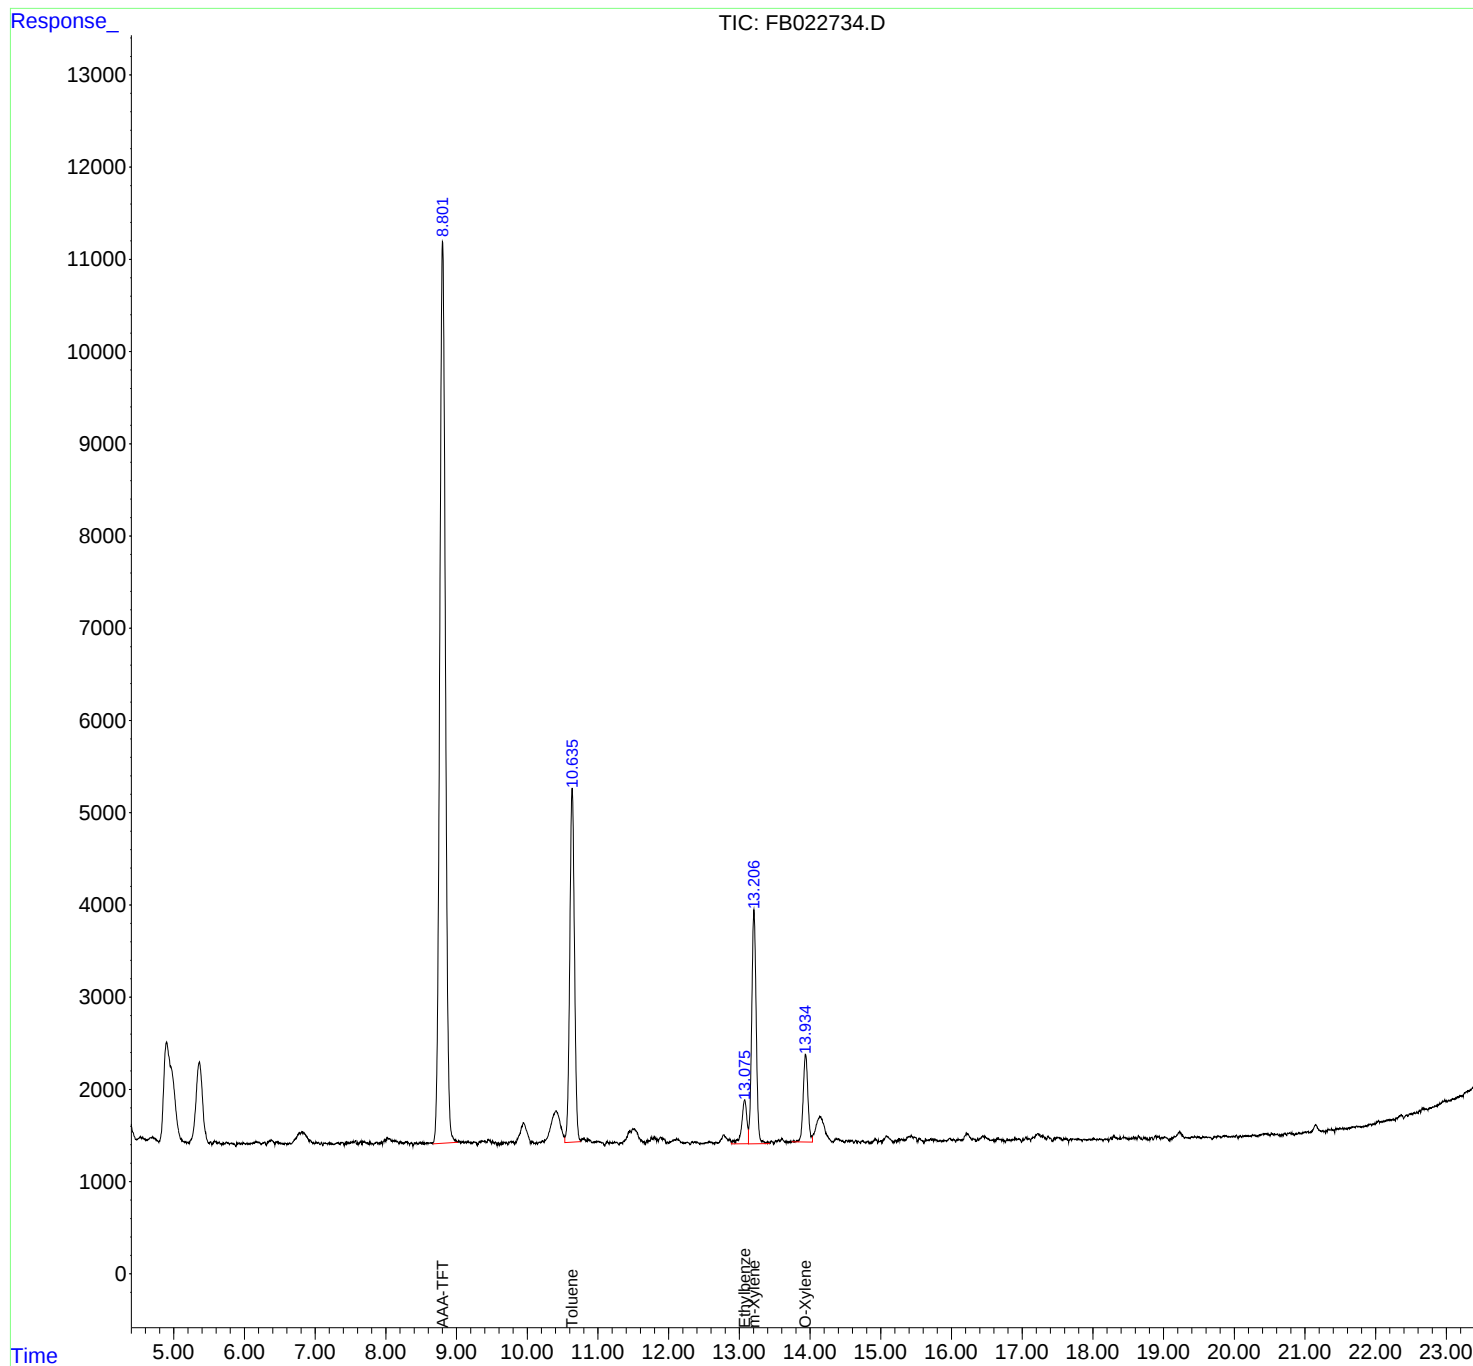


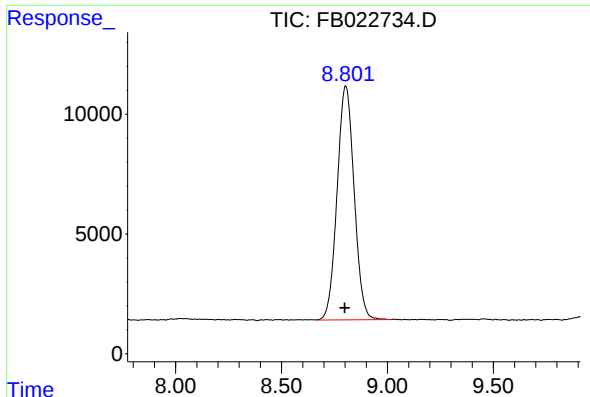

#5 AAA-TFT


R.T.: 8.803 min
Delta R.T.: 0.005 min
Response: 546031
Conc: 21.58 ng/ml

Instrument :
FID_B
ClientSampleId :

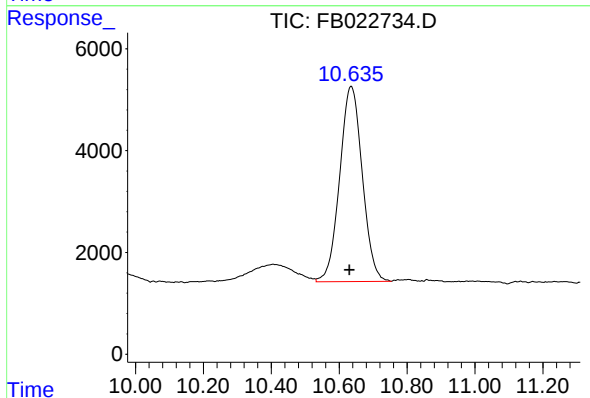


#6 Toluene

R.T.: 10.636 min
Delta R.T.: 0.006 min
Response: 177289
Conc: 4.11 ng/ml

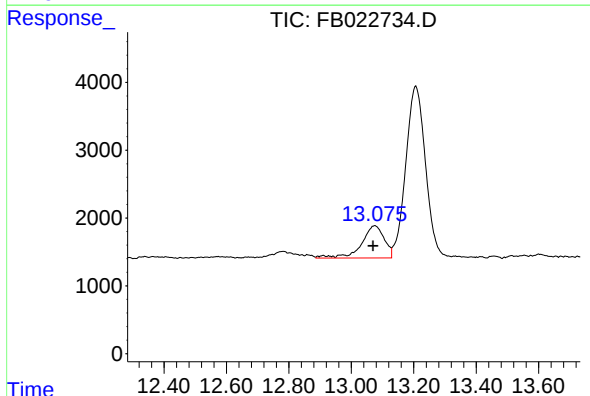


#7 Ethylbenzene

R.T.: 13.076 min
Delta R.T.: 0.006 min
Response: 23986
Conc: 0.59 ng/ml

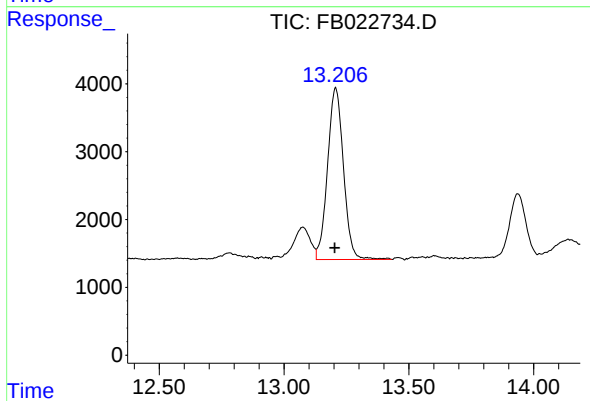

#8 m-Xylene

R.T.: 13.207 min
Delta R.T.: 0.004 min
Response: 112013
Conc: 2.91 ng/ml

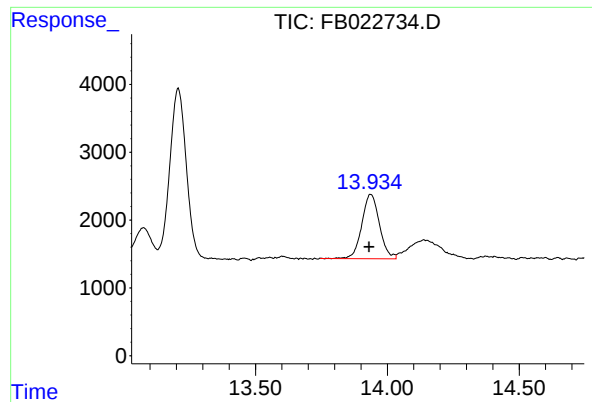

#9 O-Xylene

R.T.: 13.937 min
Delta R.T.: 0.007 min
Response: 43990
Conc: 1.21 ng/ml

Instrument :
FID_B
ClientSampleId :