

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101619\
 Data File : FB022735.D
 Signal(s) : FID2B.CH
 Acq On : 16 Oct 2019 21:17
 Operator : DD/AJ
 Sample : K5153-02MS
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 TR-04-101619-1MS

Integration File: Calibration.e
 Quant Time: Oct 17 02:09:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
 Quant Title :
 QLast Update : Wed Oct 16 15:04:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.803	468299	18.507 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.694	707173	20.809 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	705575	19.391 ng/ml
3) t n-Heptane	7.762	229271	6.284 ng/ml
4) t Benzene	7.896	372743	8.442 ng/ml
6) t Toluene	10.635	1362217	31.606 ng/ml
7) t Ethylbenzene	13.075	322024	7.929 ng/ml
8) t m-Xylene	13.208	709625	18.443 ng/ml
9) t O-Xylene	13.936	594524	16.323 ng/ml
10) t 1,2,4-Trimethylbenzene	16.216	372885	13.086 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101619\
Data File : FB022735.D
Signal(s) : FID2B.CH
Acq On : 16 Oct 2019 21:17
Operator : DD/AJ
Sample : K5153-02MS
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TR-04-101619-1MS

Integration File: Calibration.e
Quant Time: Oct 17 02:09:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

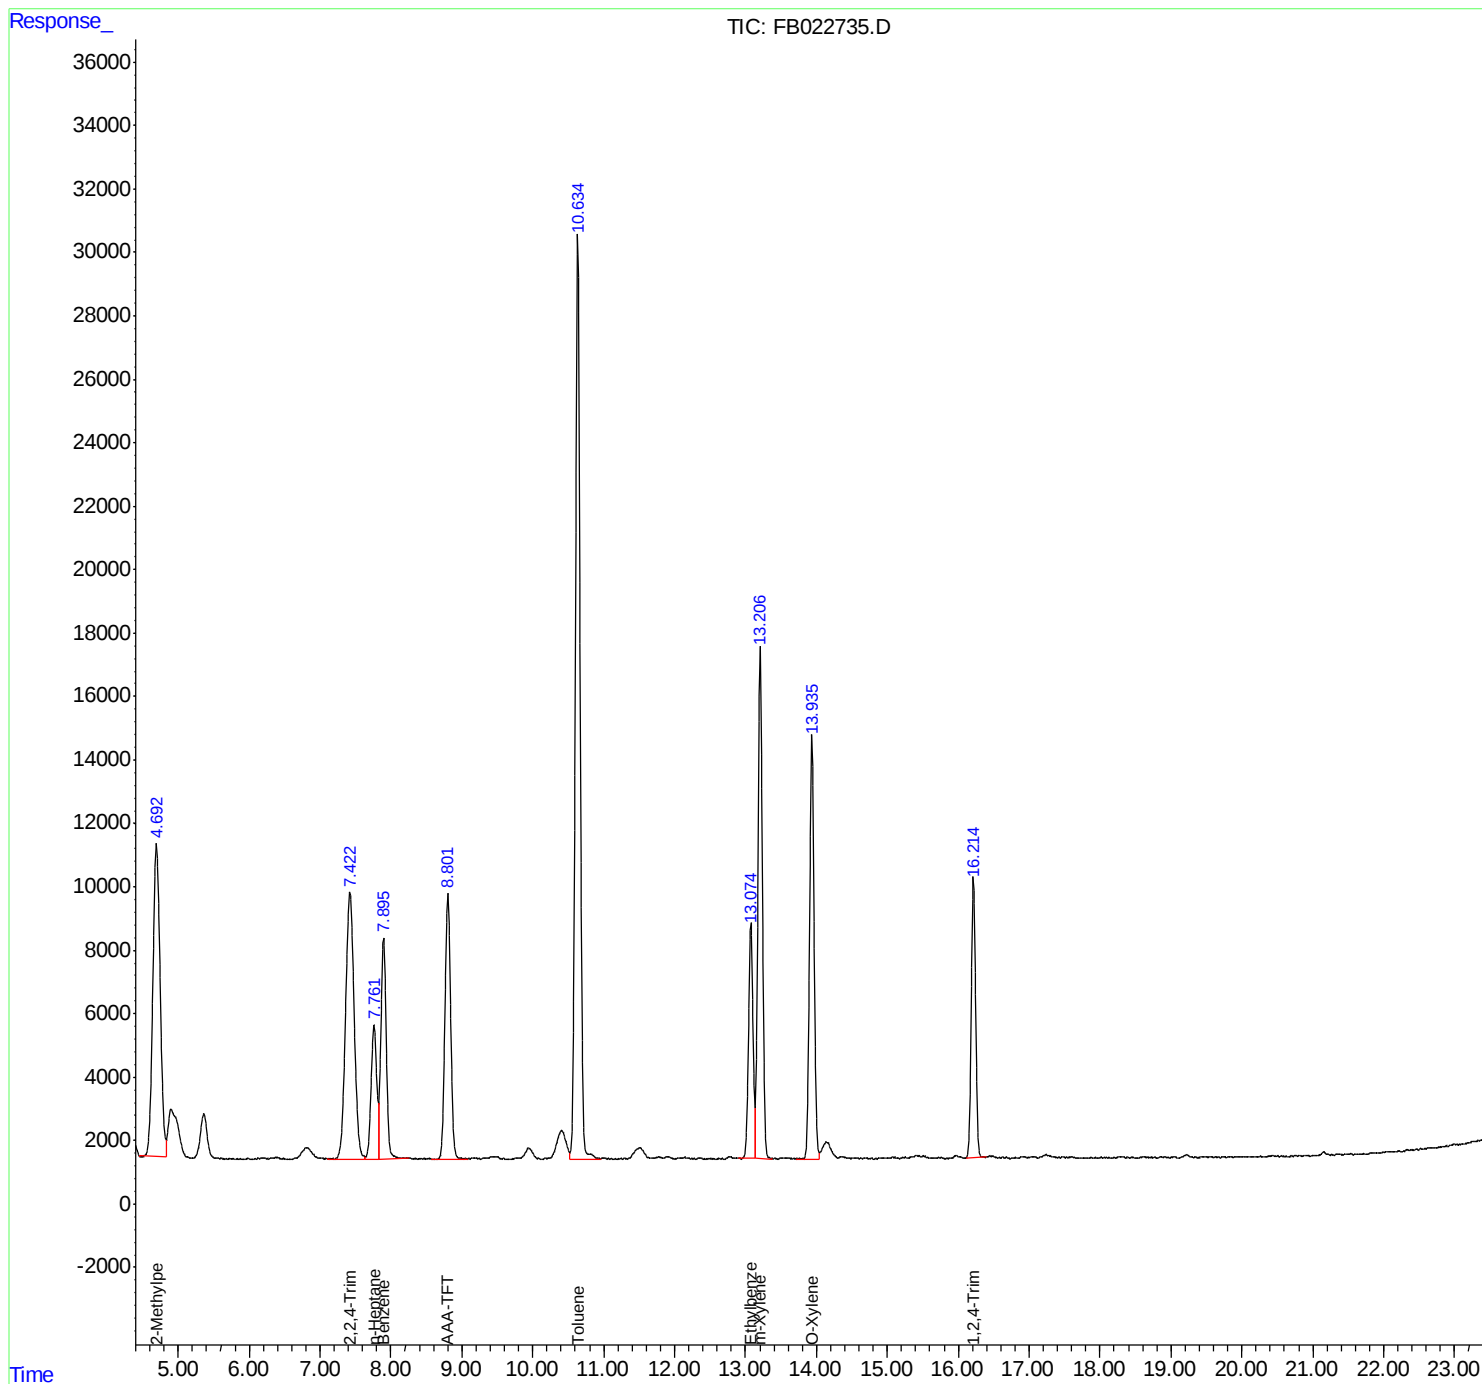


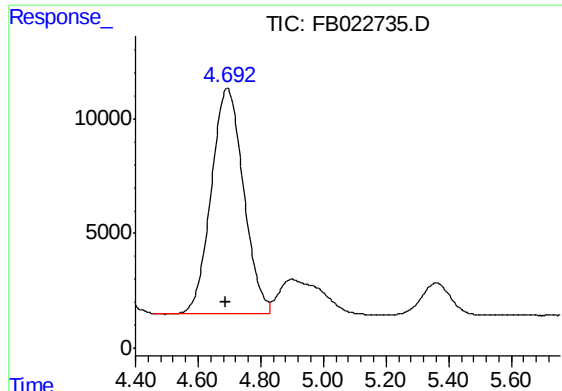

#1 2-Methylpentane


R.T.: 4.694 min
Delta R.T.: 0.004 min
Response: 707173
Conc: 20.81 ng/ml

Instrument :
FID_B
ClientSampleId :
TR-04-101619-1MS

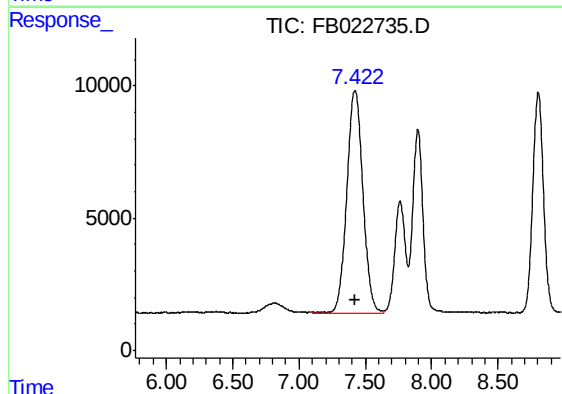


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: 0.004 min
Response: 705575
Conc: 19.39 ng/ml

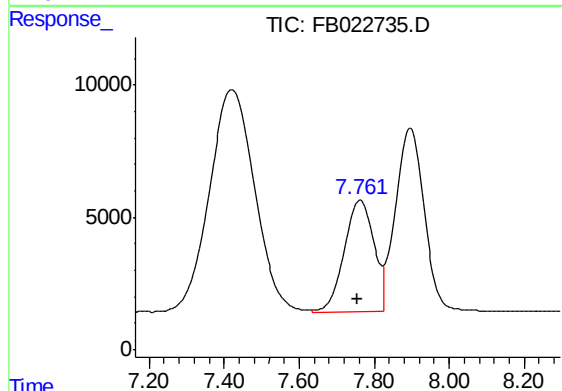


#3 n-Heptane

R.T.: 7.762 min
Delta R.T.: 0.005 min
Response: 229271
Conc: 6.28 ng/ml

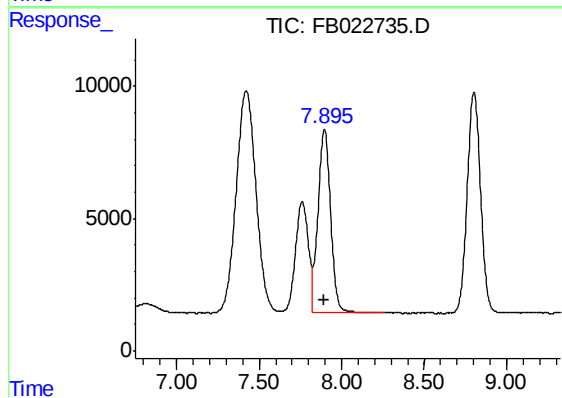

#4 Benzene


R.T.: 7.896 min
Delta R.T.: 0.004 min
Response: 372743
Conc: 8.44 ng/ml

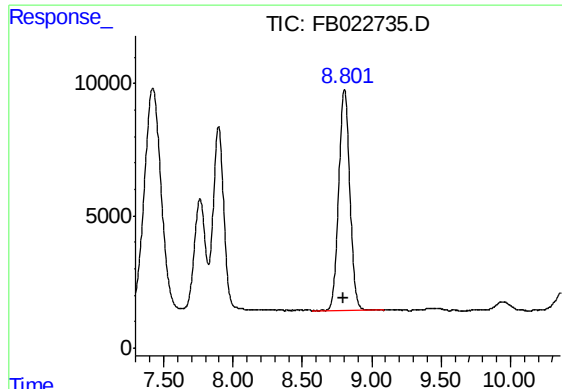

#5 AAA-TFT


R.T.: 8.803 min
Delta R.T.: 0.005 min
Response: 468299
Conc: 18.51 ng/ml

Instrument :
FID_B
ClientSampleId :
TR-04-101619-1MS

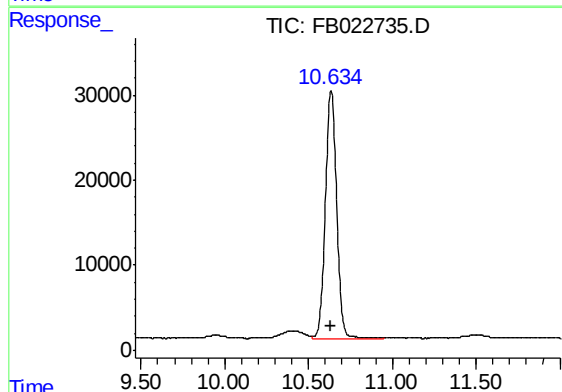


#6 Toluene

R.T.: 10.635 min
Delta R.T.: 0.005 min
Response: 1362217
Conc: 31.61 ng/ml

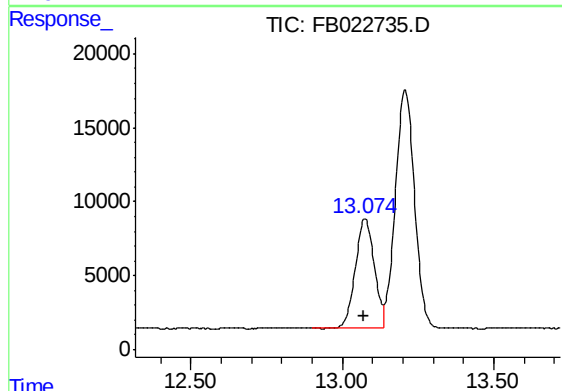


#7 Ethylbenzene

R.T.: 13.075 min
Delta R.T.: 0.006 min
Response: 322024
Conc: 7.93 ng/ml

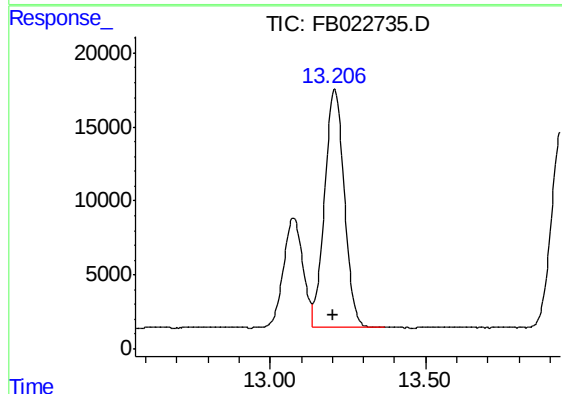

#8 m-Xylene


R.T.: 13.208 min
Delta R.T.: 0.005 min
Response: 709625
Conc: 18.44 ng/ml

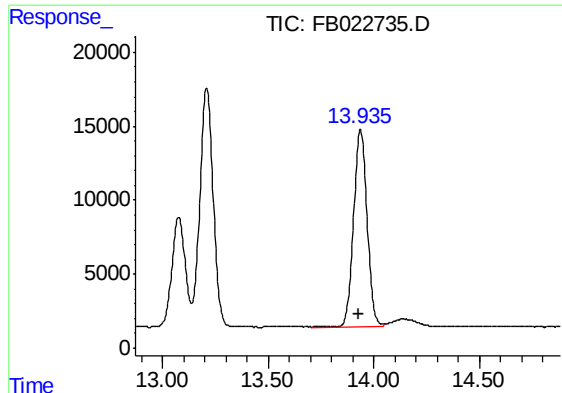

#9 O-Xylene

R.T.: 13.936 min
Delta R.T.: 0.006 min
Response: 594524
Conc: 16.32 ng/ml

Instrument :
FID_B
ClientSampleId :
TR-04-101619-1MS

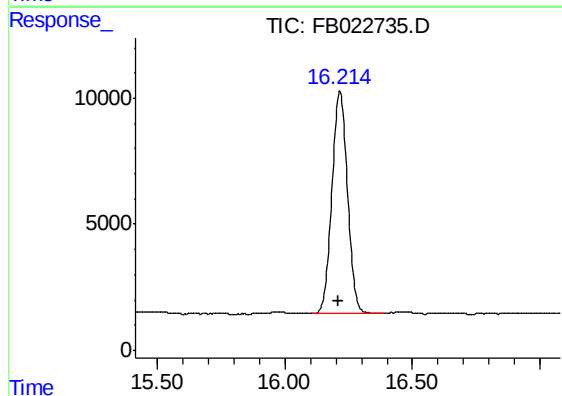

#10 1,2,4-Trimethylbenzene

R.T.: 16.216 min
Delta R.T.: 0.006 min
Response: 372885
Conc: 13.09 ng/ml