

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101619\
 Data File : FB022736.D
 Signal(s) : FID2B.CH
 Acq On : 16 Oct 2019 21:47
 Operator : DD/AJ
 Sample : K5153-02MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 TR-04-101619-1MSD

Integration File: Calibration.e
 Quant Time: Oct 17 02:10:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
 Quant Title :
 QLast Update : Wed Oct 16 15:04:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.803	508506	20.096 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.694	706551	20.790 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	736880	20.251 ng/ml
3) t n-Heptane	7.762	239420	6.562 ng/ml
4) t Benzene	7.896	371545	8.415 ng/ml
6) t Toluene	10.635	1234322	28.638 ng/ml
7) t Ethylbenzene	13.076	310128	7.636 ng/ml
8) t m-Xylene	13.208	664914	17.281 ng/ml
9) t O-Xylene	13.937	560066	15.377 ng/ml
10) t 1,2,4-Trimethylbenzene	16.216	372408	13.069 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB101619\
Data File : FB022736.D
Signal(s) : FID2B.CH
Acq On : 16 Oct 2019 21:47
Operator : DD/AJ
Sample : K5153-02MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TR-04-101619-1MSD

Integration File: Calibration.e
Quant Time: Oct 17 02:10:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

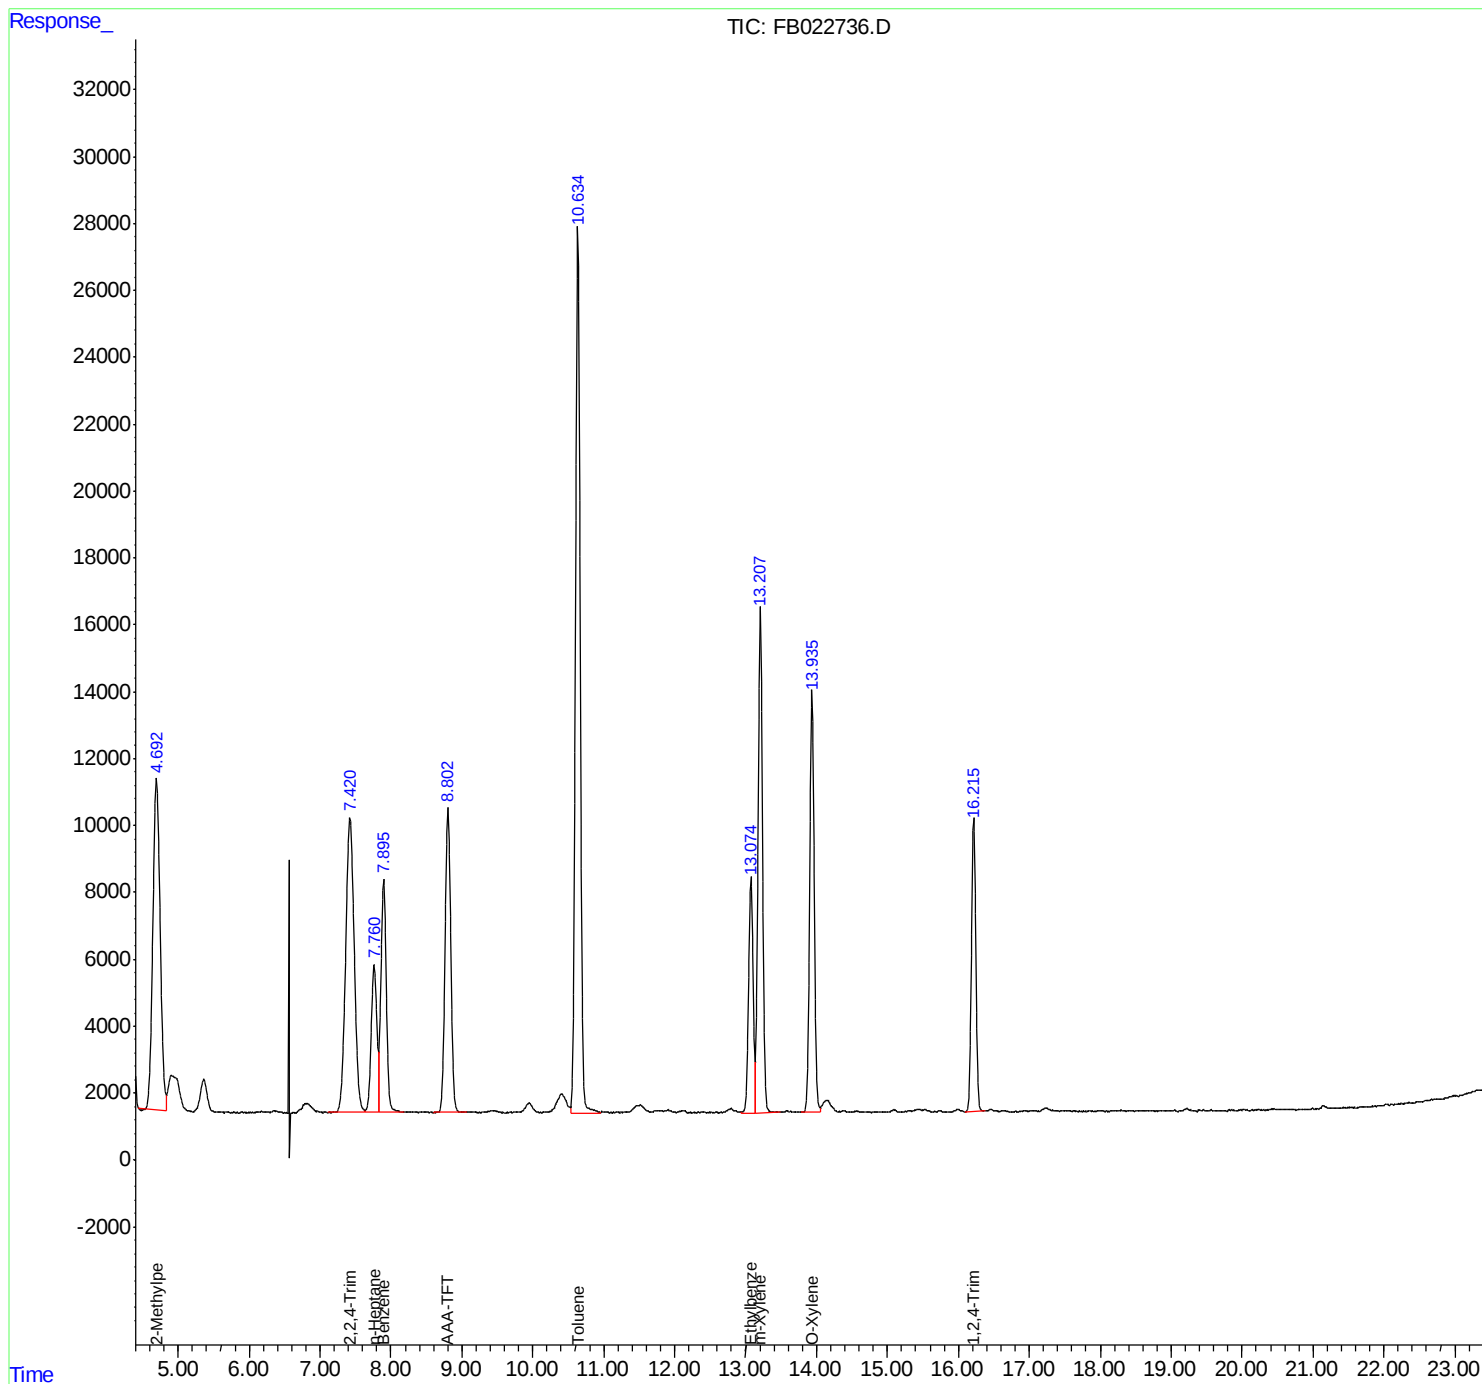


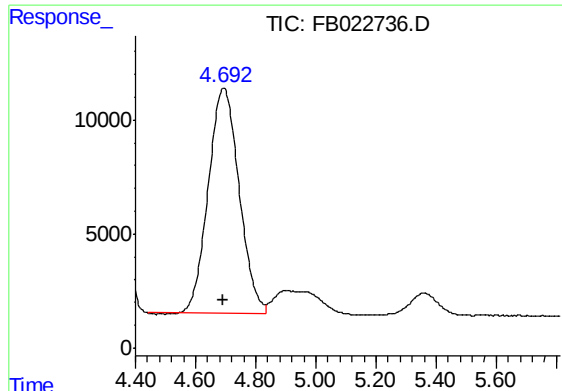

#1 2-Methylpentane


R.T.: 4.694 min
Delta R.T.: 0.004 min
Response: 706551
Conc: 20.79 ng/ml

Instrument :
FID_B
ClientSampleId :
TR-04-101619-1MSD

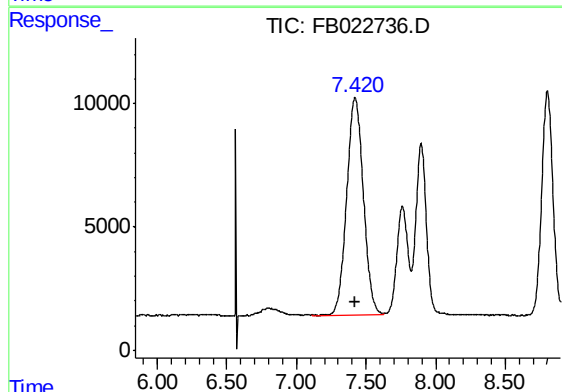


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: 0.005 min
Response: 736880
Conc: 20.25 ng/ml

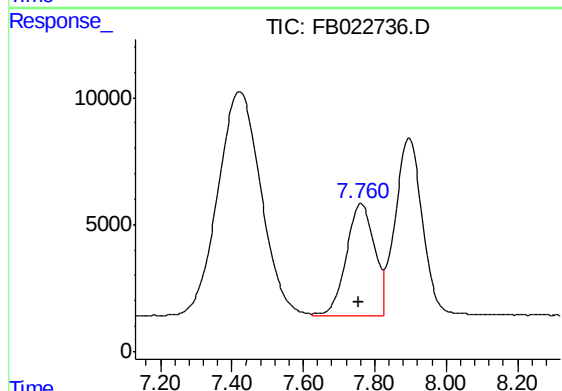


#3 n-Heptane

R.T.: 7.762 min
Delta R.T.: 0.005 min
Response: 239420
Conc: 6.56 ng/ml

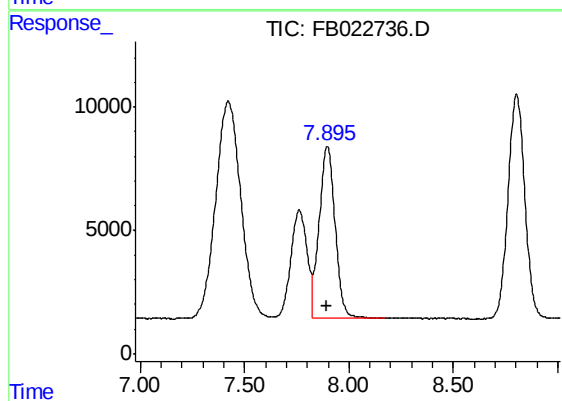

#4 Benzene


R.T.: 7.896 min
Delta R.T.: 0.005 min
Response: 371545
Conc: 8.42 ng/ml

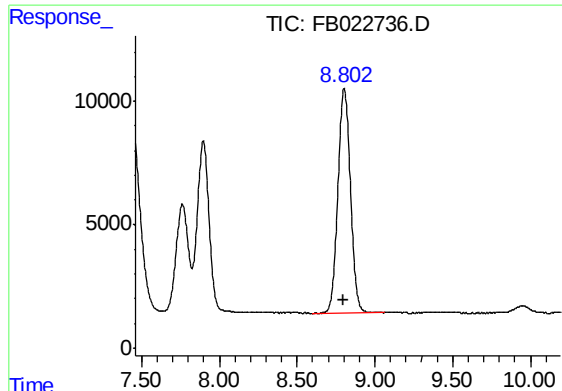

#5 AAA-TFT


R.T.: 8.803 min
Delta R.T.: 0.005 min
Response: 508506
Conc: 20.10 ng/ml

Instrument :
FID_B
ClientSampleId :
TR-04-101619-1MSD

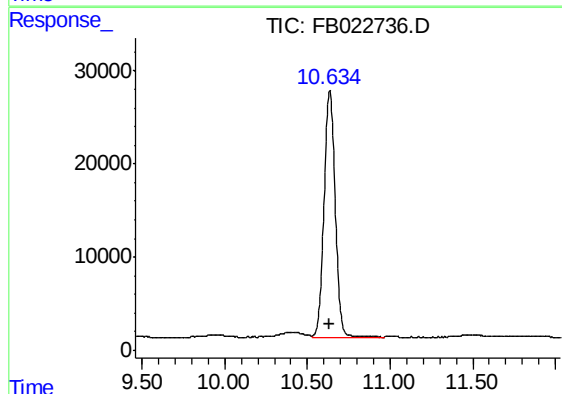


#6 Toluene

R.T.: 10.635 min
Delta R.T.: 0.006 min
Response: 1234322
Conc: 28.64 ng/ml

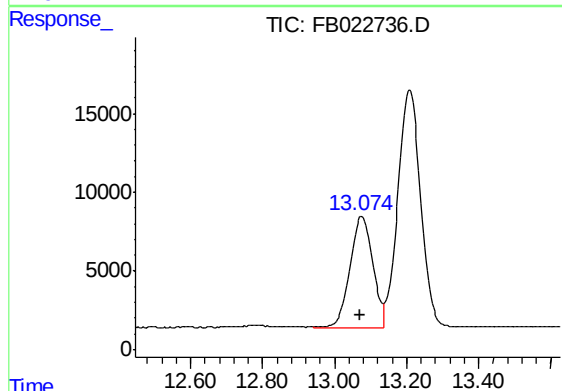


#7 Ethylbenzene

R.T.: 13.076 min
Delta R.T.: 0.006 min
Response: 310128
Conc: 7.64 ng/ml

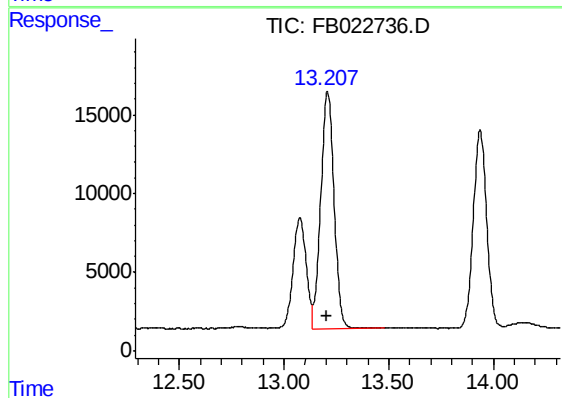

#8 m-Xylene


R.T.: 13.208 min
Delta R.T.: 0.005 min
Response: 664914
Conc: 17.28 ng/ml

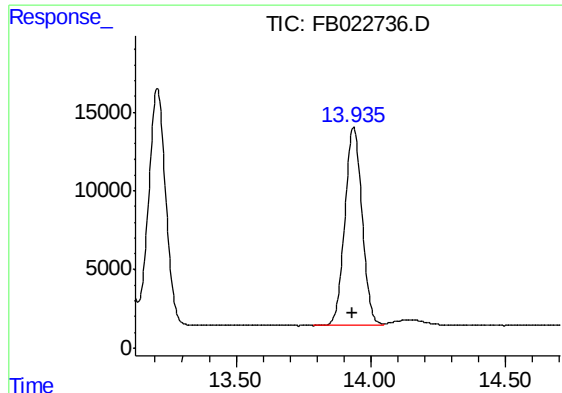

#9 O-Xylene

R.T.: 13.937 min
Delta R.T.: 0.006 min
Response: 560066
Conc: 15.38 ng/ml

Instrument :
FID_B
ClientSampleId :
TR-04-101619-1MSD

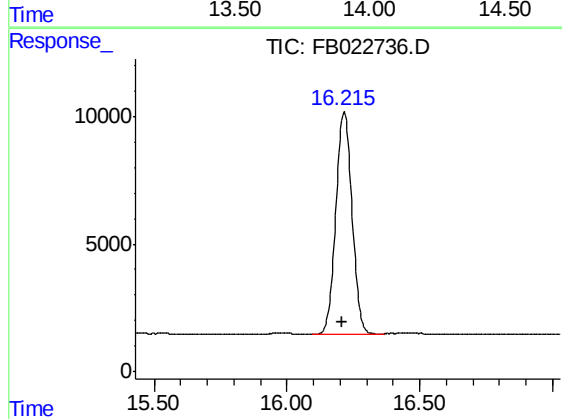

#10 1,2,4-Trimethylbenzene

R.T.: 16.216 min
Delta R.T.: 0.007 min
Response: 372408
Conc: 13.07 ng/ml